

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
 Data File : PO082624.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 21:31
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 08:35:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.962	1741987	633072	19.902	20.457
2)	SA Decachlor...	11.068	9.275	1269294	631617	20.099	21.937
Target Compounds							
8)	L2 AR-1221-1	5.206f	0.000	43740	0	46.381	N.D. #
9)	L2 AR-1221-2	5.322	4.312	21755	8237	33.562	28.372
10)	L2 AR-1221-3	0.000	4.406	0	24359	N.D.	26.325 #
11)	L3 AR-1232-1	0.000	4.406	0	24359	N.D.	30.857 #
28)	L6 AR-1254-3	7.849	0.000	21446	0	5.014	N.D. #
30)	L6 AR-1254-5	8.566	0.000	11390	0	3.542	N.D. #
45)	L9 AR-1268-5	10.724	0.000	15478	0	0.700	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082624.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 21:31
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:35:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

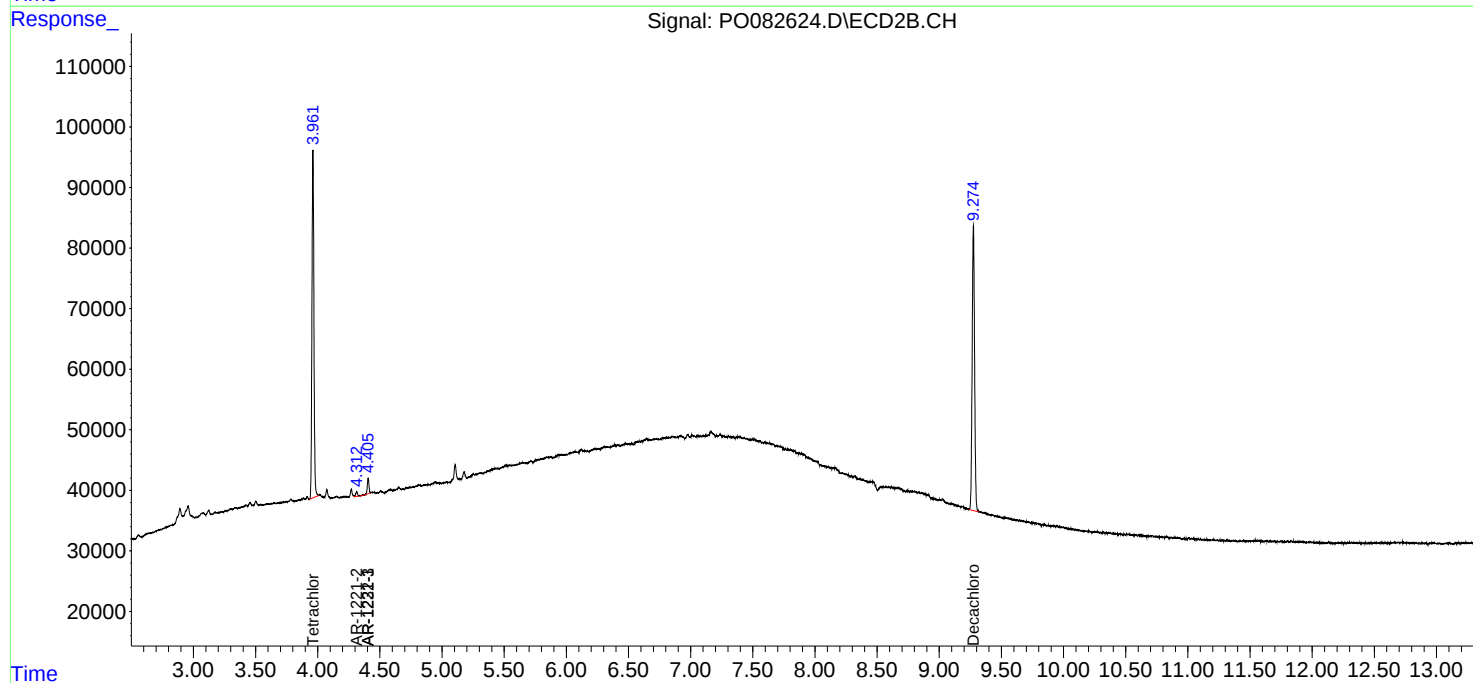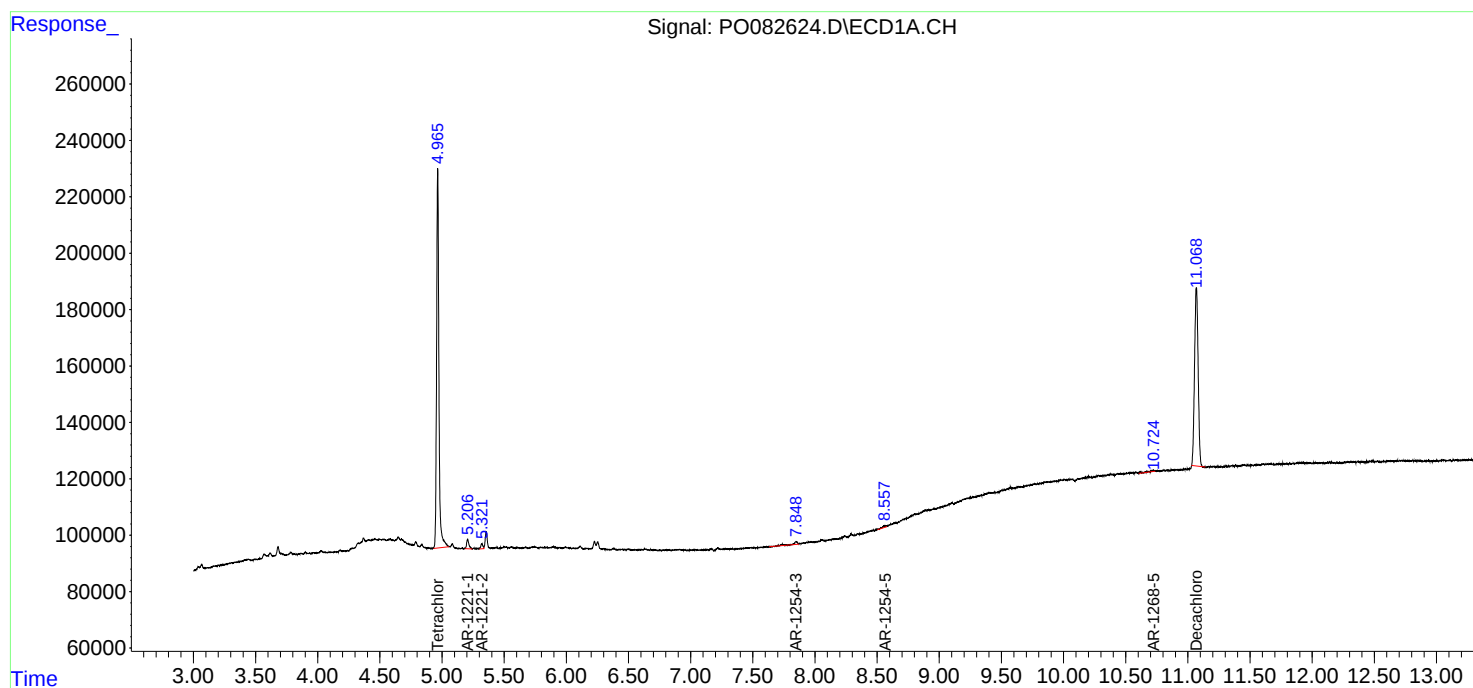


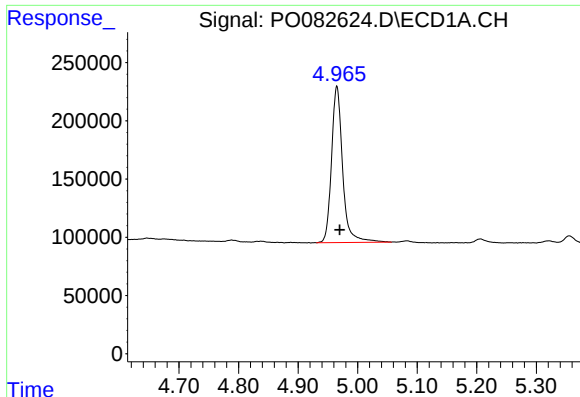

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: -0.005 min
Response: 1741987
Conc: 19.90 ng/ml

Instrument :
ECD_O
ClientSampleId :

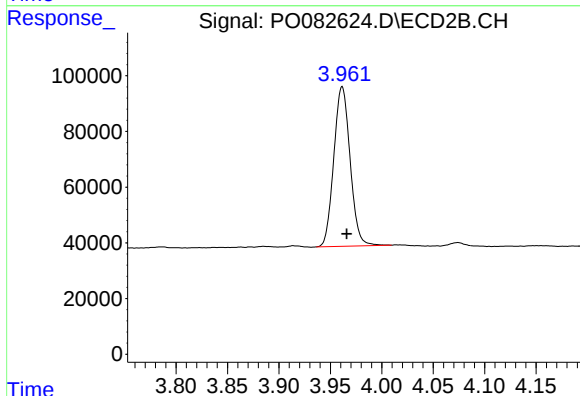


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.004 min
Response: 633072
Conc: 20.46 ng/ml

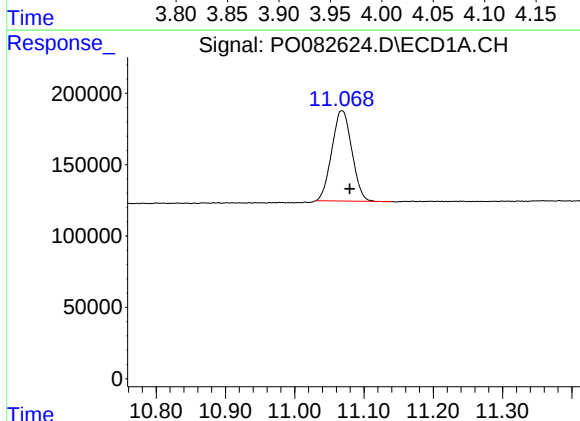


#2 Decachlorobiphenyl

R.T.: 11.068 min
Delta R.T.: -0.012 min
Response: 1269294
Conc: 20.10 ng/ml

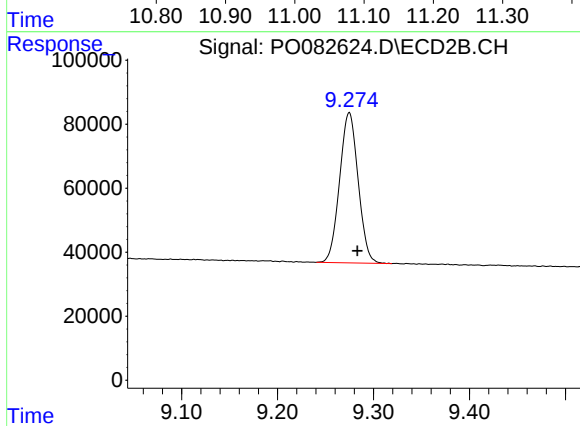

#2 Decachlorobiphenyl


R.T.: 9.275 min
Delta R.T.: -0.009 min
Response: 631617
Conc: 21.94 ng/ml

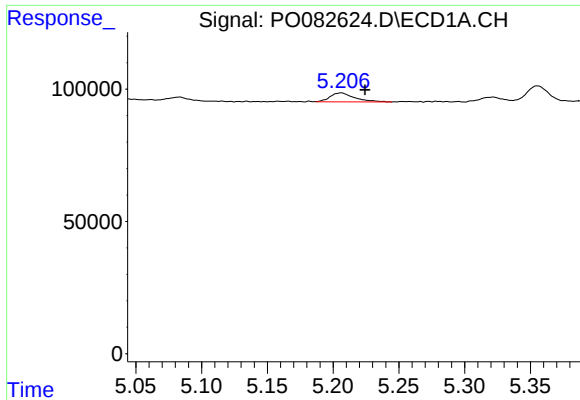

#8 AR-1221-1


R.T.: 5.206 min
Delta R.T.: -0.018 min
Response: 43740
Conc: 46.38 ng/ml

Instrument :
ECD_O
ClientSampleId :

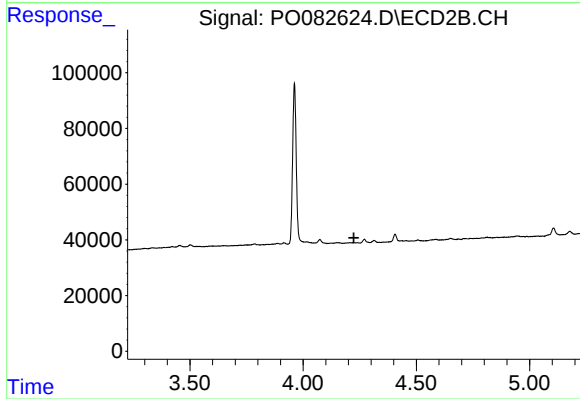


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.224 min
Response: 0
Conc: N.D.

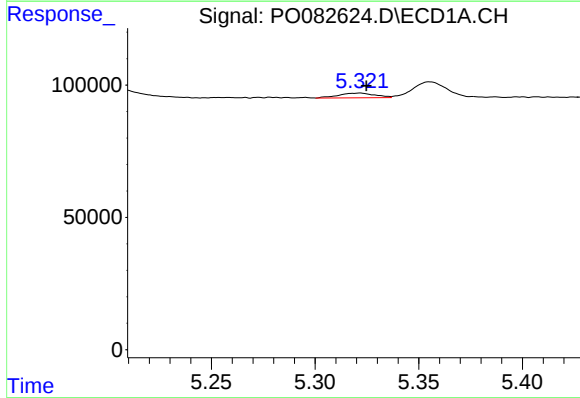


#9 AR-1221-2

R.T.: 5.322 min
Delta R.T.: -0.003 min
Response: 21755
Conc: 33.56 ng/ml

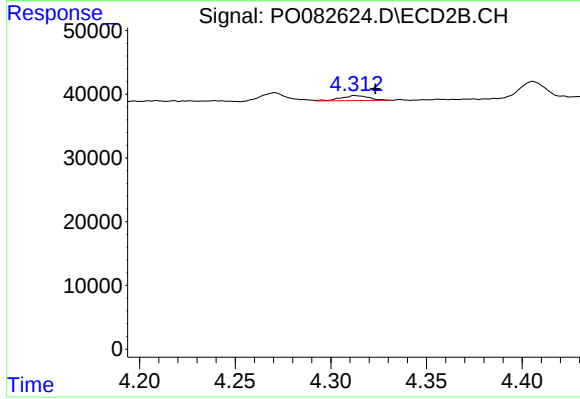

#9 AR-1221-2


R.T.: 4.312 min
Delta R.T.: -0.011 min
Response: 8237
Conc: 28.37 ng/ml

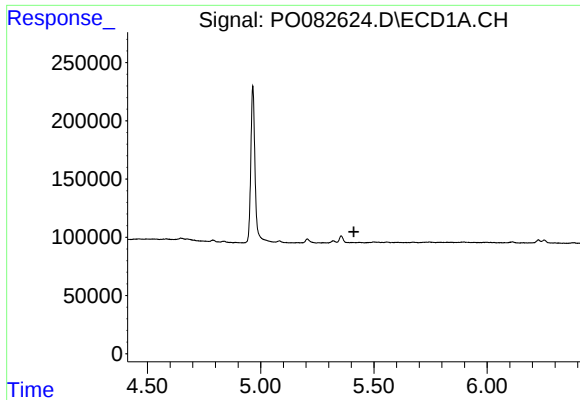

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

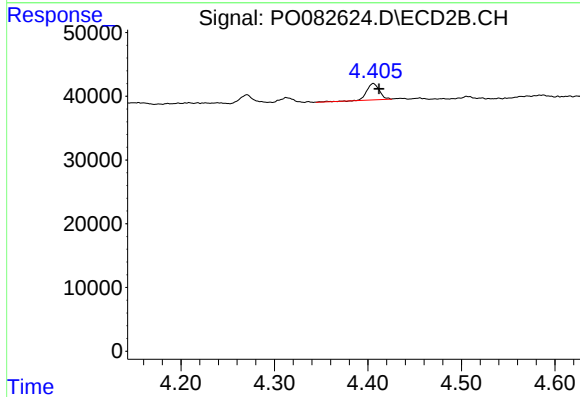


#10 AR-1221-3

R.T.: 4.406 min
Delta R.T.: -0.006 min
Response: 24359
Conc: 26.33 ng/ml

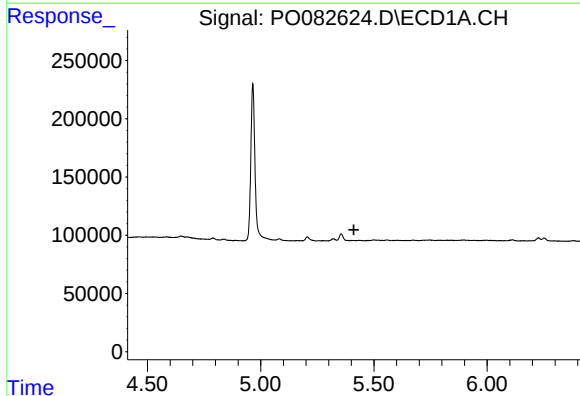


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

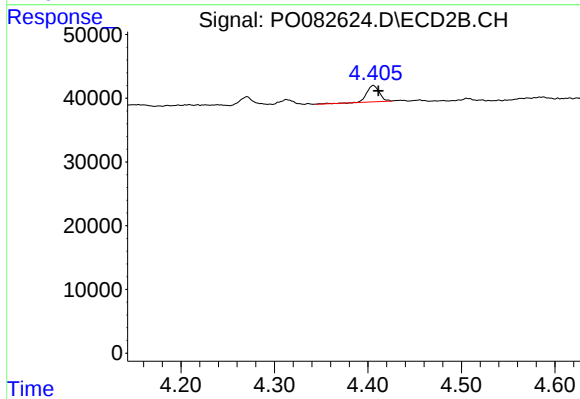

#11 AR-1232-1


R.T.: 4.406 min
Delta R.T.: -0.005 min
Response: 24359
Conc: 30.86 ng/ml

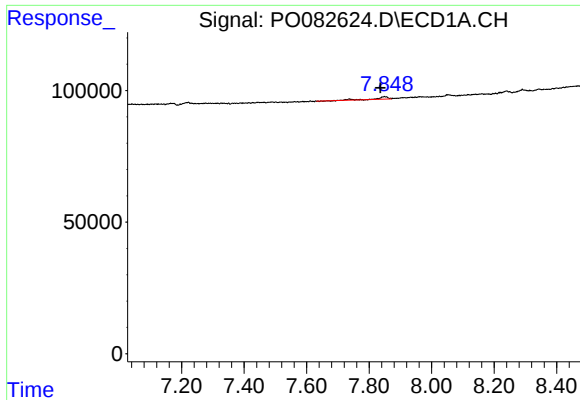

#28 AR-1254-3


R.T.: 7.849 min
Delta R.T.: 0.013 min
Response: 21446
Conc: 5.01 ng/ml

Instrument :
ECD_O
ClientSampleId :

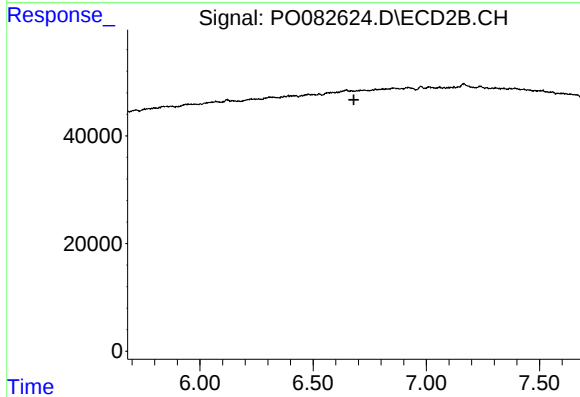


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

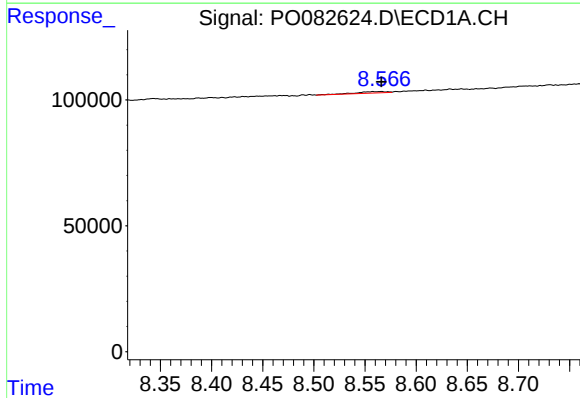


#30 AR-1254-5

R.T.: 8.566 min
Delta R.T.: 0.000 min
Response: 11390
Conc: 3.54 ng/ml

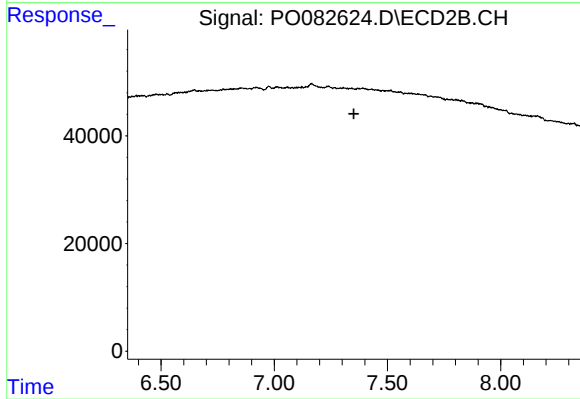

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.351 min
Response: 0
Conc: N.D.

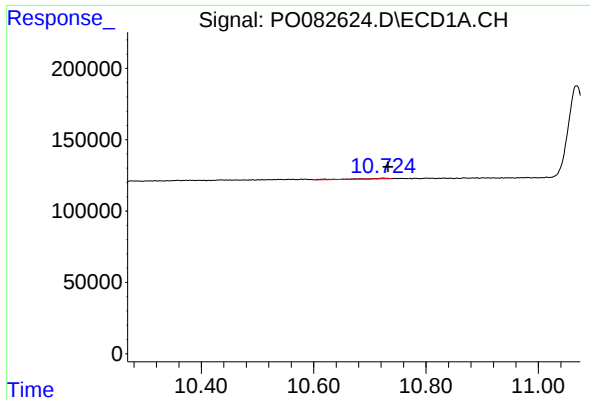

#45 AR-1268-5

R.T.: 10.724 min
Delta R.T.: -0.008 min
Response: 15478
Conc: 0.70 ng/ml

Instrument :
ECD_O
ClientSampleId :

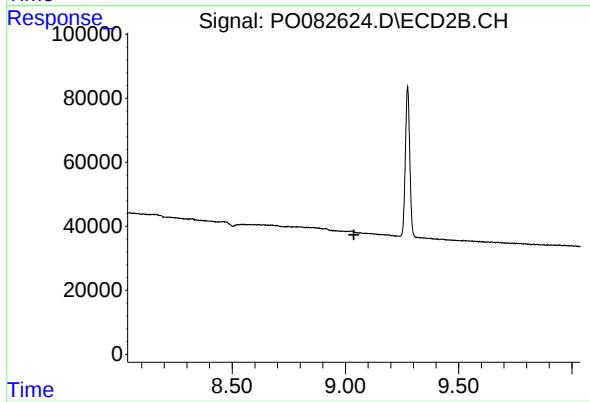

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.038 min
Response: 0
Conc: N.D.