

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
 Data File : PO082625.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2021 21:48
 Operator : AJ\MA
 Sample : M4540-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 08:36:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.962	1745425	650596	19.941	21.023
2)	SA Decachlor...	11.070	9.275	1174436	577304	18.597	20.051
Target Compounds							
4)	L1 AR-1016-2	0.000	5.281f	0	4935	N.D.	2.680 #
8)	L2 AR-1221-1	5.220	0.000	117950	0	125.072	N.D. #
9)	L2 AR-1221-2	5.320	4.314	21344	9305	32.928	32.053
10)	L2 AR-1221-3	5.422	4.409	63900	27654	30.976	29.886
11)	L3 AR-1232-1	5.422	4.409	63900	27654	36.887	35.030
17)	L4 AR-1242-2	0.000	5.281f	0	4935	N.D.	3.666 #
29)	L6 AR-1254-4	0.000	6.927	0	28525	N.D.	15.692 #
34)	L7 AR-1260-4	8.882	0.000	2799	0	0.840	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082625.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 21:48
Operator : AJ\MA
Sample : M4540-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:36:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

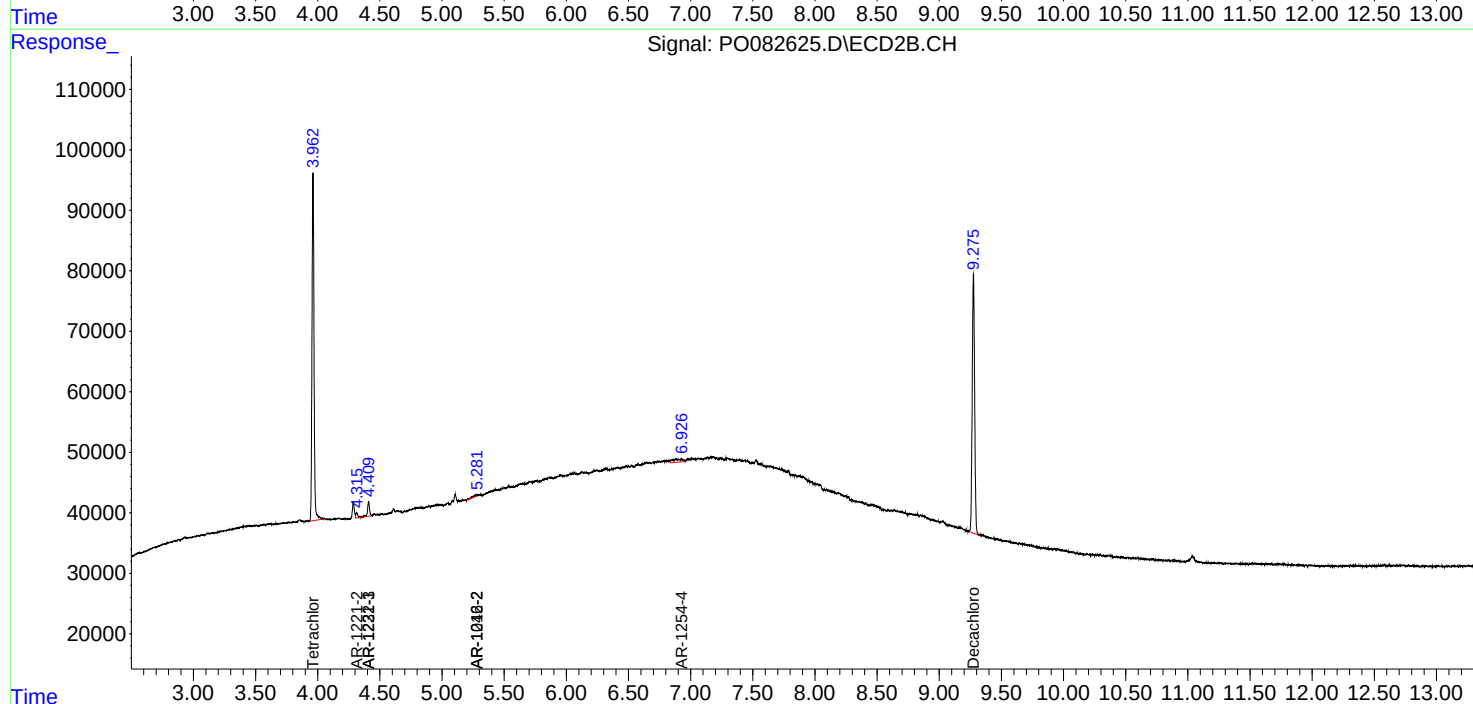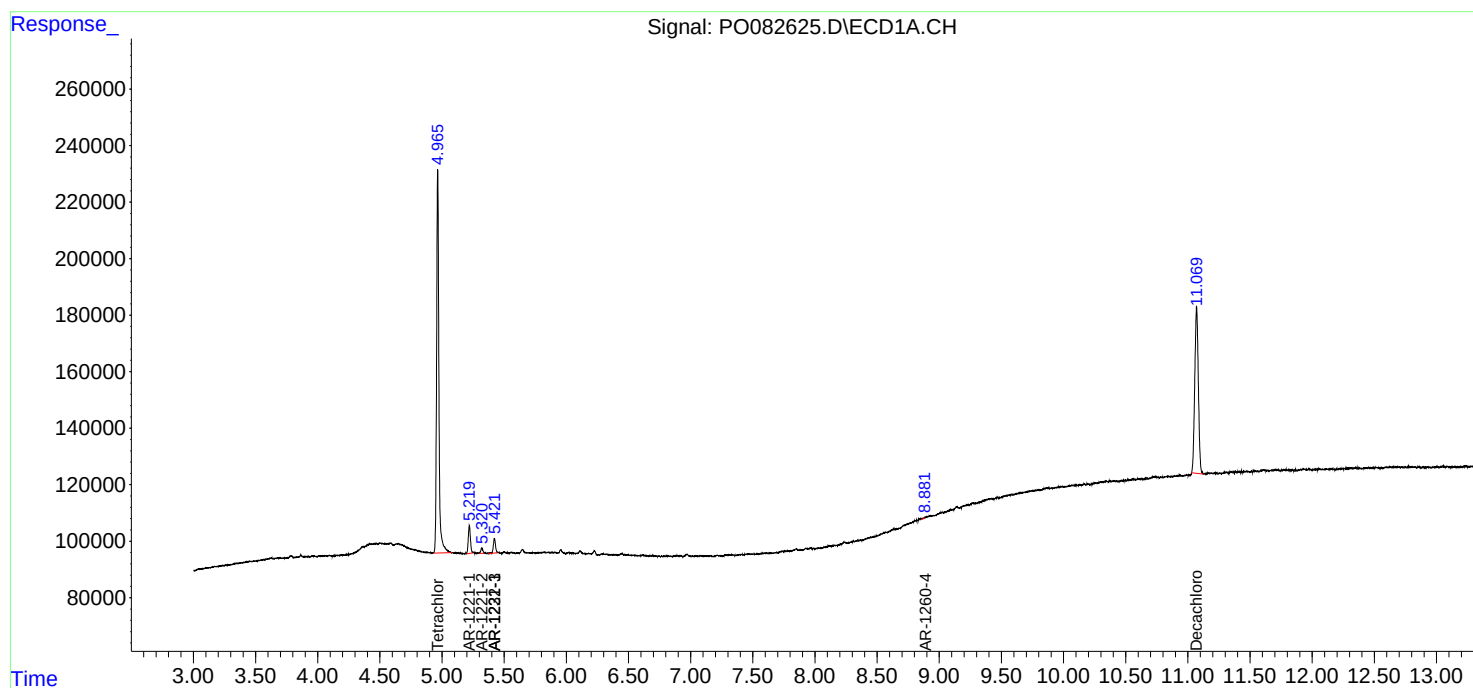


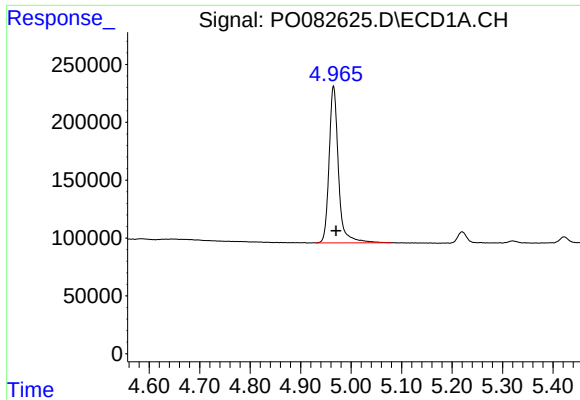

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: -0.005 min
Response: 1745425
Conc: 19.94 ng/ml

Instrument :
ECD_O
ClientSampleId :

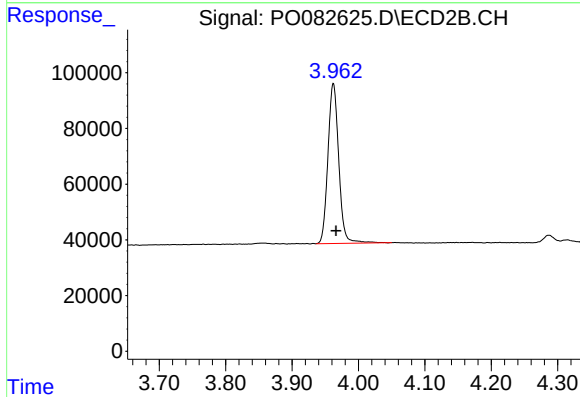


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.004 min
Response: 650596
Conc: 21.02 ng/ml

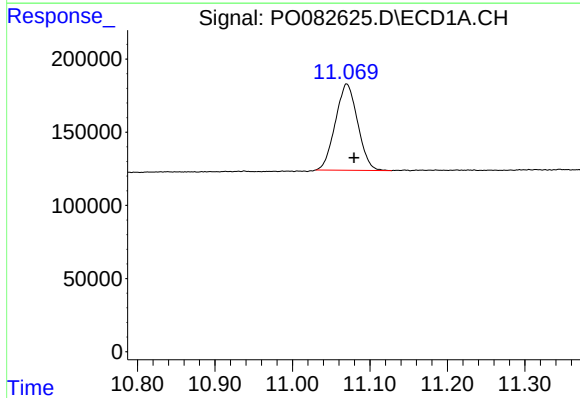


#2 Decachlorobiphenyl

R.T.: 11.070 min
Delta R.T.: -0.010 min
Response: 1174436
Conc: 18.60 ng/ml

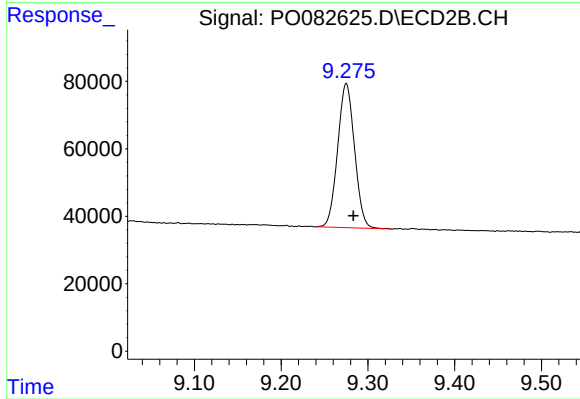

#2 Decachlorobiphenyl


R.T.: 9.275 min
Delta R.T.: -0.008 min
Response: 577304
Conc: 20.05 ng/ml

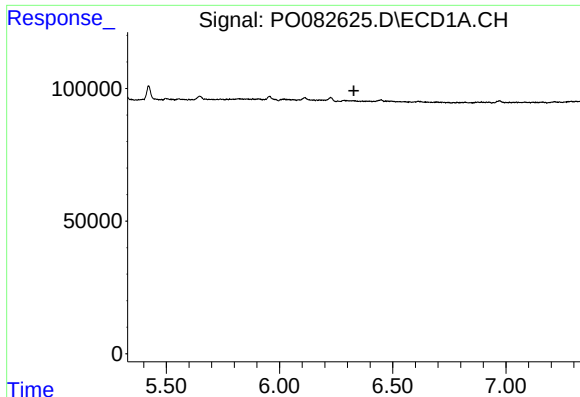

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T.: 6.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

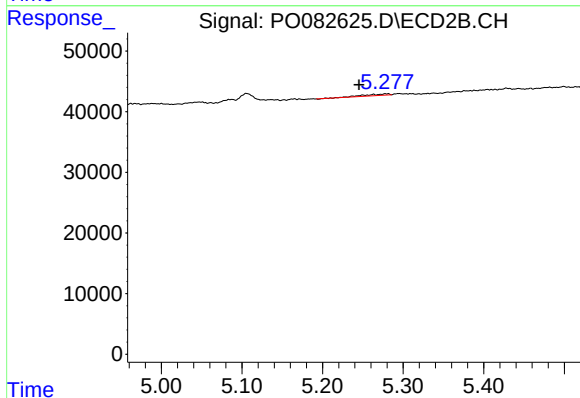


#4 AR-1016-2

R.T.: 5.281 min
Delta R.T.: 0.036 min
Response: 4935
Conc: 2.68 ng/ml

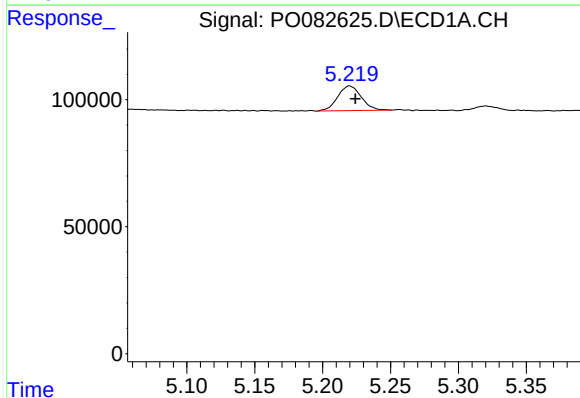


#8 AR-1221-1

R.T.: 5.220 min
Delta R.T.: -0.004 min
Response: 117950
Conc: 125.07 ng/ml

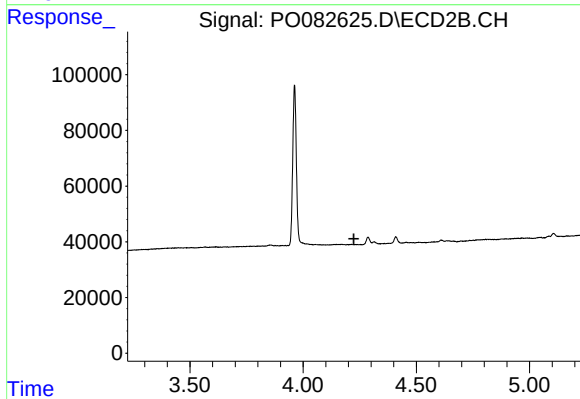

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.224 min
Response: 0
Conc: N.D.

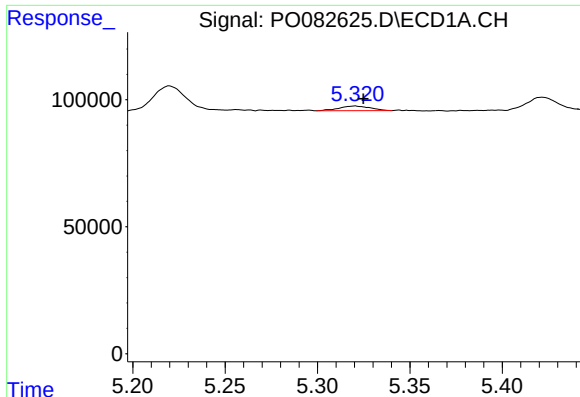

#9 AR-1221-2


R.T.: 5.320 min
Delta R.T.: -0.004 min
Response: 21344
Conc: 32.93 ng/ml

Instrument :
ECD_O
ClientSampleId :

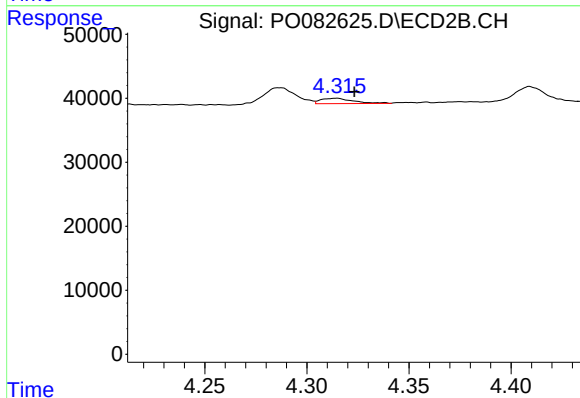


#9 AR-1221-2

R.T.: 4.314 min
Delta R.T.: -0.009 min
Response: 9305
Conc: 32.05 ng/ml

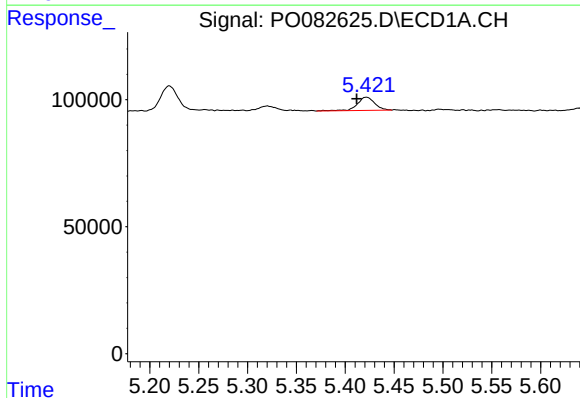


#10 AR-1221-3

R.T.: 5.422 min
Delta R.T.: 0.010 min
Response: 63900
Conc: 30.98 ng/ml

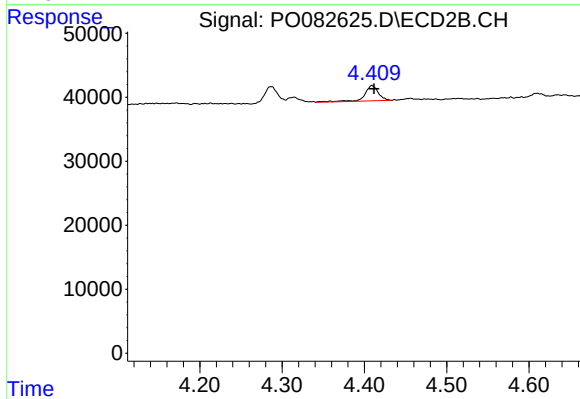

#10 AR-1221-3

R.T.: 4.409 min
Delta R.T.: -0.003 min
Response: 27654
Conc: 29.89 ng/ml

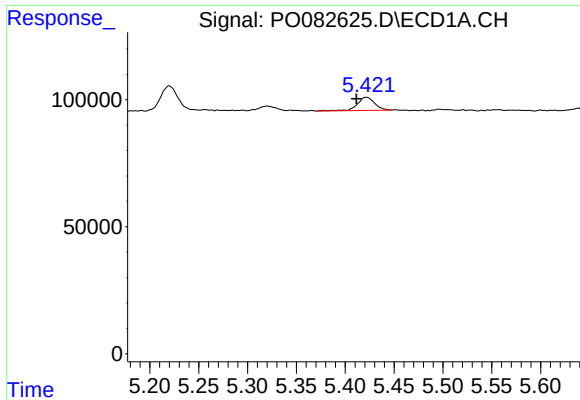

#11 AR-1232-1

R.T.: 5.422 min
Delta R.T.: 0.010 min
Response: 63900
Conc: 36.89 ng/ml

Instrument :
ECD_O
ClientSampleId :

#11 AR-1232-1


R.T.: 4.409 min
Delta R.T.: -0.002 min
Response: 27654
Conc: 35.03 ng/ml

#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 6.328 min
Response: 0
Conc: N.D.

#17 AR-1242-2


R.T.: 5.281 min
Delta R.T.: 0.036 min
Response: 4935
Conc: 3.67 ng/ml

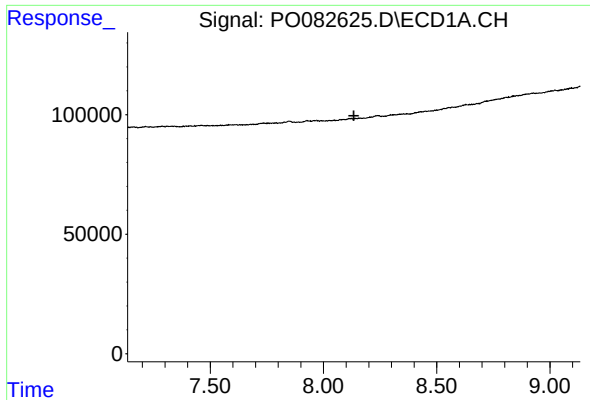

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 8.134 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

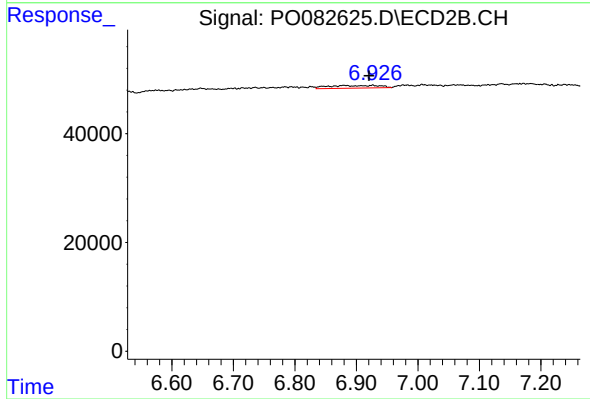


#29 AR-1254-4

R.T.: 6.927 min
Delta R.T.: 0.006 min
Response: 28525
Conc: 15.69 ng/ml

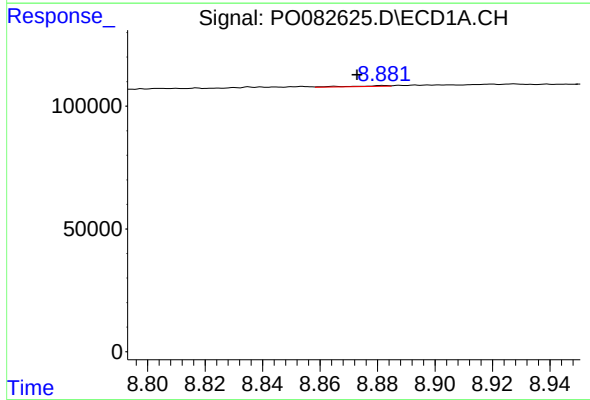

#34 AR-1260-4

R.T.: 8.882 min
Delta R.T.: 0.009 min
Response: 2799
Conc: 0.84 ng/ml

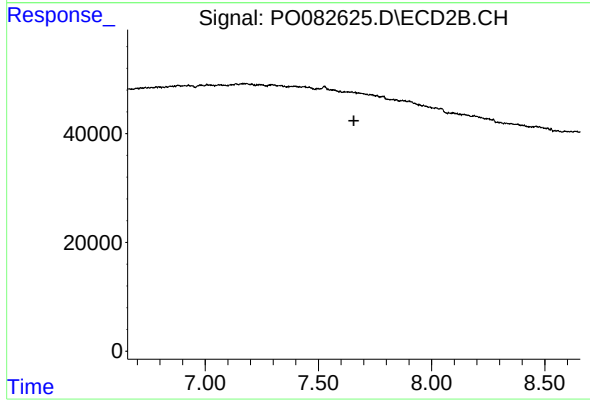

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.657 min
Response: 0
Conc: N.D.