

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
 Data File : PO082648.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 4:41
 Operator : AJ\MA
 Sample : M4577-03
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 08:51:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.964	3.961	1580478	591291	18.057	19.107
2) SA Decachlor...	11.066	9.273	869156	417742	13.763	14.509
Target Compounds						
8) L2 AR-1221-1	5.219	0.000	408947	0	433.638	N.D. #
9) L2 AR-1221-2	5.319	0.000	24590	0	37.936	N.D. #
20) L4 AR-1242-5	0.000	6.127f	0	3242	N.D.	3.511 #
25) L5 AR-1248-5	0.000	6.127	0	3242	N.D.	2.623 #
26) L6 AR-1254-1	0.000	6.127f	0	3242	N.D.	1.669 #
30) L6 AR-1254-5	8.561	0.000	11368	0	3.535	N.D. #
32) L7 AR-1260-2	8.262	0.000	15795	0	4.202	N.D. #
33) L7 AR-1260-3	8.635	0.000	4994	0	1.763	N.D. #
36) L8 AR-1262-1	8.635	0.000	4994	0	1.346	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082648.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 4:41
Operator : AJ\MA
Sample : M4577-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:51:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

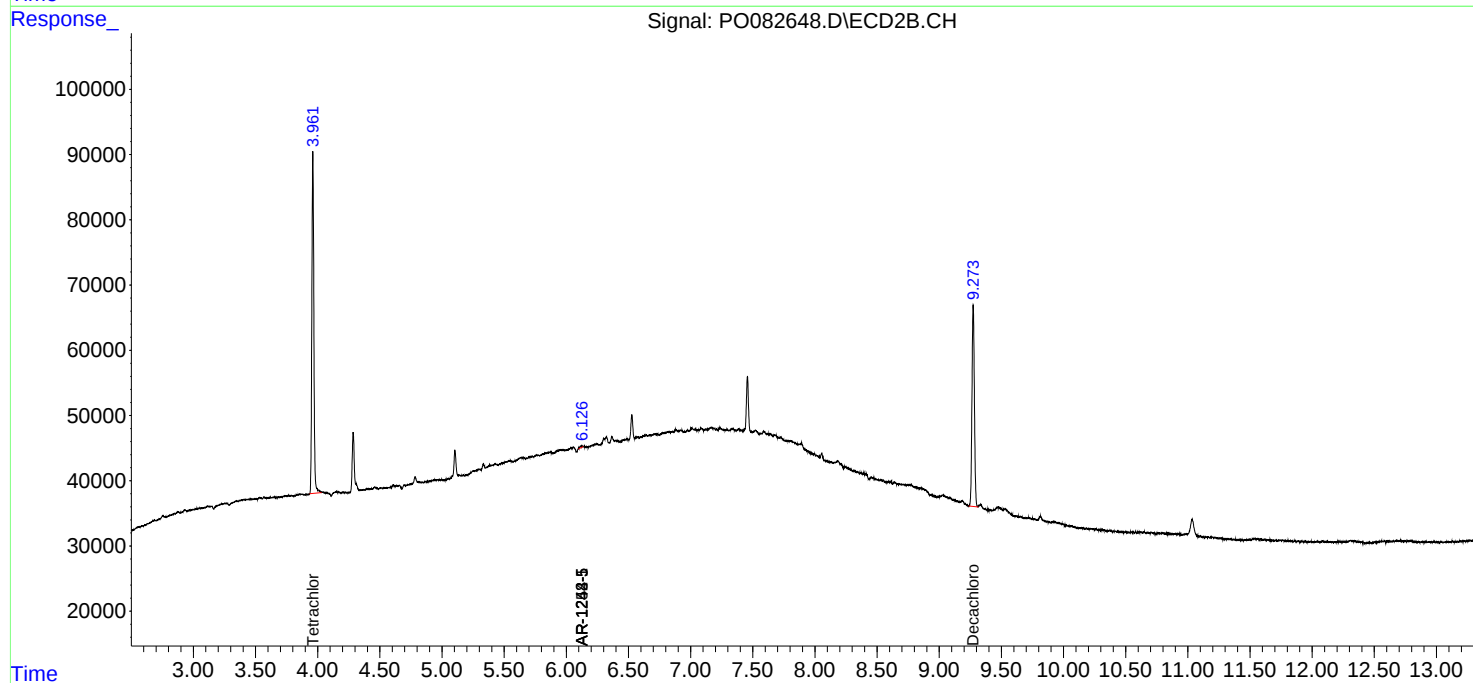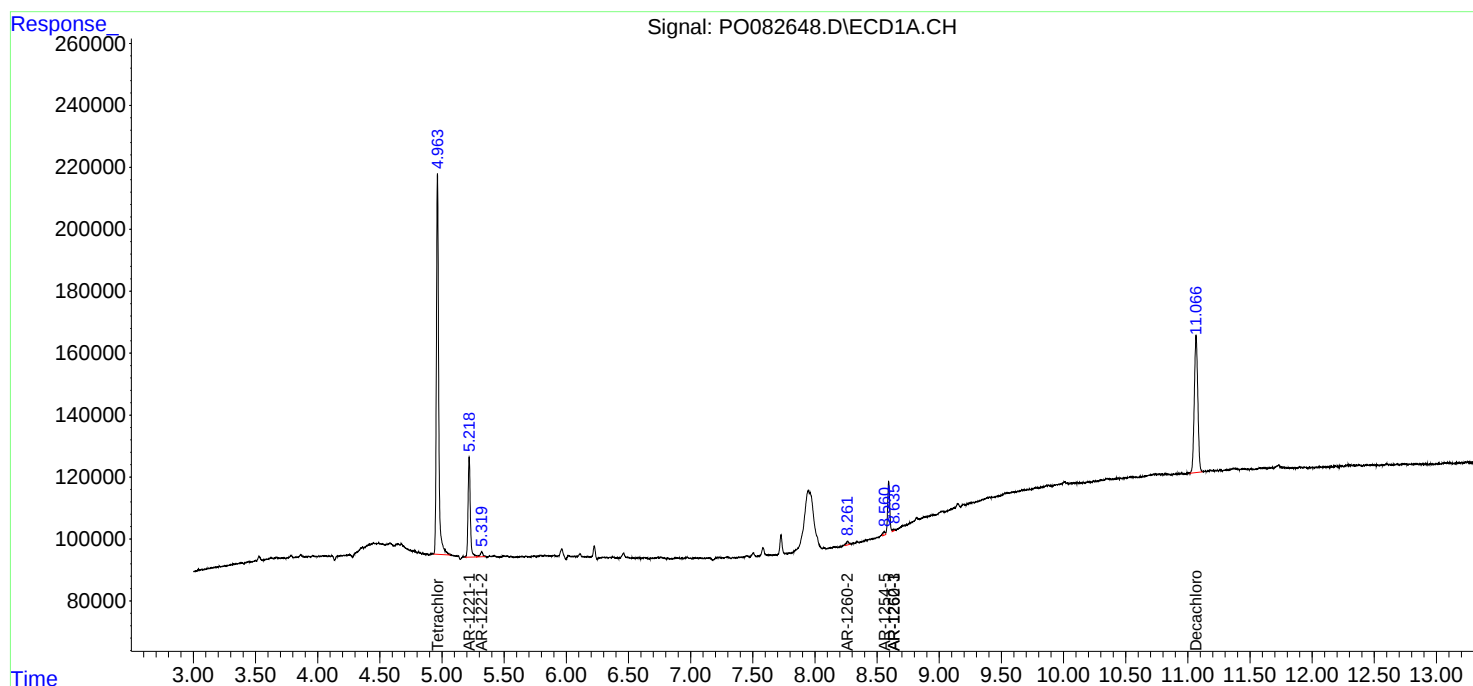


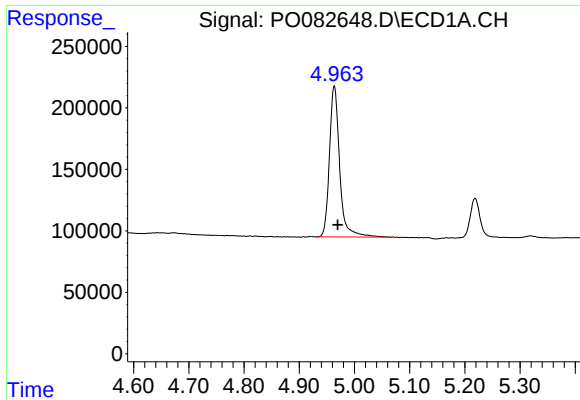

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: -0.006 min
Response: 1580478
Conc: 18.06 ng/ml

Instrument :
ECD_O
ClientSampleId :

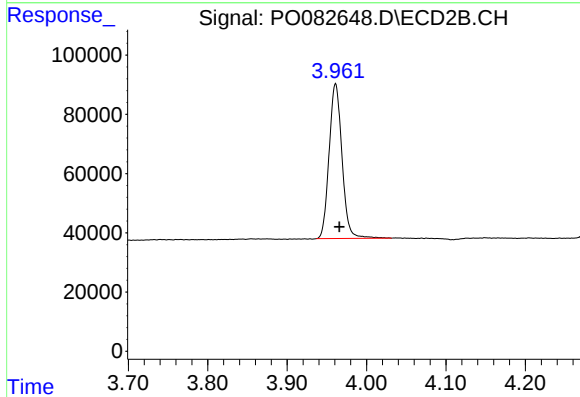


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: -0.005 min
Response: 591291
Conc: 19.11 ng/ml

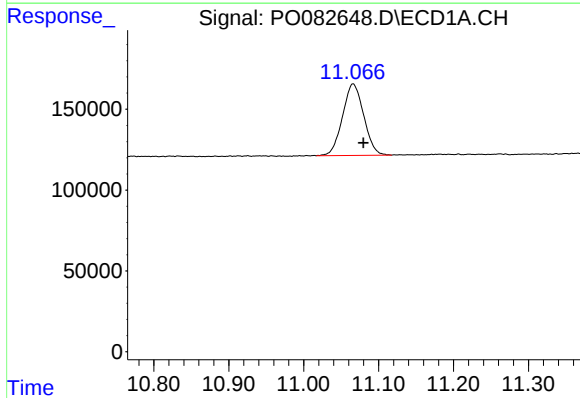


#2 Decachlorobiphenyl

R.T.: 11.066 min
Delta R.T.: -0.014 min
Response: 869156
Conc: 13.76 ng/ml

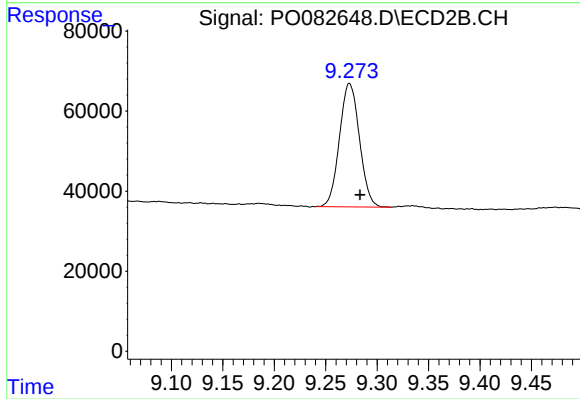

#2 Decachlorobiphenyl


R.T.: 9.273 min
Delta R.T.: -0.010 min
Response: 417742
Conc: 14.51 ng/ml

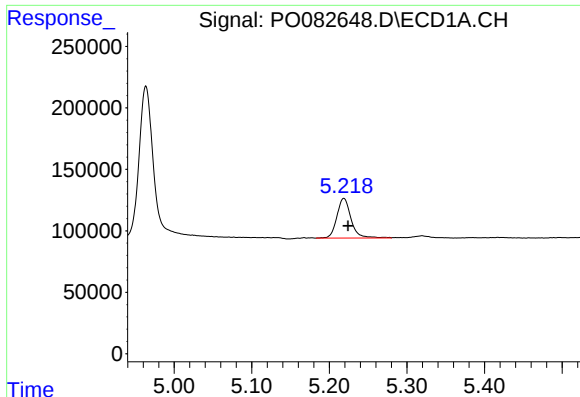

#8 AR-1221-1


R.T.: 5.219 min
Delta R.T.: -0.005 min
Response: 408947
Conc: 433.64 ng/ml

Instrument :
ECD_O
ClientSampleId :

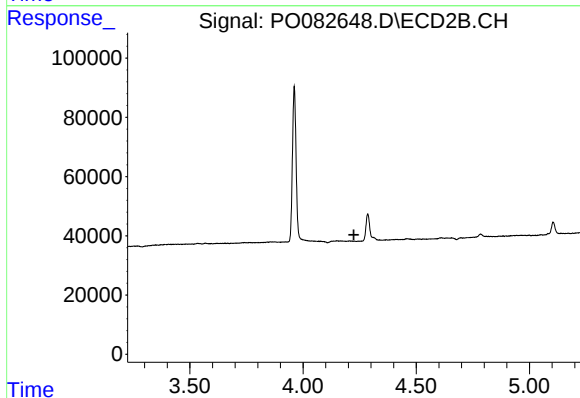


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.224 min
Response: 0
Conc: N.D.

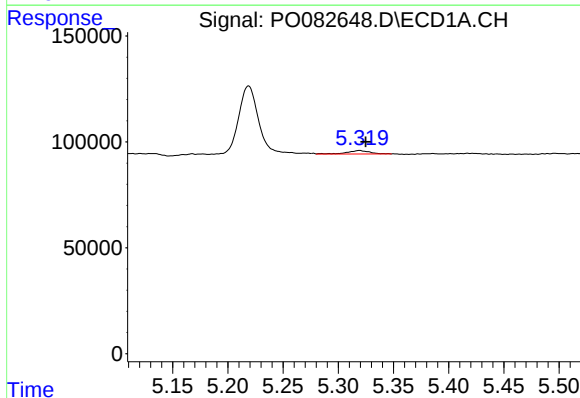


#9 AR-1221-2

R.T.: 5.319 min
Delta R.T.: -0.005 min
Response: 24590
Conc: 37.94 ng/ml

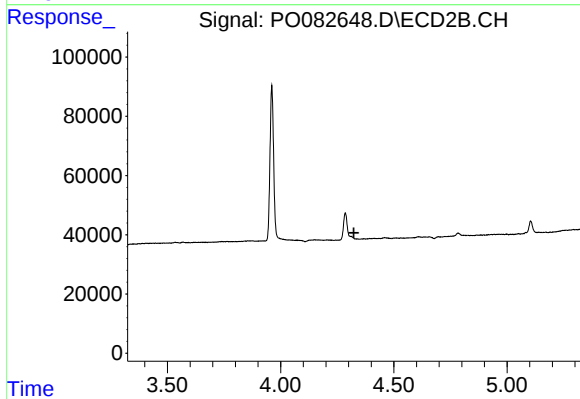

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.323 min
Response: 0
Conc: N.D.

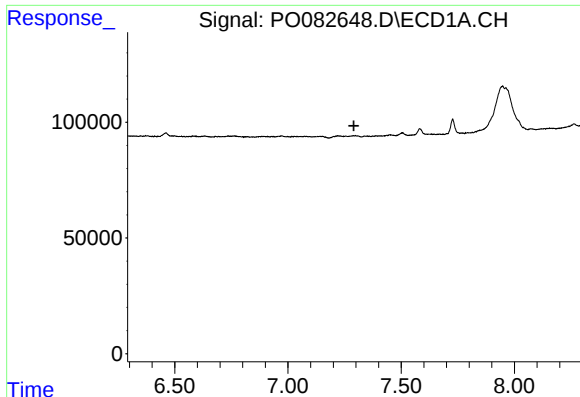

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

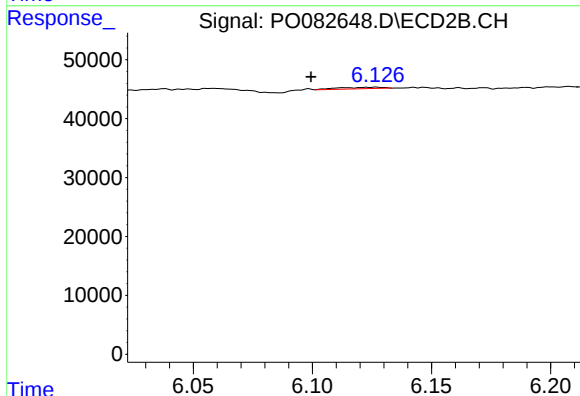


#20 AR-1242-5

R.T.: 6.127 min
Delta R.T.: 0.027 min
Response: 3242
Conc: 3.51 ng/ml

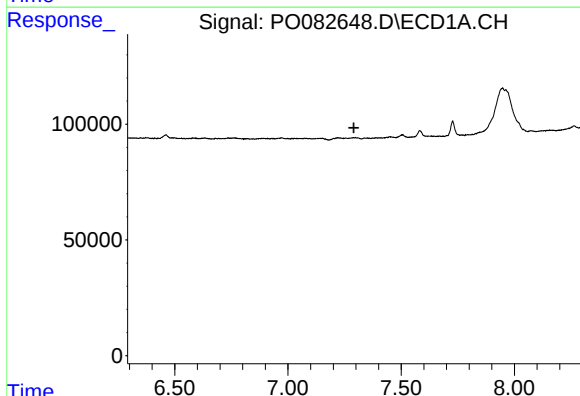


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.291 min
Response: 0
Conc: N.D.

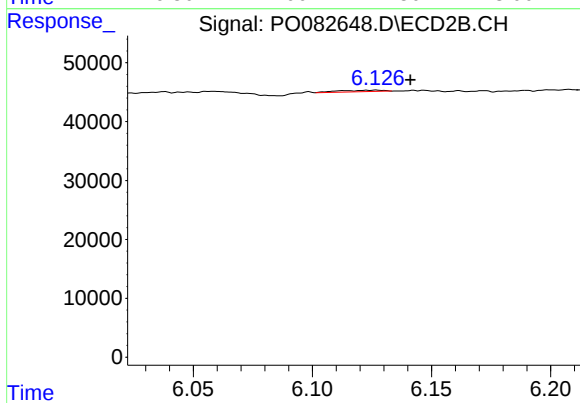

#25 AR-1248-5


R.T.: 6.127 min
Delta R.T.: -0.014 min
Response: 3242
Conc: 2.62 ng/ml

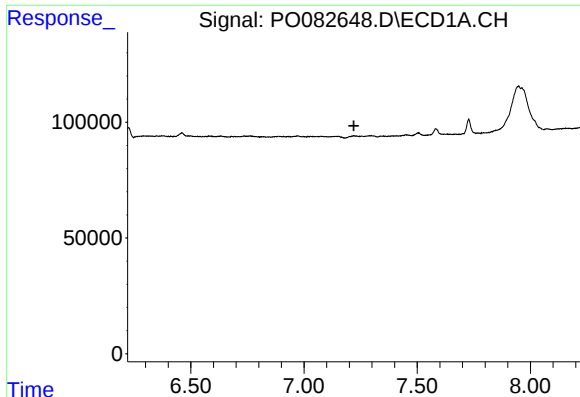

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 7.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

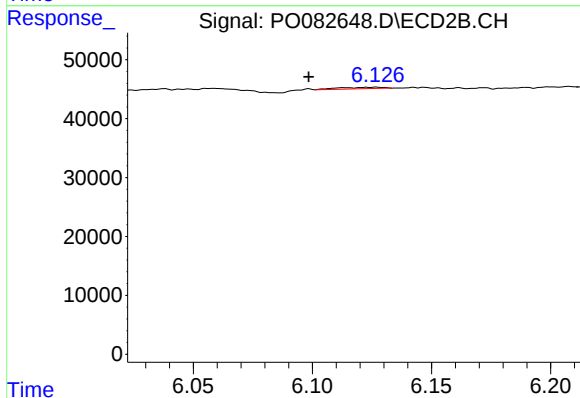


#26 AR-1254-1

R.T.: 6.127 min
Delta R.T.: 0.028 min
Response: 3242
Conc: 1.67 ng/ml

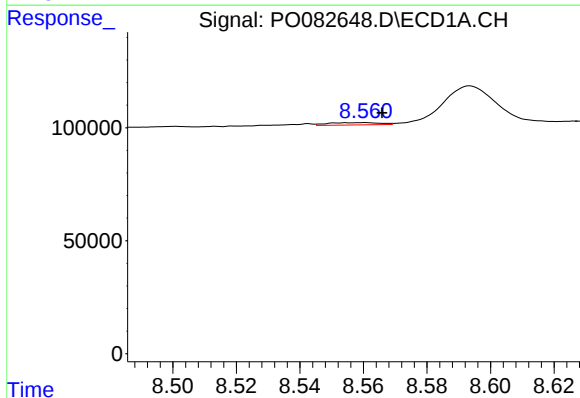


#30 AR-1254-5

R.T.: 8.561 min
Delta R.T.: -0.005 min
Response: 11368
Conc: 3.53 ng/ml

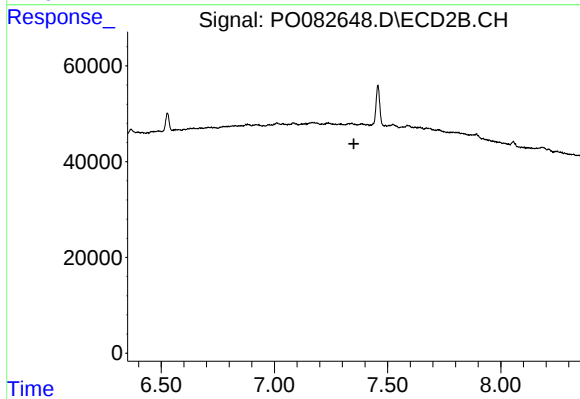

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.351 min
Response: 0
Conc: N.D.

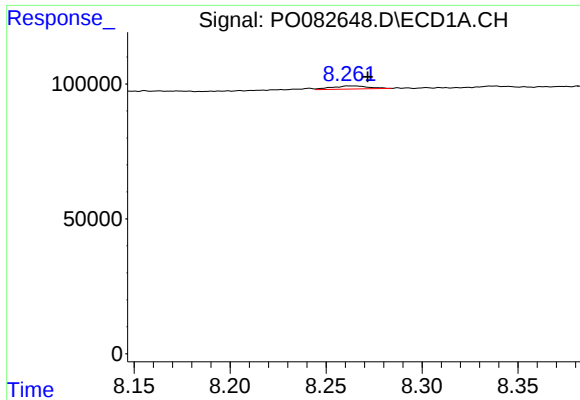

#32 AR-1260-2


R.T.: 8.262 min
Delta R.T.: -0.010 min
Response: 15795
Conc: 4.20 ng/ml

Instrument :
ECD_O
ClientSampleId :

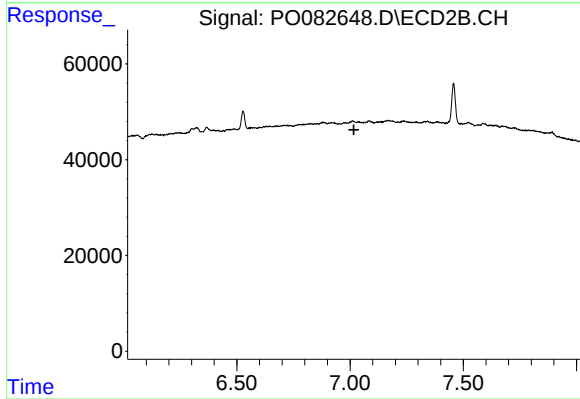


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

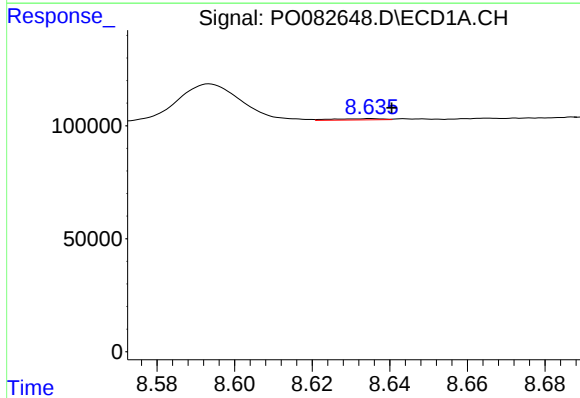


#33 AR-1260-3

R.T.: 8.635 min
Delta R.T.: -0.005 min
Response: 4994
Conc: 1.76 ng/ml

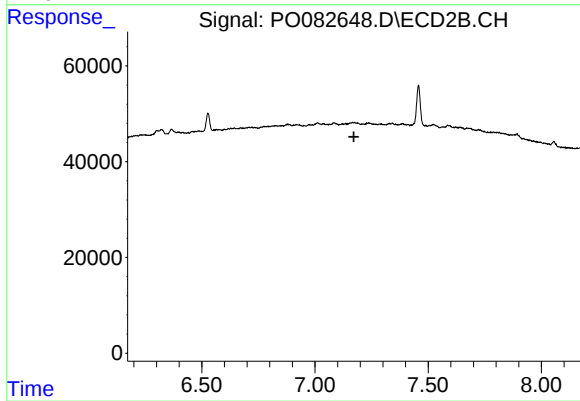

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.172 min
Response: 0
Conc: N.D.

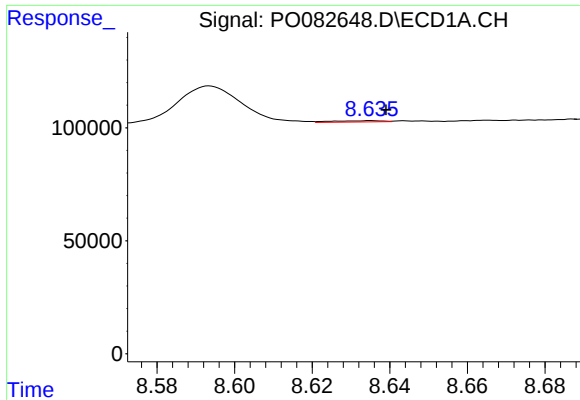

#36 AR-1262-1

R.T.: 8.635 min
Delta R.T.: -0.004 min
Response: 4994
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :

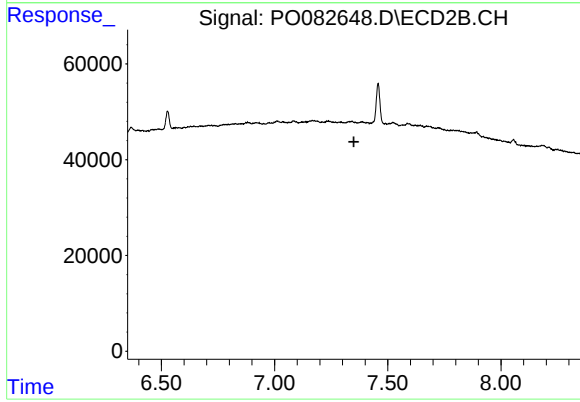

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.350 min
Response: 0
Conc: N.D.