

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082601.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 14:37
Operator : AJ\MA
Sample : PB140443BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140443BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:25:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.966	3.964	1622596	599157	18.538	19.361
2)	SA Decachlor...	11.070	9.278	1179192	607998	18.672	21.117

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082601.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 14:37
Operator : AJ\MA
Sample : PB140443BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140443BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:25:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

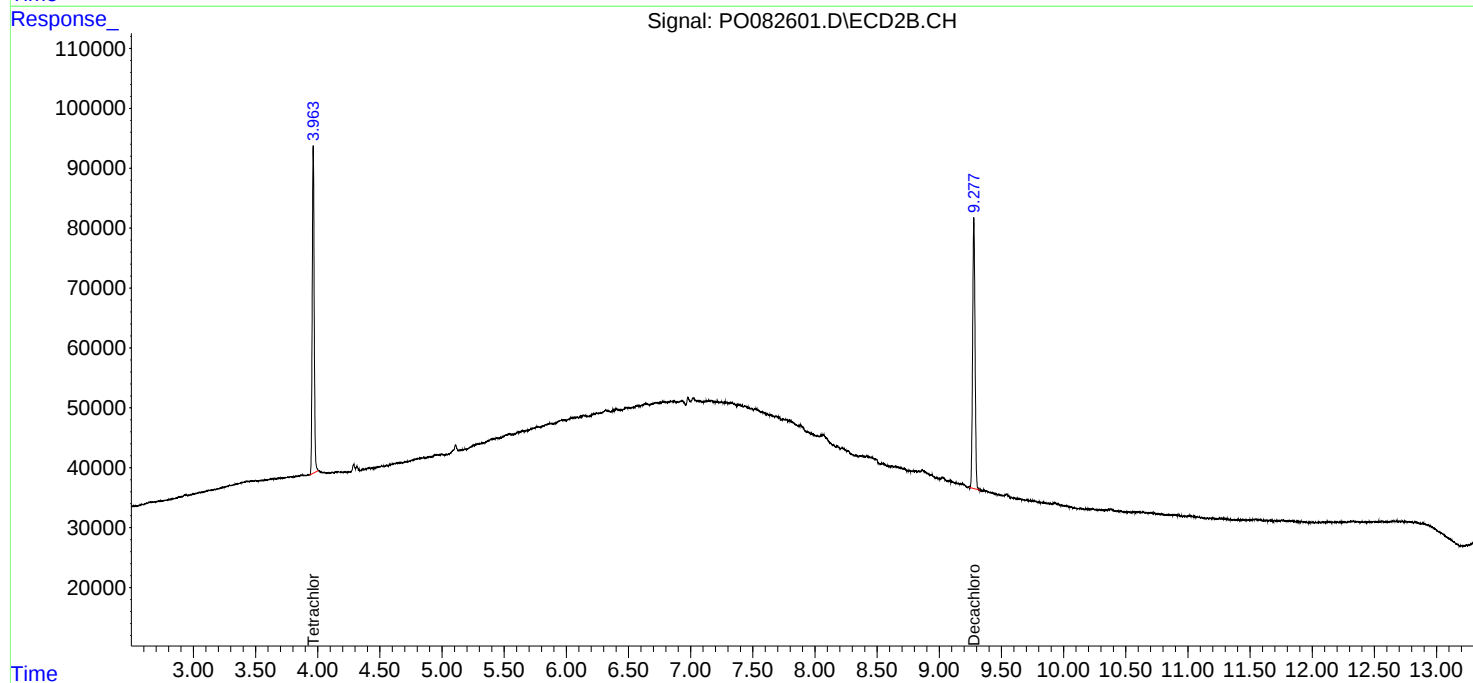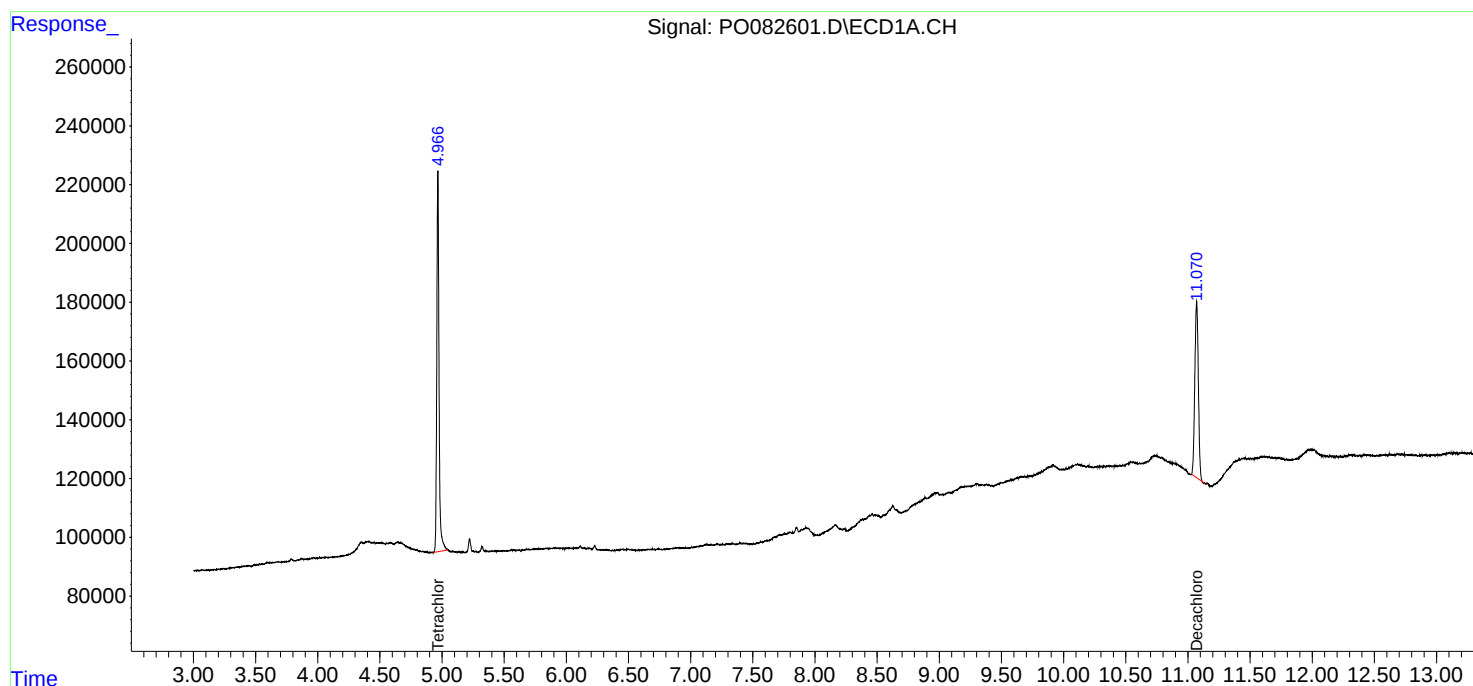


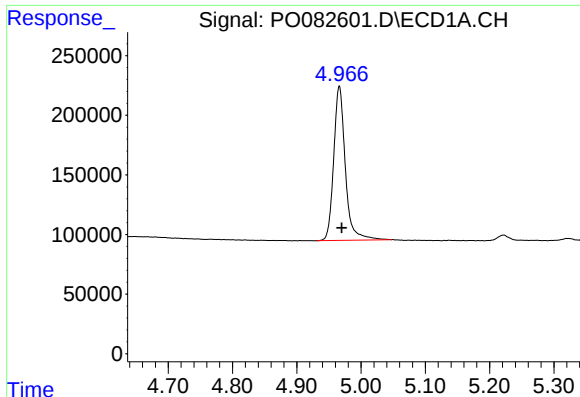

#1 Tetrachloro-m-xylene


R.T.: 4.966 min
Delta R.T.: -0.004 min
Response: 1622596
Conc: 18.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB140443BL

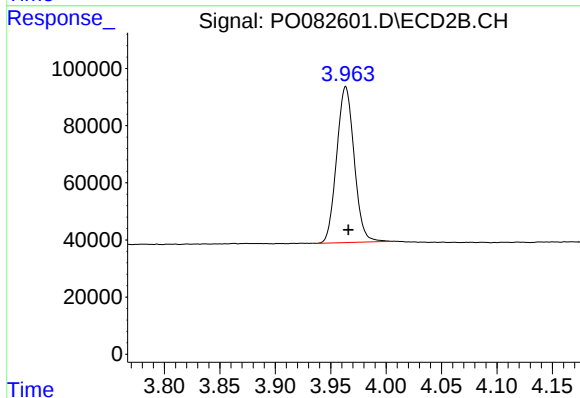


#1 Tetrachloro-m-xylene

R.T.: 3.964 min
Delta R.T.: -0.002 min
Response: 599157
Conc: 19.36 ng/ml

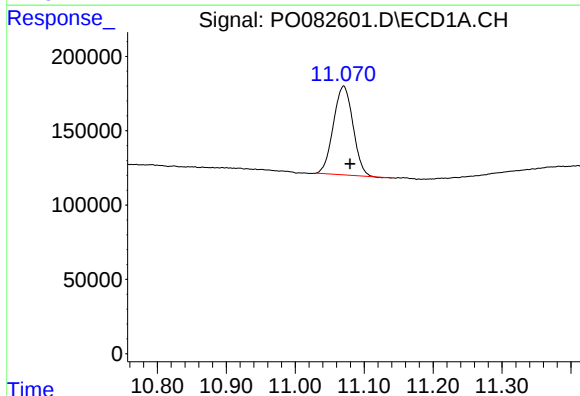

#2 Decachlorobiphenyl

R.T.: 11.070 min
Delta R.T.: -0.009 min
Response: 1179192
Conc: 18.67 ng/ml

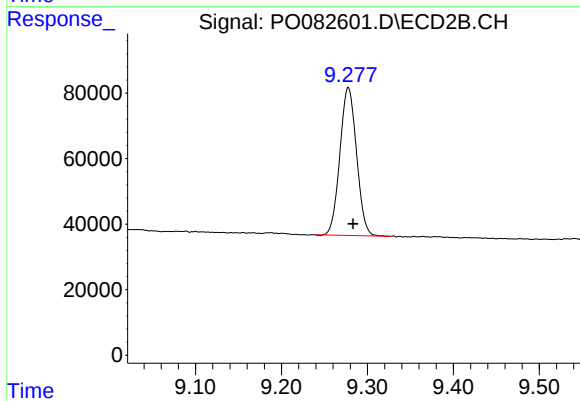

#2 Decachlorobiphenyl

R.T.: 9.278 min
Delta R.T.: -0.006 min
Response: 607998
Conc: 21.12 ng/ml