

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 19:13
Operator : AJ\MA
Sample : M4540-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:30:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.965	3.962	1817981	673050	20.770	21.749
2)	SA Decachlor...	11.069	9.276	1081940	511781	17.132	17.775

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110821\
Data File : PO082617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2021 19:13
Operator : AJ\MA
Sample : M4540-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:30:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

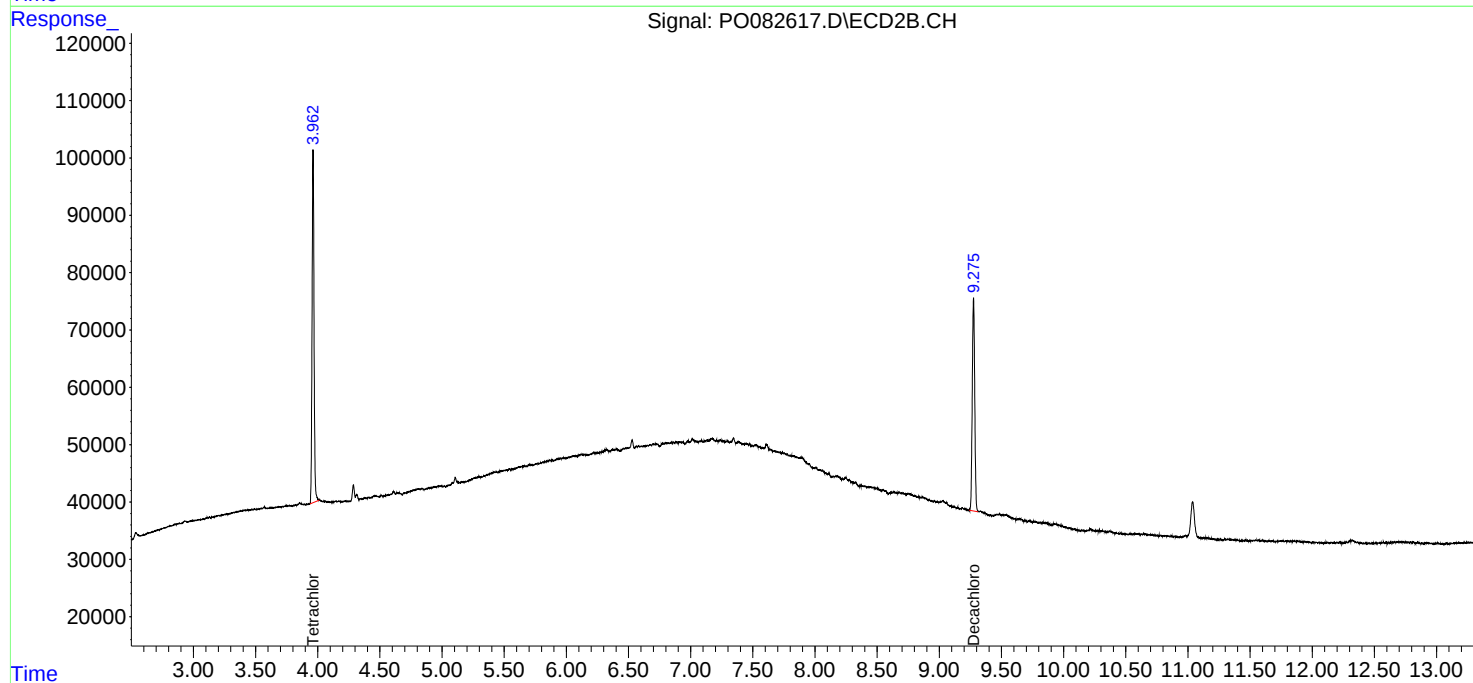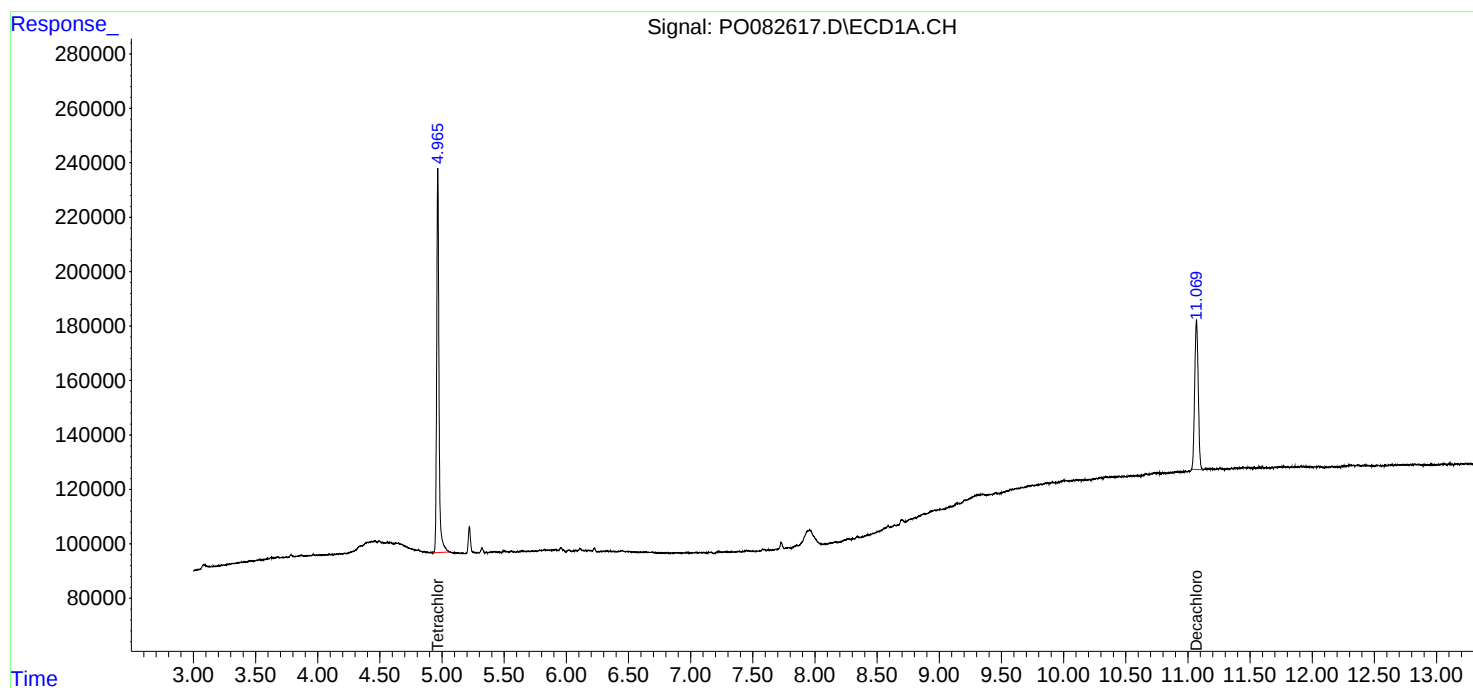


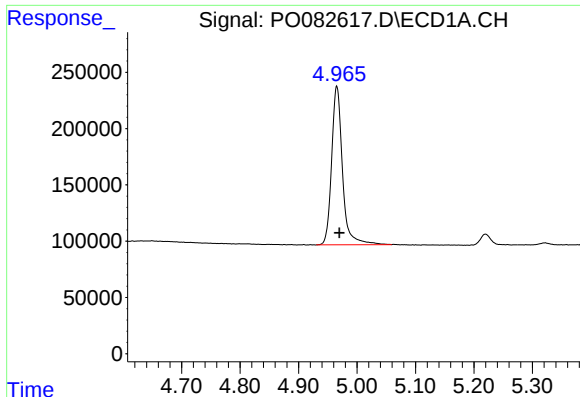

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: -0.005 min
Response: 1817981
Conc: 20.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2

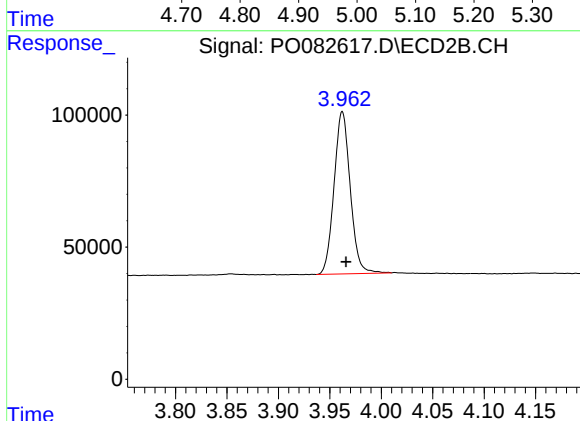


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.004 min
Response: 673050
Conc: 21.75 ng/ml

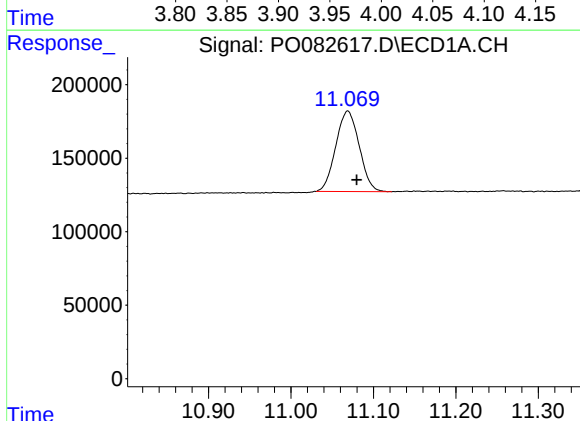

#2 Decachlorobiphenyl

R.T.: 11.069 min
Delta R.T.: -0.011 min
Response: 1081940
Conc: 17.13 ng/ml

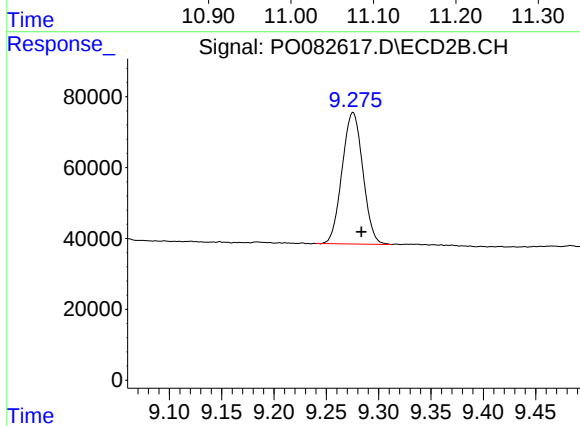

#2 Decachlorobiphenyl

R.T.: 9.276 min
Delta R.T.: -0.008 min
Response: 511781
Conc: 17.77 ng/ml