

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110824\
 Data File : PO107820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Nov 2024 17:43
 Operator : YP/AJ
 Sample : P4771-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2024
 Supervised By :Ankita Jodhani 11/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 01:40:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Oct 28 11:34:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.371	3.642	136.1E6	63692852	14.930m	19.790 #
2) SA Decachlor...	10.084	8.638	53267612	57723236	21.712	21.055m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110824\
Data File : PO107820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Nov 2024 17:43
Operator : YP/AJ
Sample : P4771-05
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :Ankita Jodhani 11/11/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 01:40:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101524.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 28 11:34:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

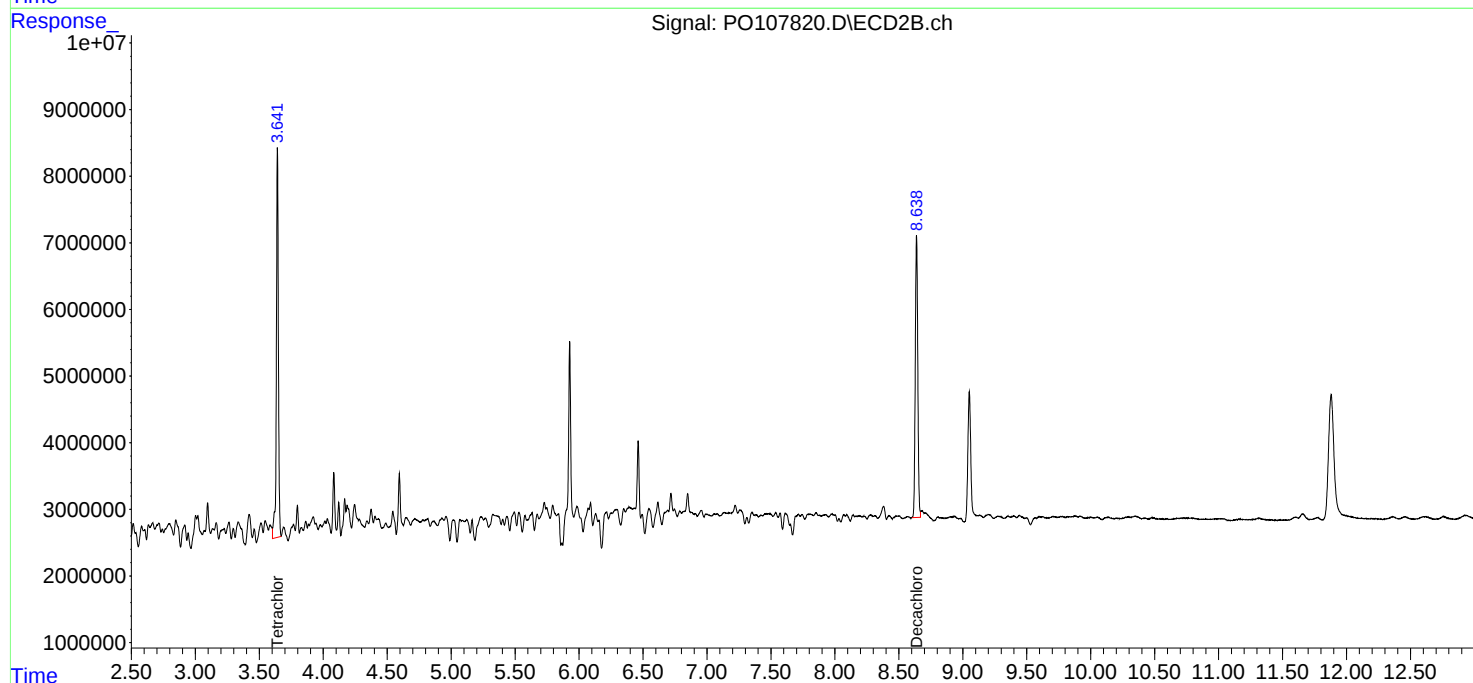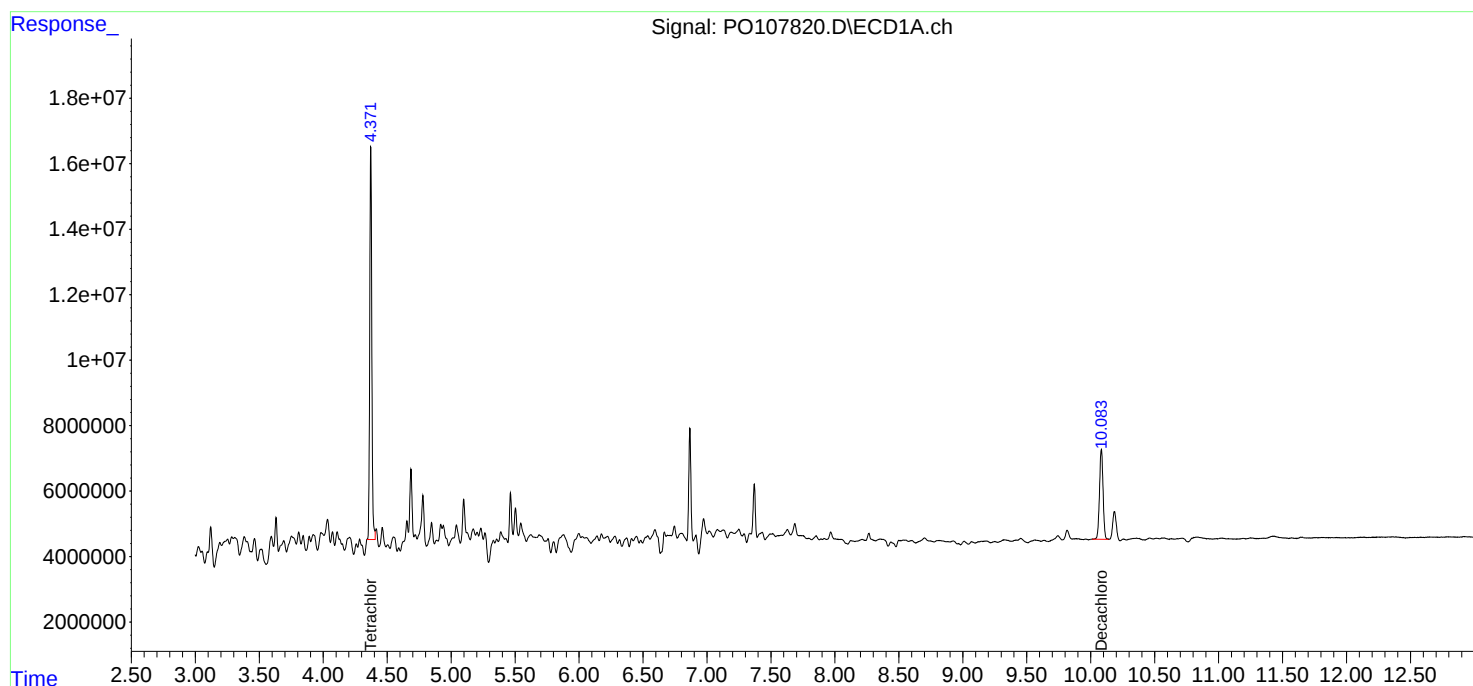

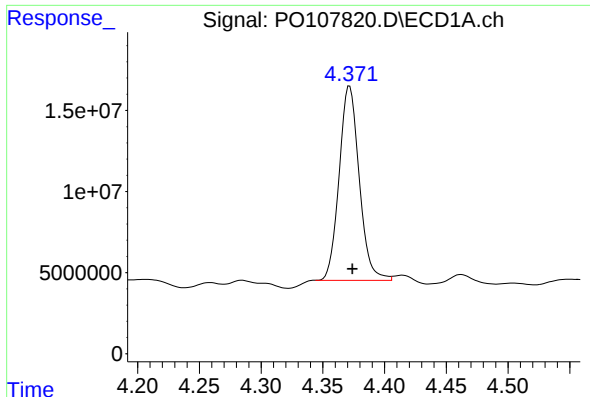


#1 Tetrachloro-m-xylene

R.T.: 4.371 min
Delta R.T.: -0.003 min
Response: 136068307
Conc: 14.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
P-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2024
Supervised By :Ankita Jodhani 11/11/2024

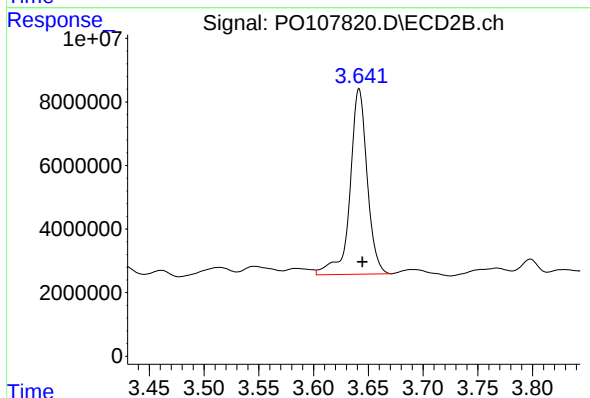


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.003 min
Response: 63692852
Conc: 19.79 ng/ml

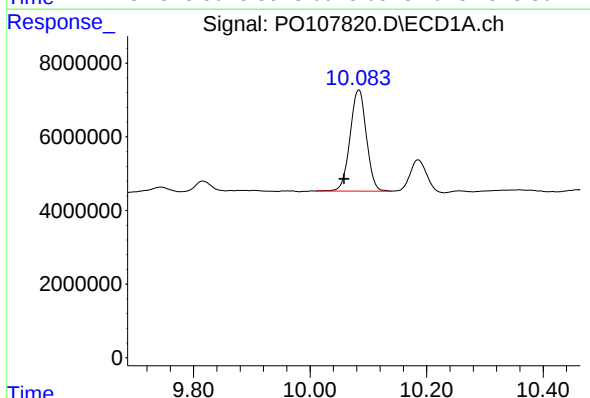

#2 Decachlorobiphenyl

R.T.: 10.084 min
Delta R.T.: 0.025 min
Response: 53267612
Conc: 21.71 ng/ml

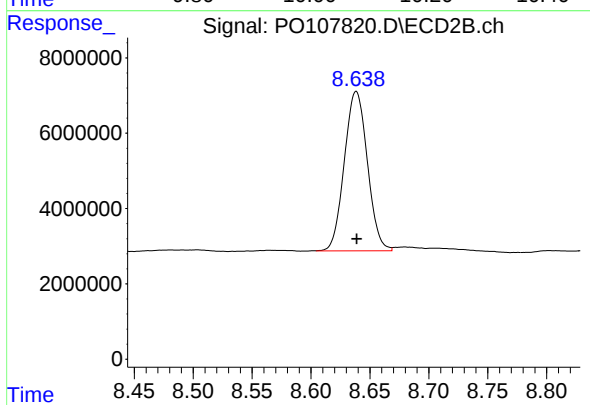

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: 0.000 min
Response: 57723236
Conc: 21.05 ng/ml m