

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110918\
 Data File : P0051280.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Nov 2018 18:27
 Operator : SM/SJ
 Sample : J5796-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 435X-14A

Manual Integrations
 APPROVED

Sohil
 11/9/2018 4:38:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 07:35:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 08 14:50:13 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.335	3.334	11277265	3742592	20.003	16.773
2) SA Decachlor...	9.973	8.067	4435744	2767975	11.954m	12.488m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110918\
Data File : P0051280.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2018 18:27
Operator : SM/SJ
Sample : J5796-15
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
435X-14A


Manual Integrations
APPROVED

Sohil
11/9/2018 4:38:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 07:35:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

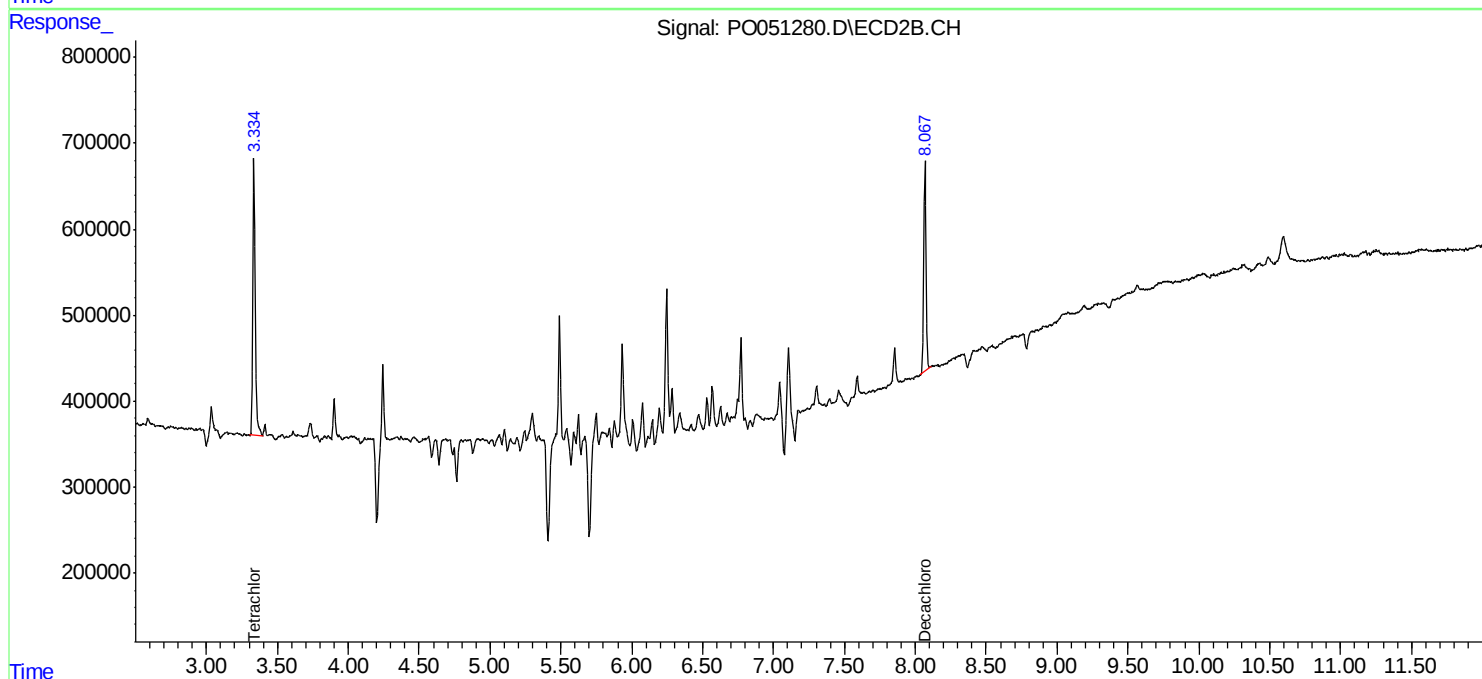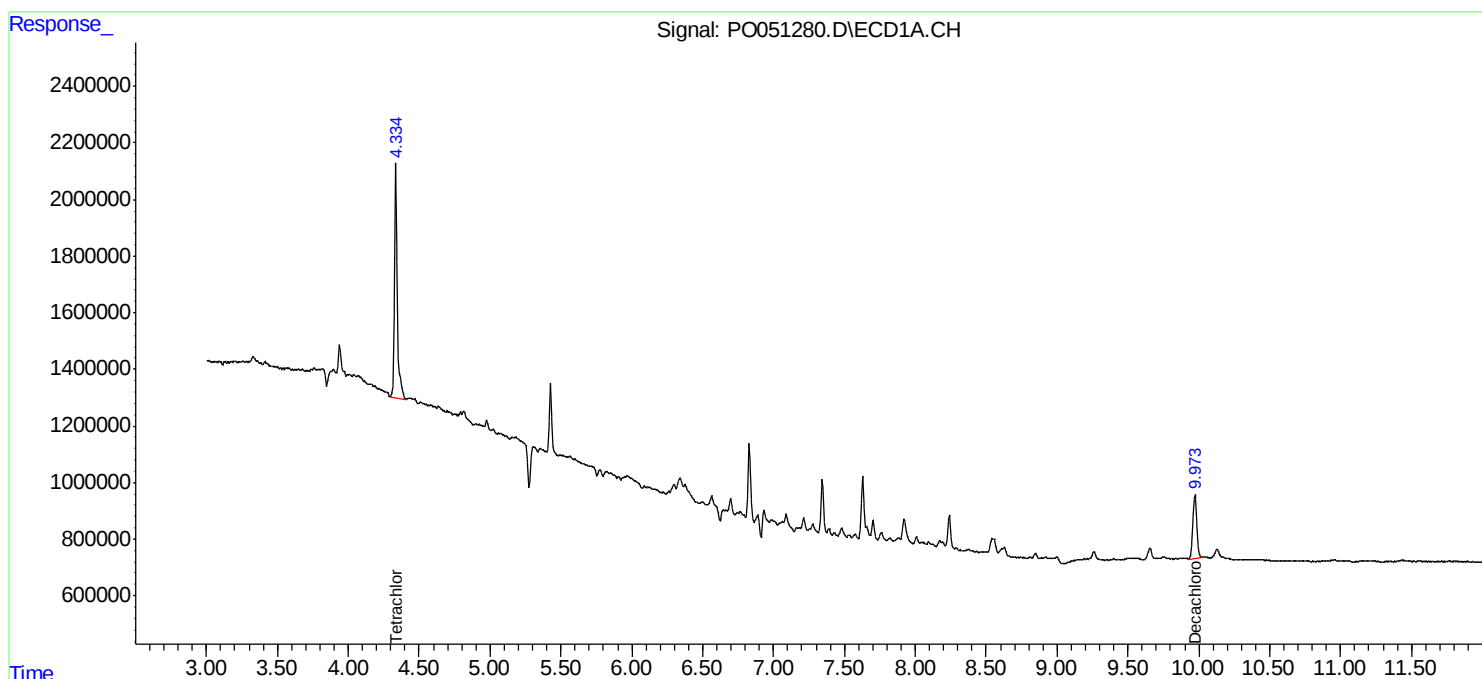

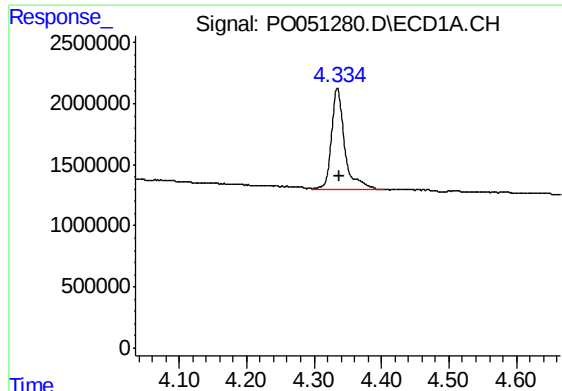


#1 Tetrachloro-m-xylene

R.T.: 4.335 min
Delta R.T.: -0.003 min
Response: 11277265
Conc: 20.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
435X-14A


Manual Integrations
APPROVED

Sohil
11/9/2018 4:38:26 PM

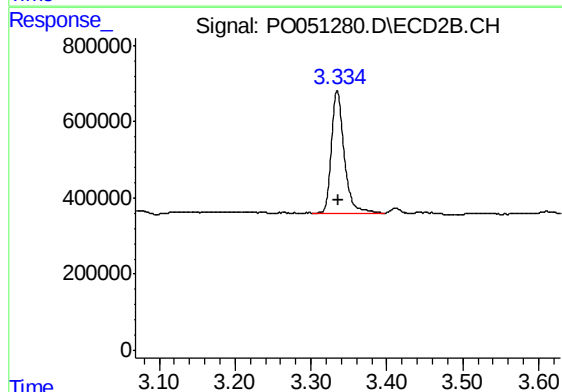


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: -0.002 min
Response: 3742592
Conc: 16.77 ng/ml

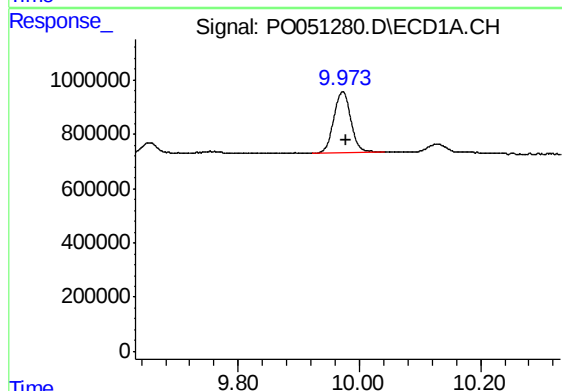

#2 Decachlorobiphenyl

R.T.: 9.973 min
Delta R.T.: -0.005 min
Response: 4435744
Conc: 11.95 ng/ml m

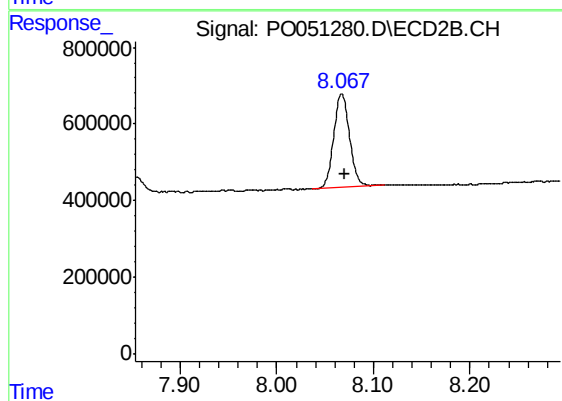

#2 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: -0.003 min
Response: 2767975
Conc: 12.49 ng/ml m