

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110918\
Data File : P0051286.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2018 20:25
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 07:37:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.336	3.336	14796087	5481842	26.245	24.567
2)	SA Decachlor...	9.972	8.069	8884273	5669439	23.943	25.579

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110918\
Data File : PO051286.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Nov 2018 20:25
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 07:37:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

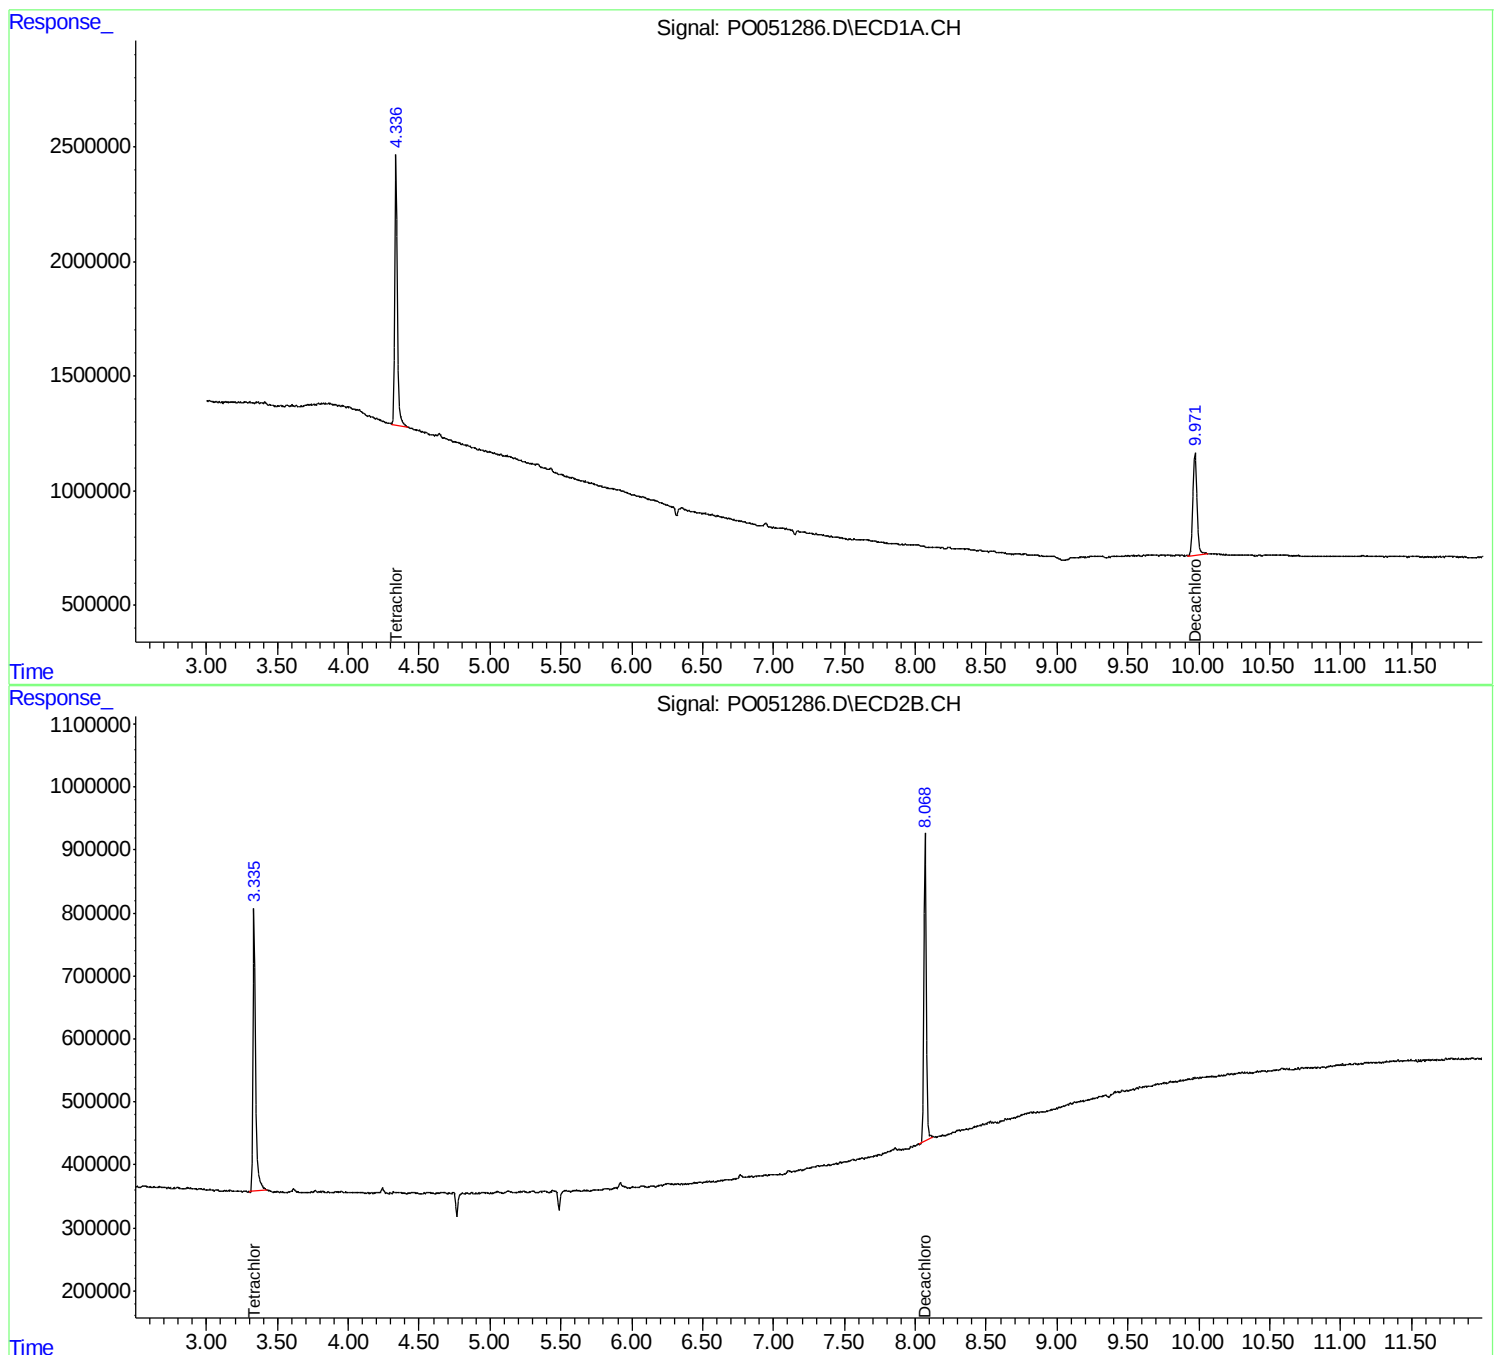


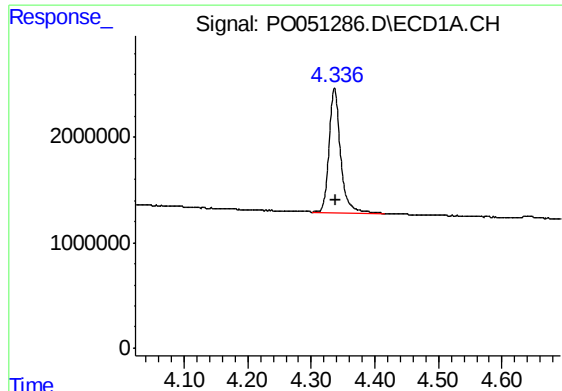

#1 Tetrachloro-m-xylene


R.T.: 4.336 min
Delta R.T.: -0.002 min
Response: 14796087
Conc: 26.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

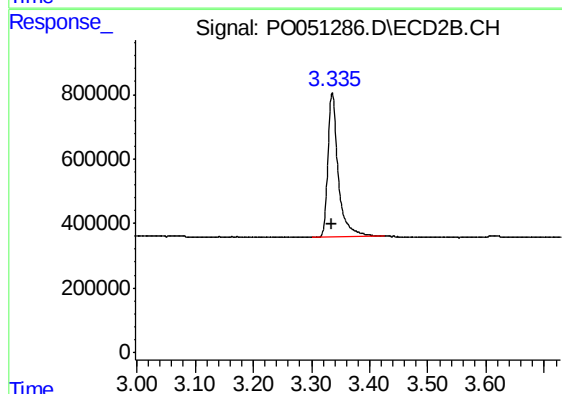


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 5481842
Conc: 24.57 ng/ml

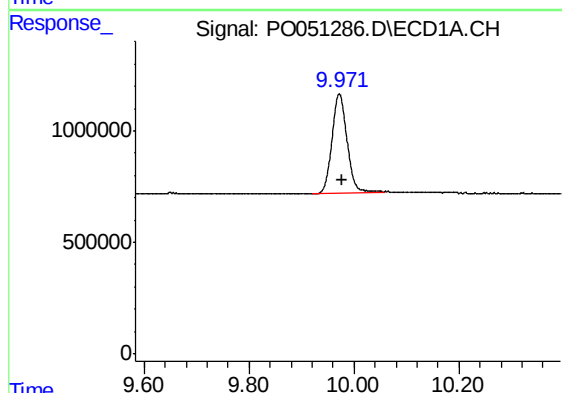

#2 Decachlorobiphenyl

R.T.: 9.972 min
Delta R.T.: -0.005 min
Response: 8884273
Conc: 23.94 ng/ml

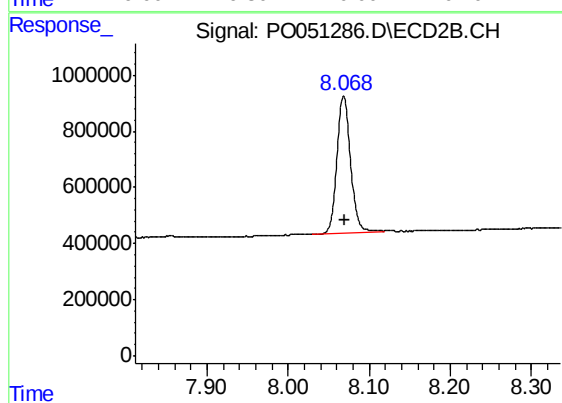

#2 Decachlorobiphenyl

R.T.: 8.069 min
Delta R.T.: -0.001 min
Response: 5669439
Conc: 25.58 ng/ml