

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110918\
Data File : P0051300.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 00:56
Operator : SM/SJ
Sample : J5805-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLES(11-15)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:16:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.335	3.336	11996409	5028633	21.279	22.536
2)	SA Decachlor...	9.971	8.068	5956839	2519988	16.053	11.370 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110918\
Data File : P0051300.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 00:56
Operator : SM/SJ
Sample : J5805-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLES(11-15)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 08:16:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

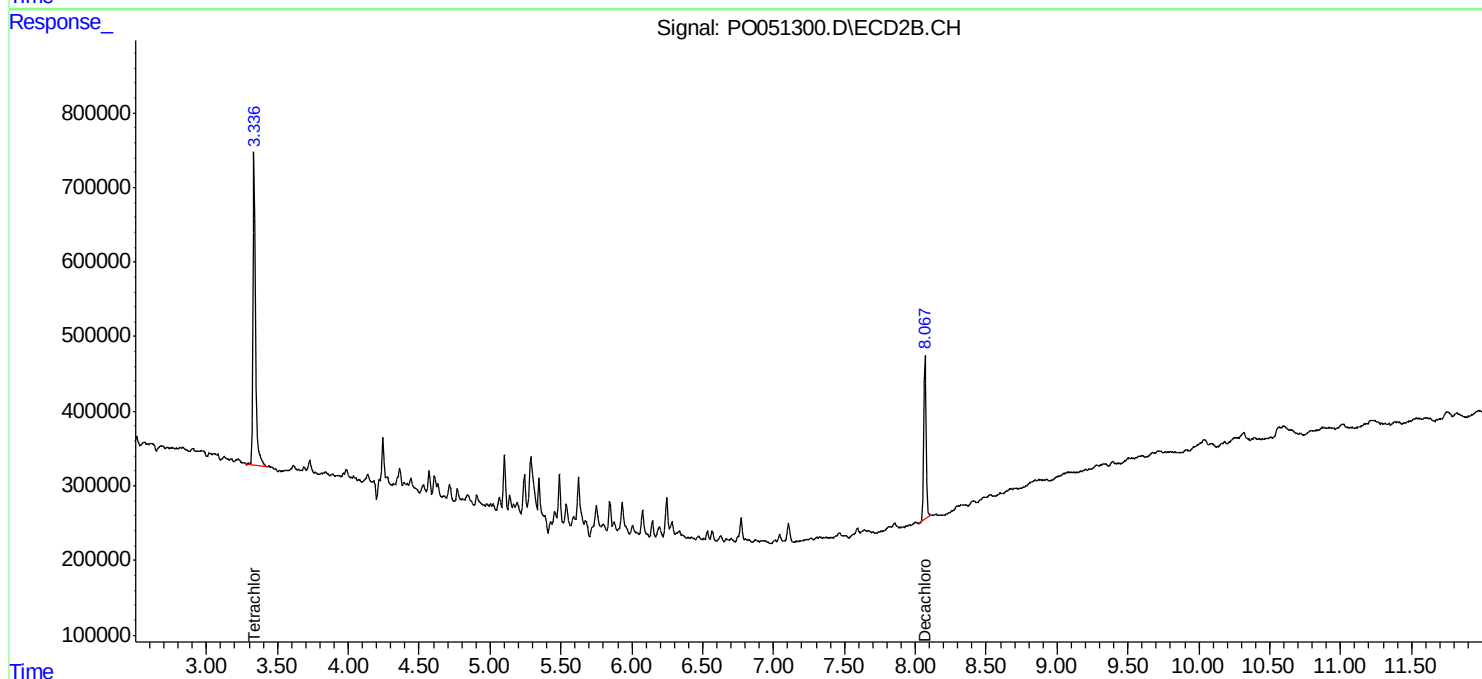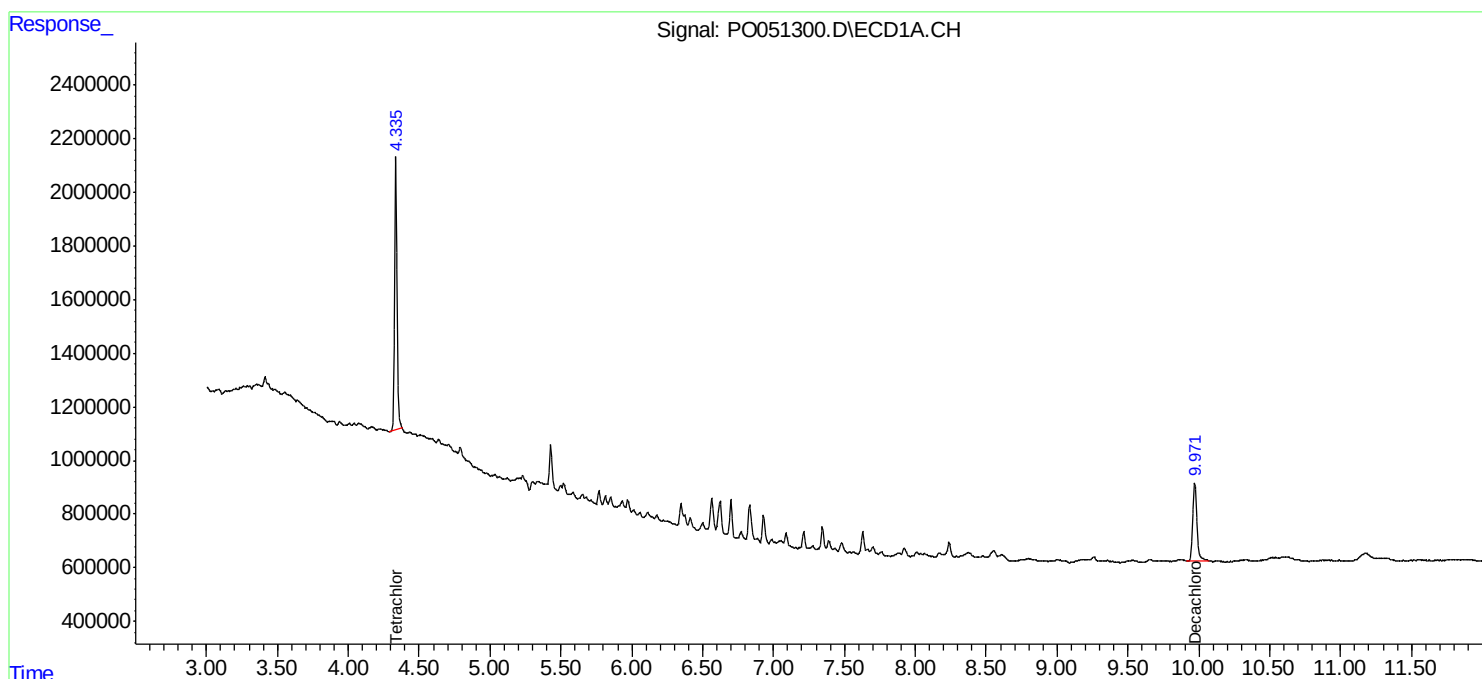


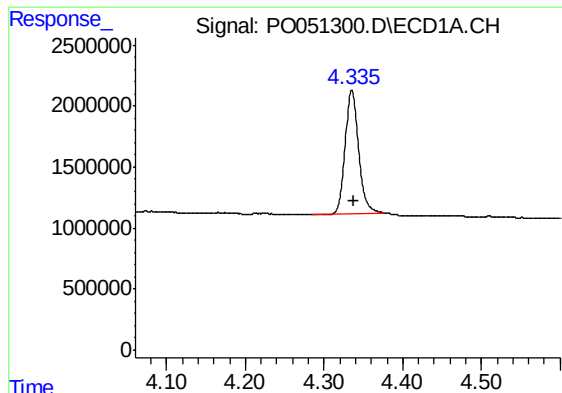

#1 Tetrachloro-m-xylene


R.T.: 4.335 min
Delta R.T.: -0.003 min
Response: 11996409
Conc: 21.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLES(11-15)

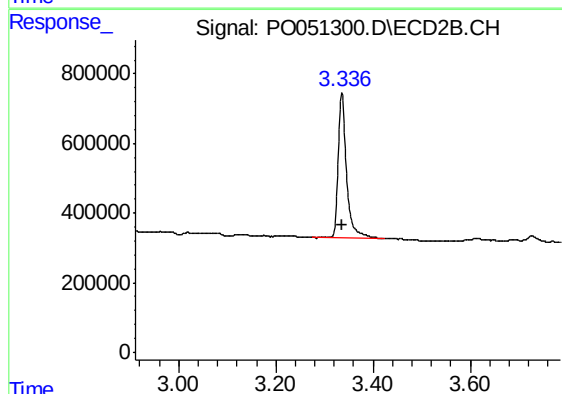


#1 Tetrachloro-m-xylene

R.T.: 3.336 min
Delta R.T.: 0.000 min
Response: 5028633
Conc: 22.54 ng/ml

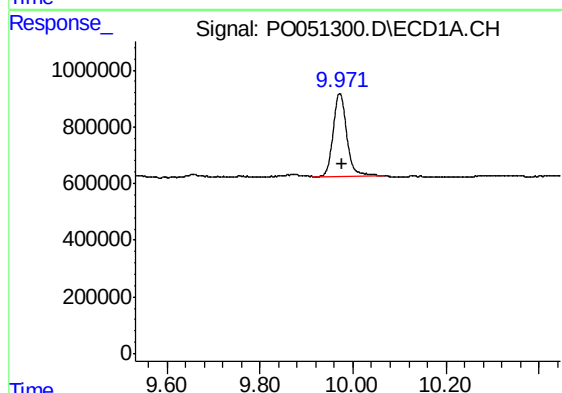

#2 Decachlorobiphenyl

R.T.: 9.971 min
Delta R.T.: -0.006 min
Response: 5956839
Conc: 16.05 ng/ml

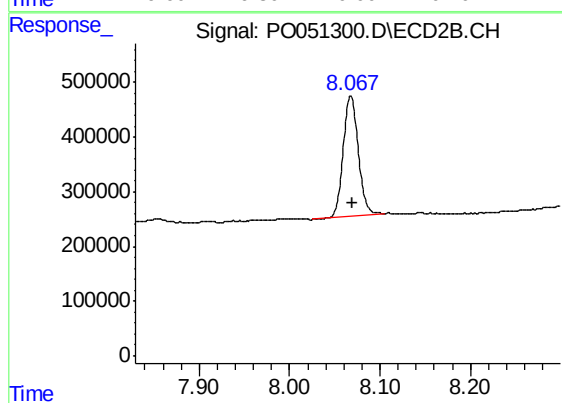

#2 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: -0.002 min
Response: 2519988
Conc: 11.37 ng/ml