

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110921\
 Data File : PO082661.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 10:09
 Operator : AJ\MA
 Sample : PB140588BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB140588BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 13:34:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.964	3.962	1785216	668641	20.396	21.606
2)	SA Decachlor...	11.065	9.275	1371966	679006	21.725	23.583

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110921\
Data File : PO082661.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 10:09
Operator : AJ\MA
Sample : PB140588BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140588BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 13:34:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

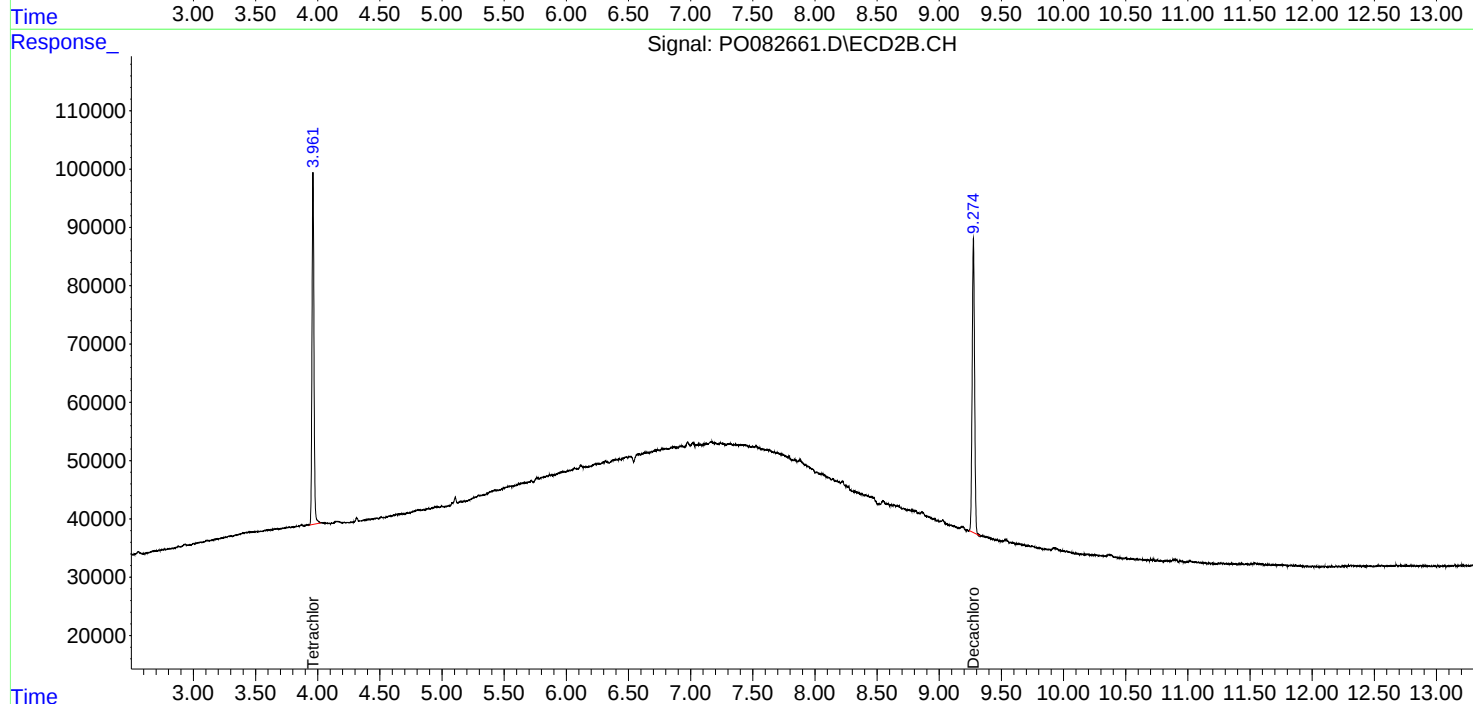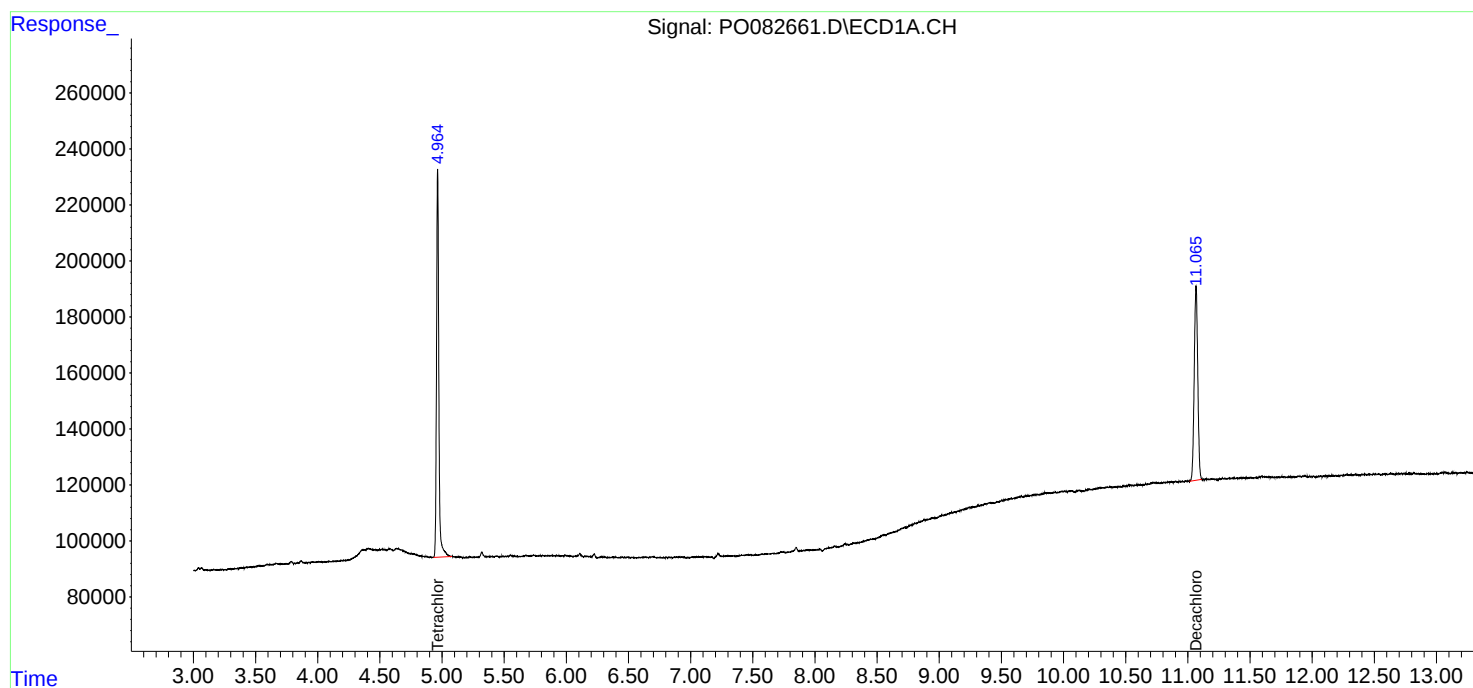


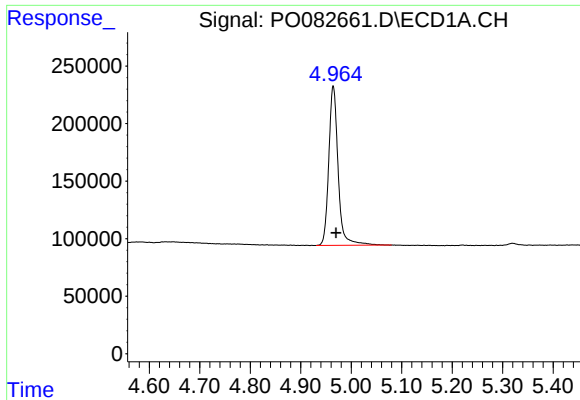

#1 Tetrachloro-m-xylene


R.T.: 4.964 min
Delta R.T.: -0.006 min
Response: 1785216
Conc: 20.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB140588BL

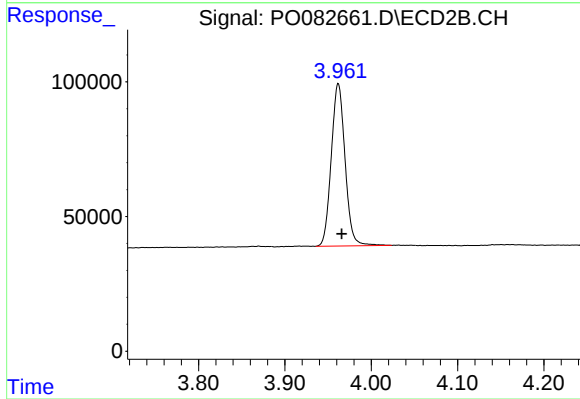


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: -0.004 min
Response: 668641
Conc: 21.61 ng/ml

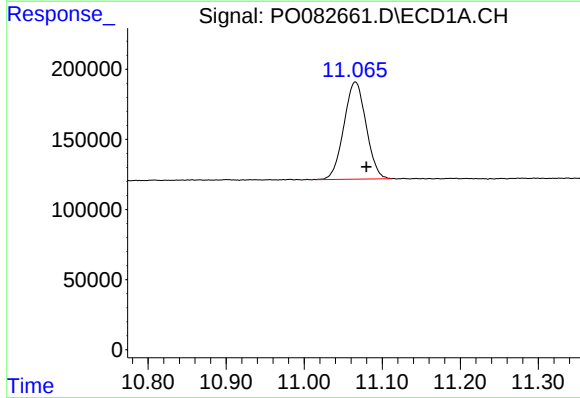

#2 Decachlorobiphenyl

R.T.: 11.065 min
Delta R.T.: -0.014 min
Response: 1371966
Conc: 21.72 ng/ml

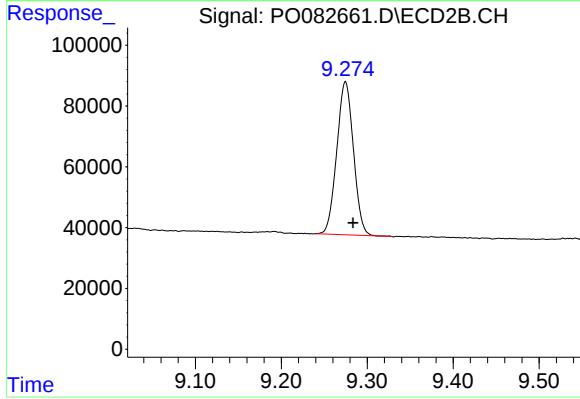

#2 Decachlorobiphenyl

R.T.: 9.275 min
Delta R.T.: -0.009 min
Response: 679006
Conc: 23.58 ng/ml