

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110921\
Data File : PO082665.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 11:18
Operator : AJ\MA
Sample : M4567-01
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BASEMENT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 13:54:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.963	1712161	639889	19.561	20.677
2) SA Decachlor...	11.067	9.274	2148590	1054541	34.023	36.626

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO110921\
Data File : PO082665.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 11:18
Operator : AJ\MA
Sample : M4567-01
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
BASEMENT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 13:54:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

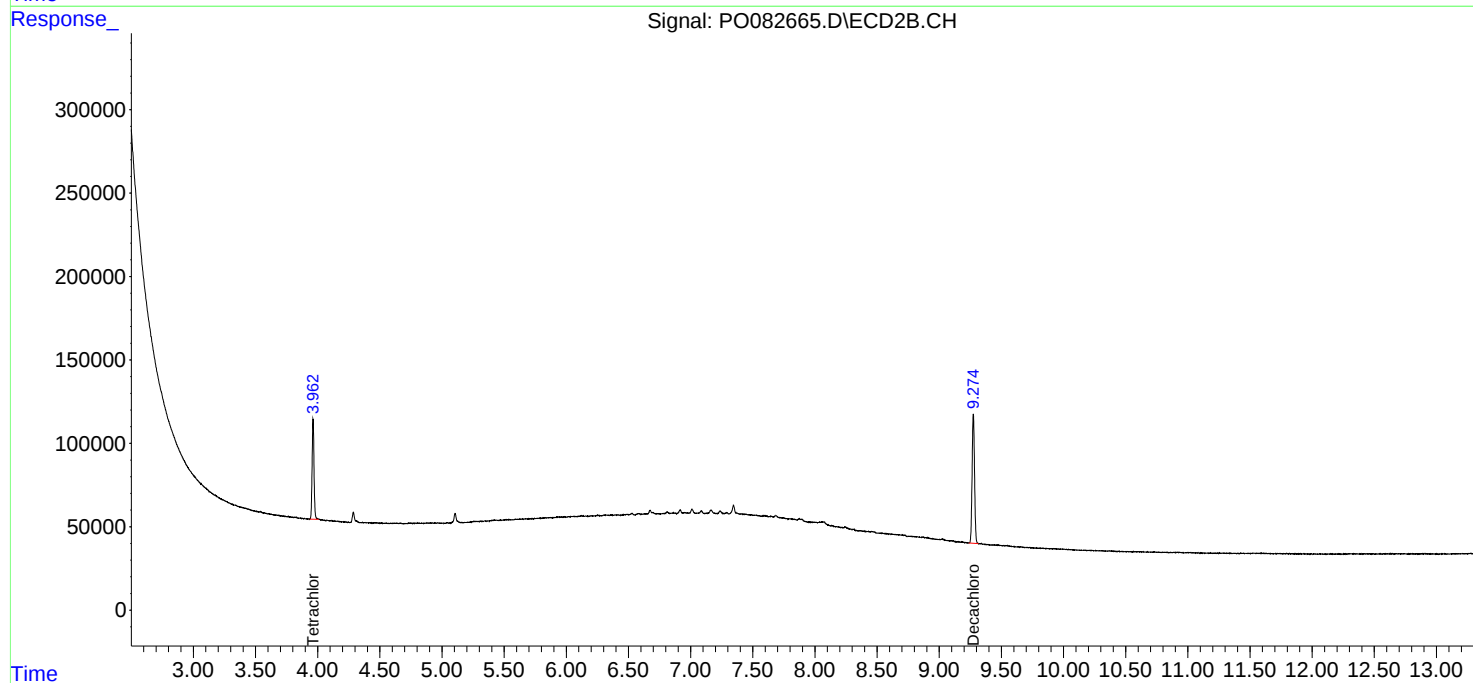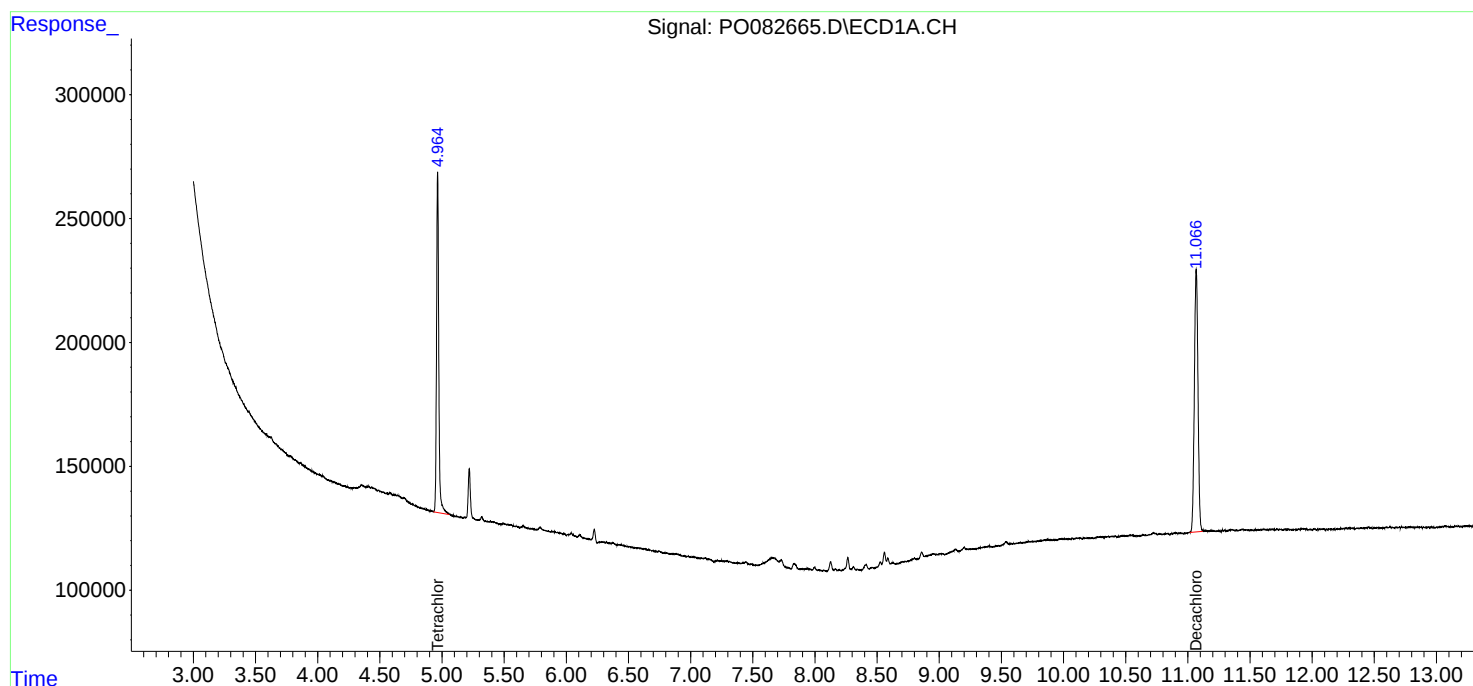


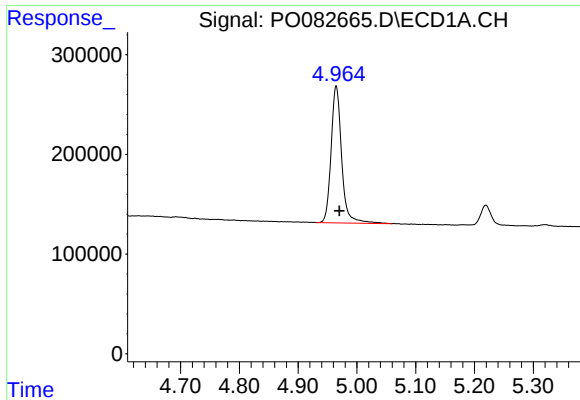

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: -0.005 min
Response: 1712161
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
BASEMENT

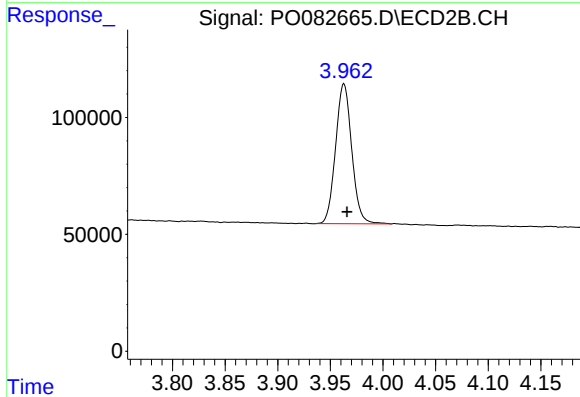


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 639889
Conc: 20.68 ng/ml

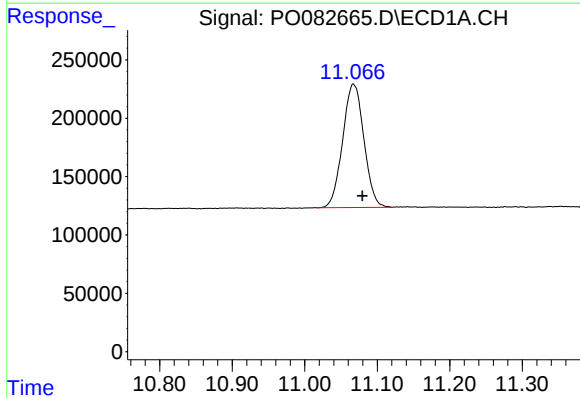

#2 Decachlorobiphenyl

R.T.: 11.067 min
Delta R.T.: -0.013 min
Response: 2148590
Conc: 34.02 ng/ml

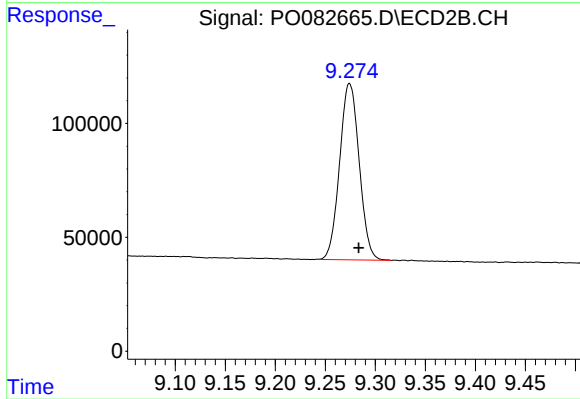

#2 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: -0.009 min
Response: 1054541
Conc: 36.63 ng/ml