

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110921\
 Data File : PO082666.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 11:35
 Operator : AJ\MA
 Sample : M4567-02
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PUMP-ROOM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 13:54:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.965	3.963	1664062	642966	19.012	20.776
2) SA Decachlor...	11.067	9.275	1597663	784727	25.299	27.255

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110921\
Data File : PO082666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 11:35
Operator : AJ\MA
Sample : M4567-02
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PUMP-ROOM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 13:54:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

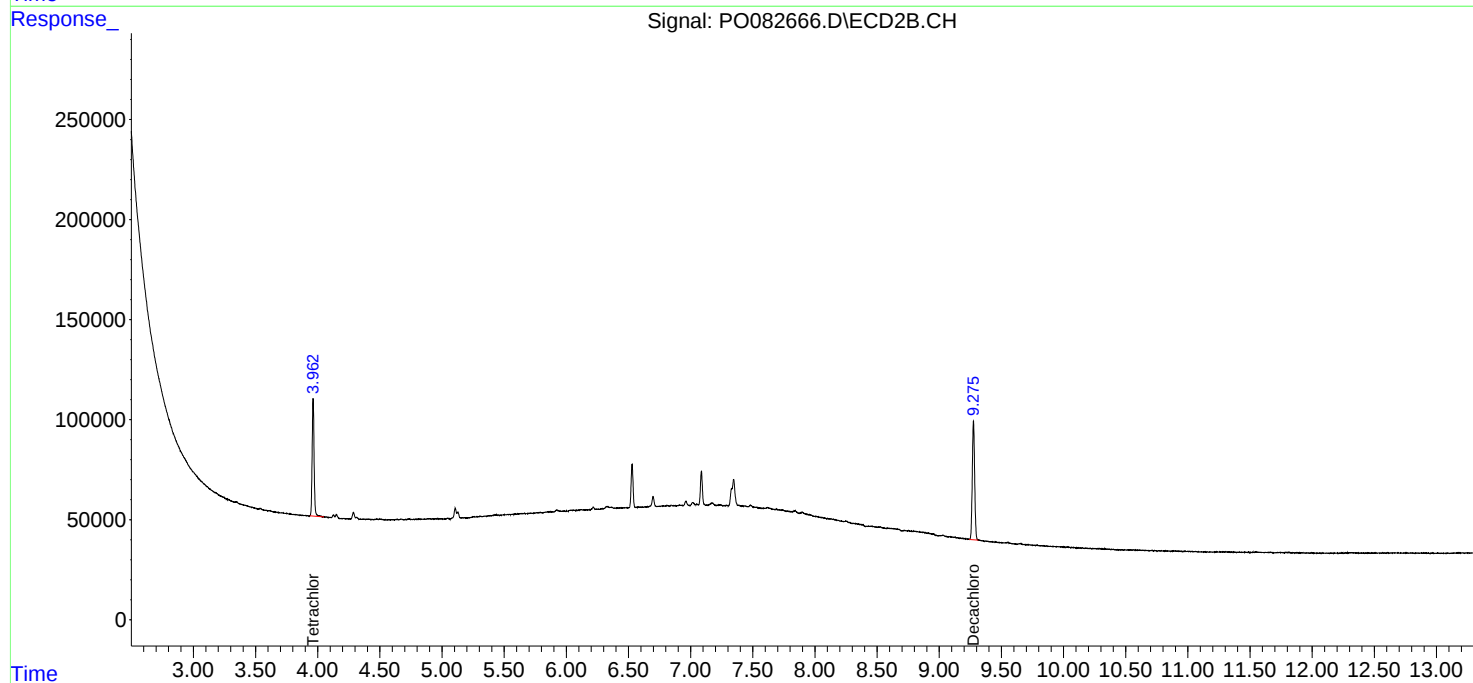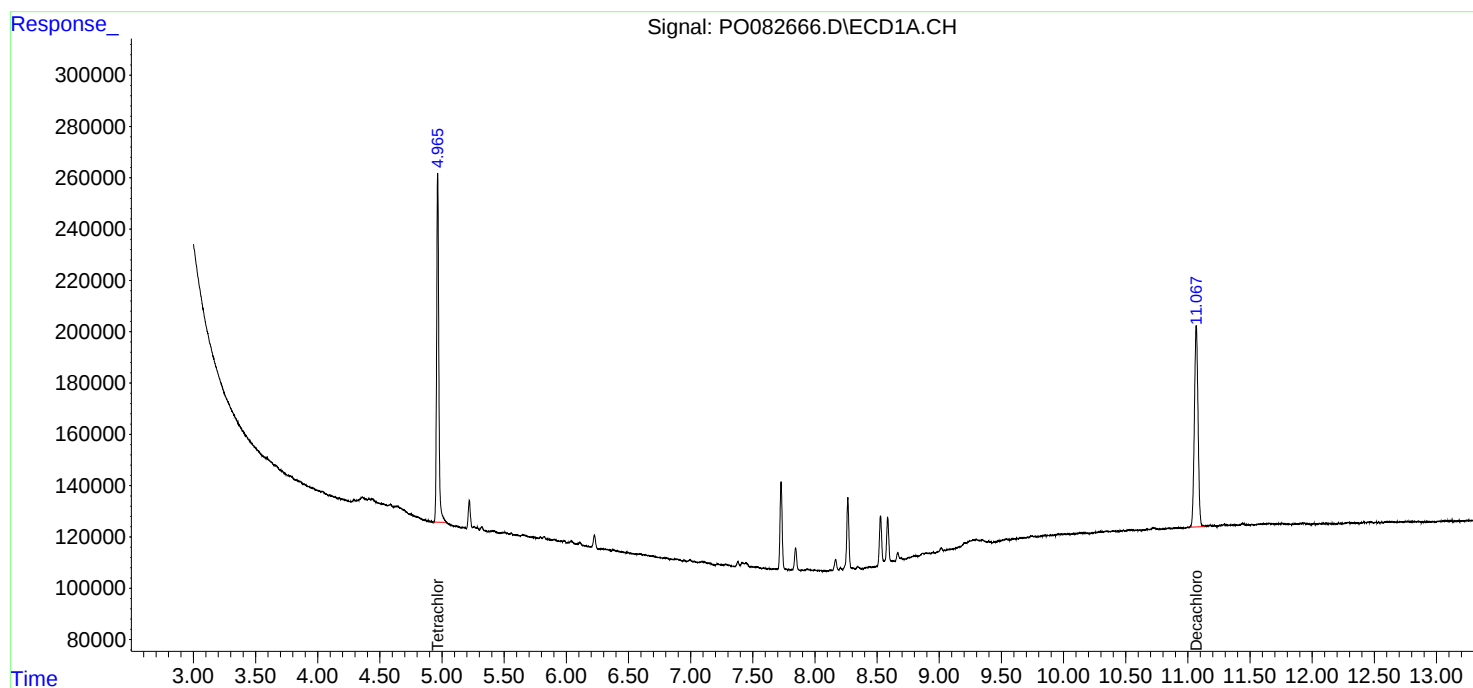


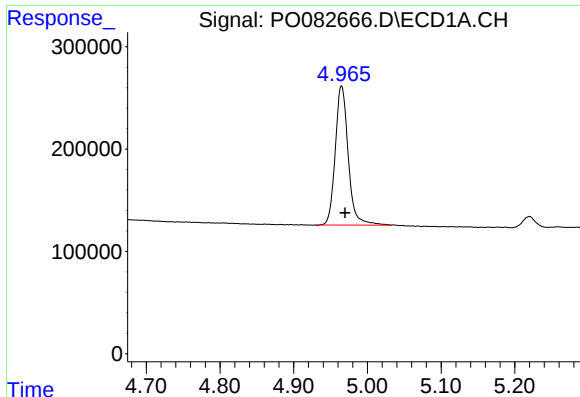

#1 Tetrachloro-m-xylene


R.T.: 4.965 min
Delta R.T.: -0.005 min
Response: 1664062
Conc: 19.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
PUMP-ROOM

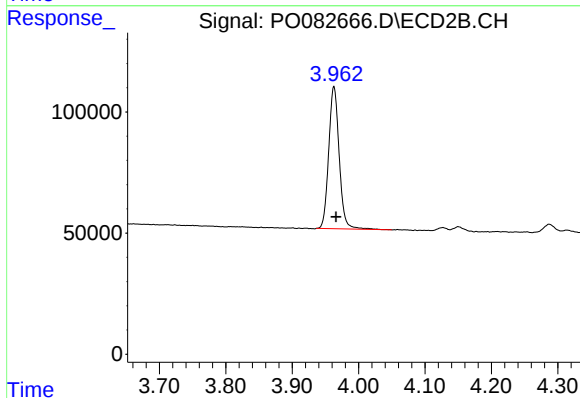


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 642966
Conc: 20.78 ng/ml

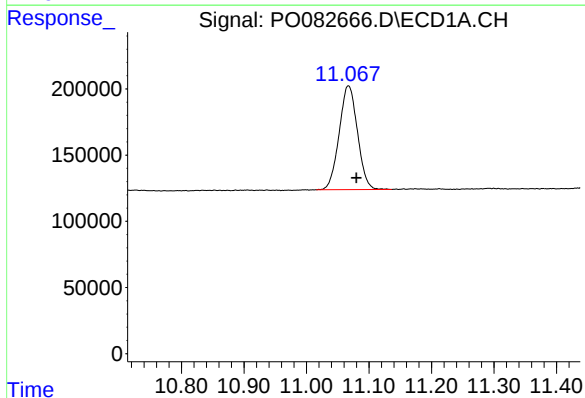

#2 Decachlorobiphenyl

R.T.: 11.067 min
Delta R.T.: -0.013 min
Response: 1597663
Conc: 25.30 ng/ml

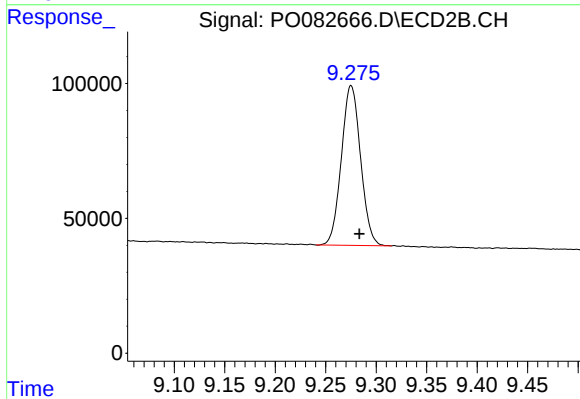

#2 Decachlorobiphenyl

R.T.: 9.275 min
Delta R.T.: -0.008 min
Response: 784727
Conc: 27.25 ng/ml