

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110921\
 Data File : PO082675.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2021 14:46
 Operator : AJ\MA
 Sample : PB140518BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB140518BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 17:46:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 03 05:20:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.968	3.963	1646308	626486	18.809	20.244
2)	SA Decachlor...	11.070	9.277	1280902	626686	20.283	21.766

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110921\
Data File : PO082675.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2021 14:46
Operator : AJ\MA
Sample : PB140518BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB140518BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 17:46:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

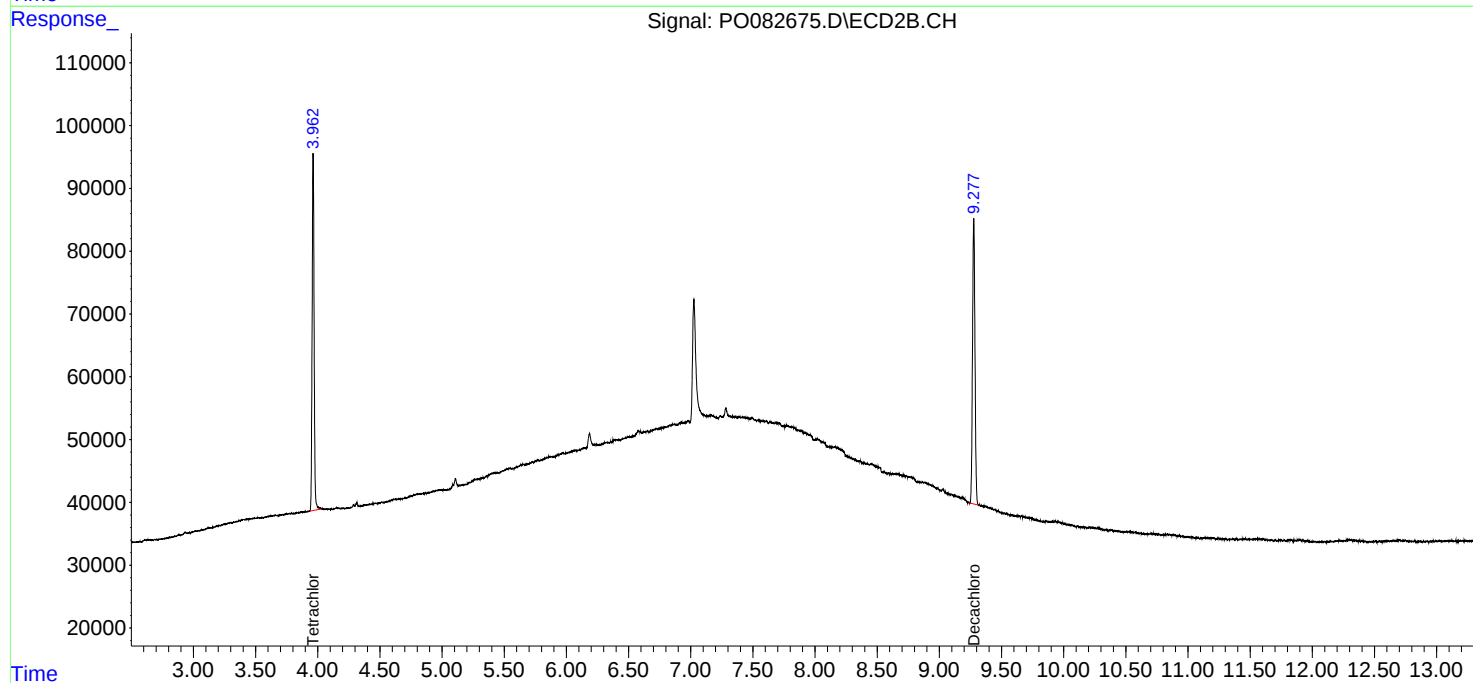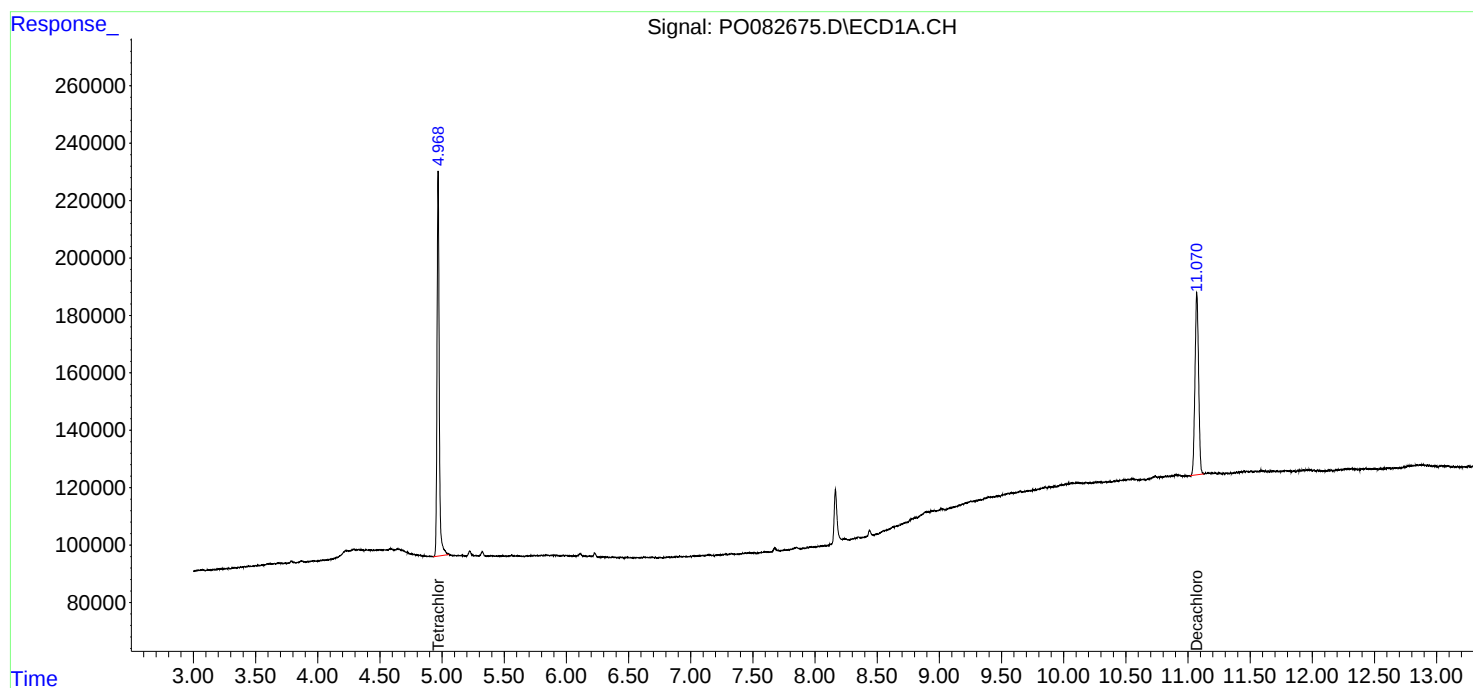


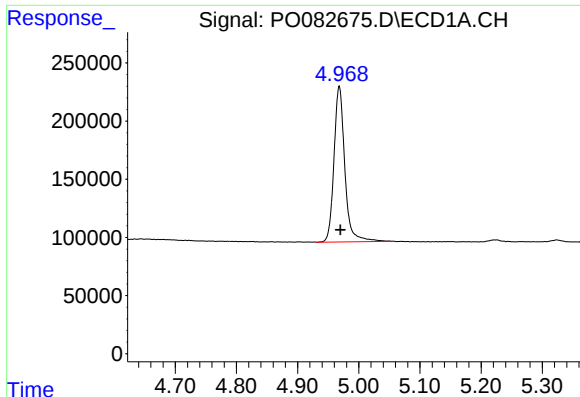

#1 Tetrachloro-m-xylene


R.T.: 4.968 min
Delta R.T.: -0.002 min
Response: 1646308
Conc: 18.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB140518BL

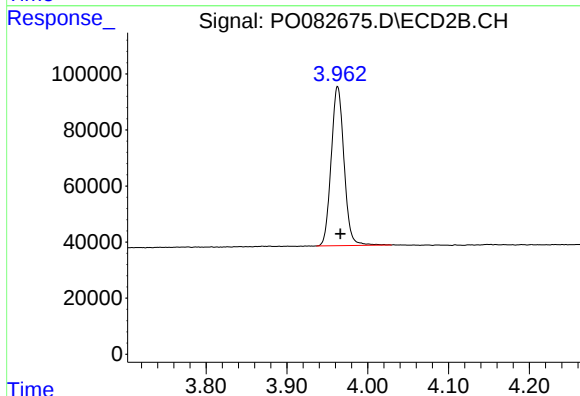


#1 Tetrachloro-m-xylene

R.T.: 3.963 min
Delta R.T.: -0.003 min
Response: 626486
Conc: 20.24 ng/ml

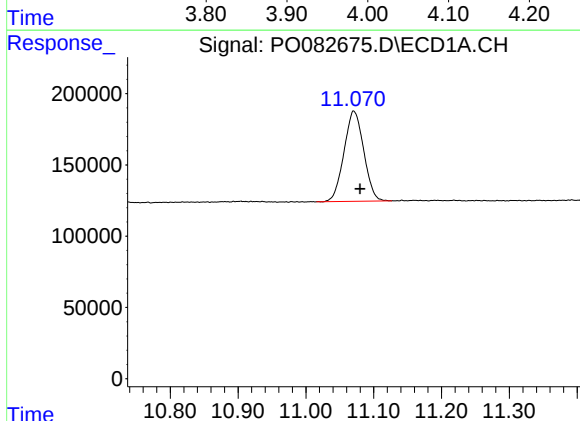

#2 Decachlorobiphenyl

R.T.: 11.070 min
Delta R.T.: -0.009 min
Response: 1280902
Conc: 20.28 ng/ml

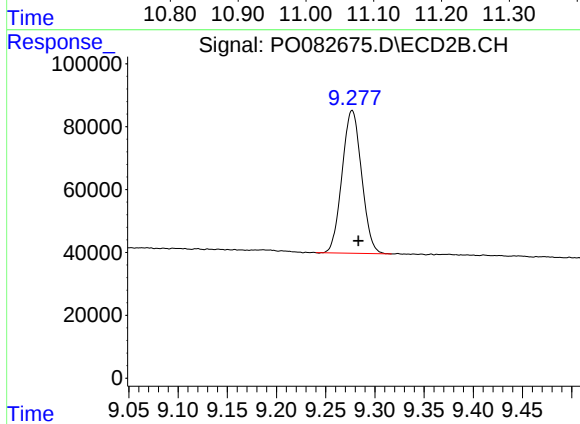

#2 Decachlorobiphenyl

R.T.: 9.277 min
Delta R.T.: -0.006 min
Response: 626686
Conc: 21.77 ng/ml