

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110922\
 Data File : PO090397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Nov 2022 23:24
 Operator : YP/AJ
 Sample : N5489-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 P-RB-20221102-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/10/2022
 Supervised By :Ankita Jodhani 11/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 03:29:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.301	3.479	6315397	2106338	1.965	1.982m
2) SA Decachlor...	10.045	8.481	5210056	2497728	2.126	2.425

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110922\
Data File : PO090397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Nov 2022 23:24
Operator : YP/AJ
Sample : N5489-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P-RB-20221102-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2022
Supervised By :Ankita Jodhani 11/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 03:29:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

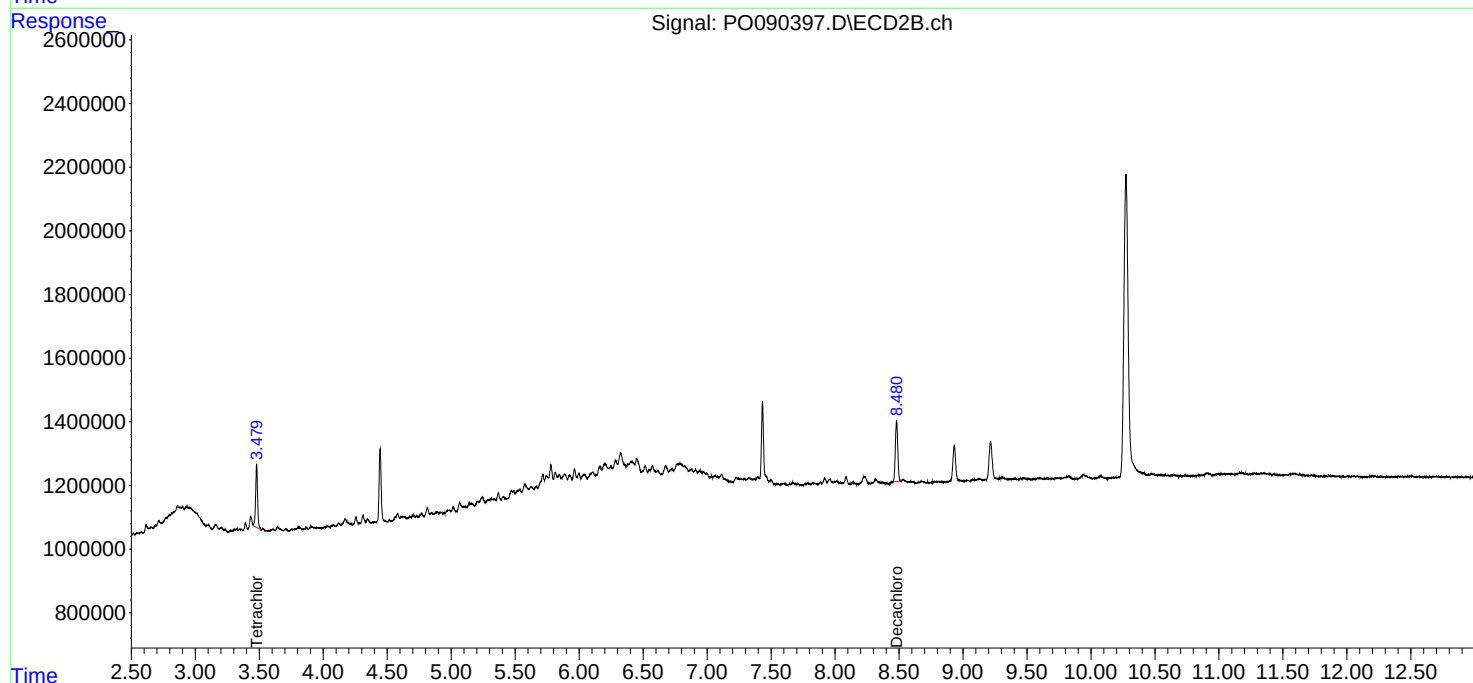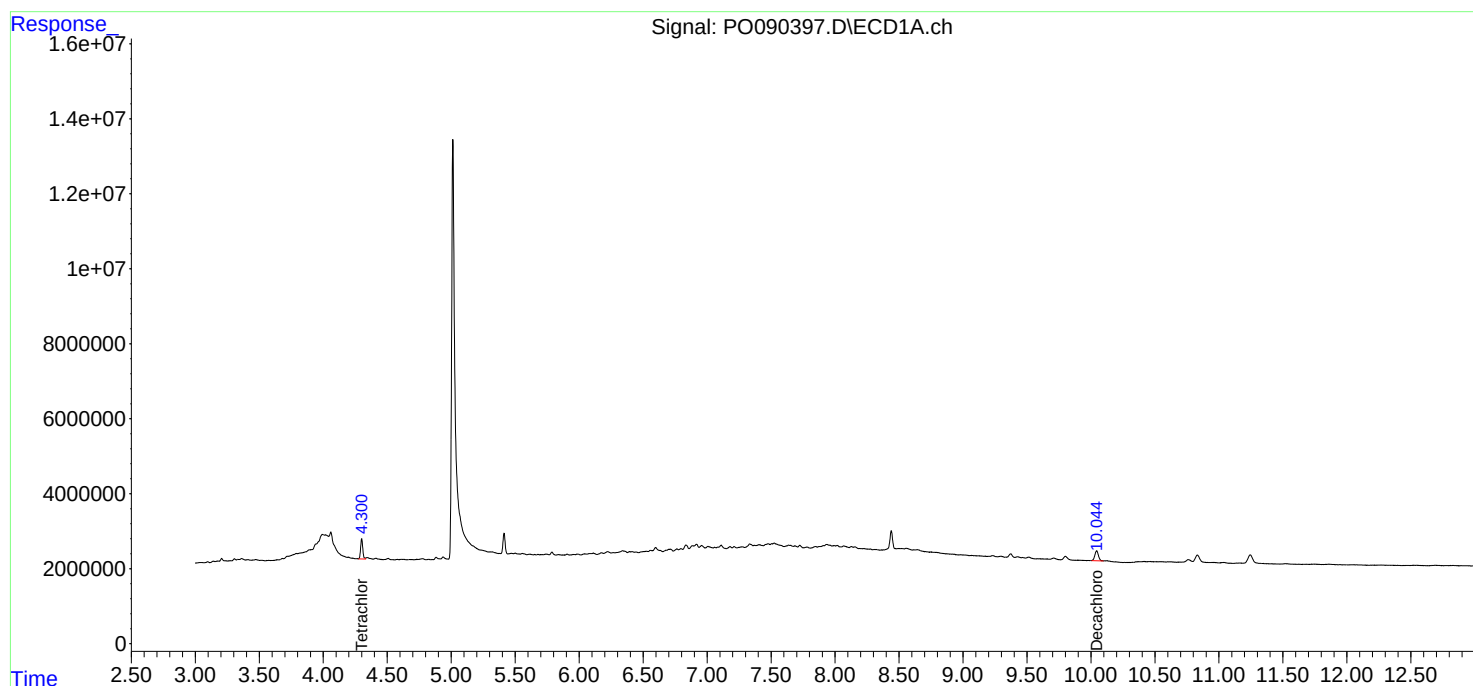

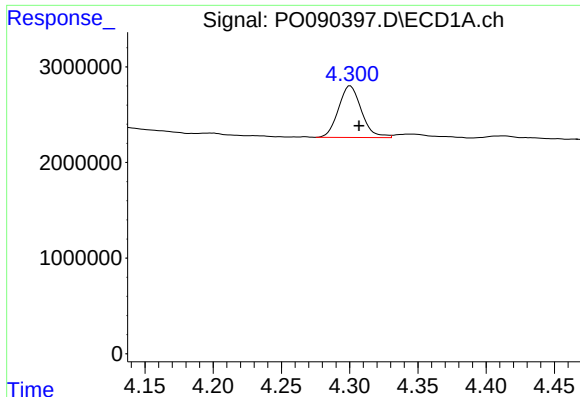


#1 Tetrachloro-m-xylene

R.T.: 4.301 min
Delta R.T.: -0.006 min
Response: 6315397
Conc: 1.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
P-RB-20221102-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/10/2022
Supervised By :Ankita Jodhani 11/10/2022

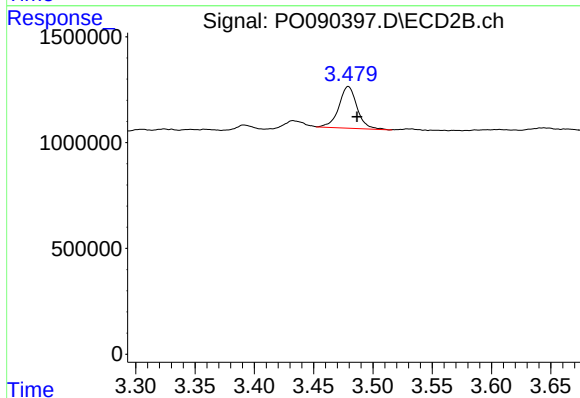


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: -0.008 min
Response: 2106338
Conc: 1.98 ng/ml m

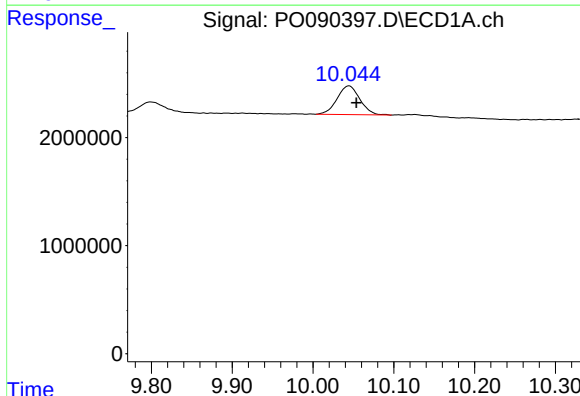

#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.009 min
Response: 5210056
Conc: 2.13 ng/ml

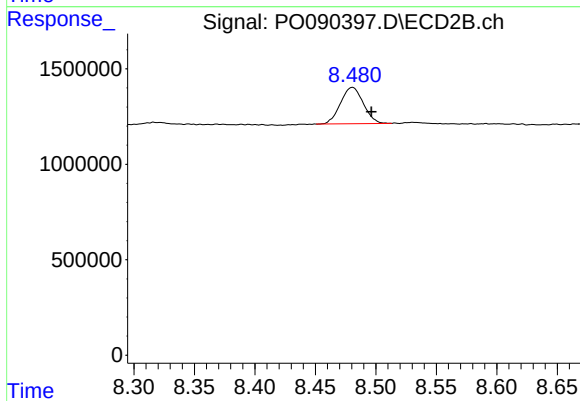

#2 Decachlorobiphenyl

R.T.: 8.481 min
Delta R.T.: -0.016 min
Response: 2497728
Conc: 2.43 ng/ml