

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110923\
 Data File : PO099564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2023 09:06
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 09:57:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 10 09:43:08 2023
 Response via : Initial Calibration
 Integrator: ChemStation

11/13/2023
 Supervised By :Ankita
 Jodhani

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	11/13/2023

System Monitoring Compounds							
1) SA Tetrachlo...	4.492	3.723	8426421	6231408	4.852	5.017	
2) SA Decachlor...	10.377	8.837	2798313	3207363	4.465	4.408	
Target Compounds							
26) L6 AR-1254-1	6.544	5.648	2278954	1767771	50.640	48.599	
27) L6 AR-1254-2	6.766	5.796	3075537	1569732	48.770	48.322	
28) L6 AR-1254-3	7.136	6.206	2679314	2700528	46.001	49.804	
29) L6 AR-1254-4	7.425	6.436	1581778	1350980	46.664m	47.972	
30) L6 AR-1254-5	7.849	6.860	1803305	2374157	46.087	48.726	

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110923\
Data File : PO099564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2023 09:06
Operator : YP/AJ
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050



Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 09:57:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 10 09:43:08 2023
Response via : Initial Calibration
Integrator: ChemStation

11/13/2023
Supervised By :Ankita
Jodhani

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

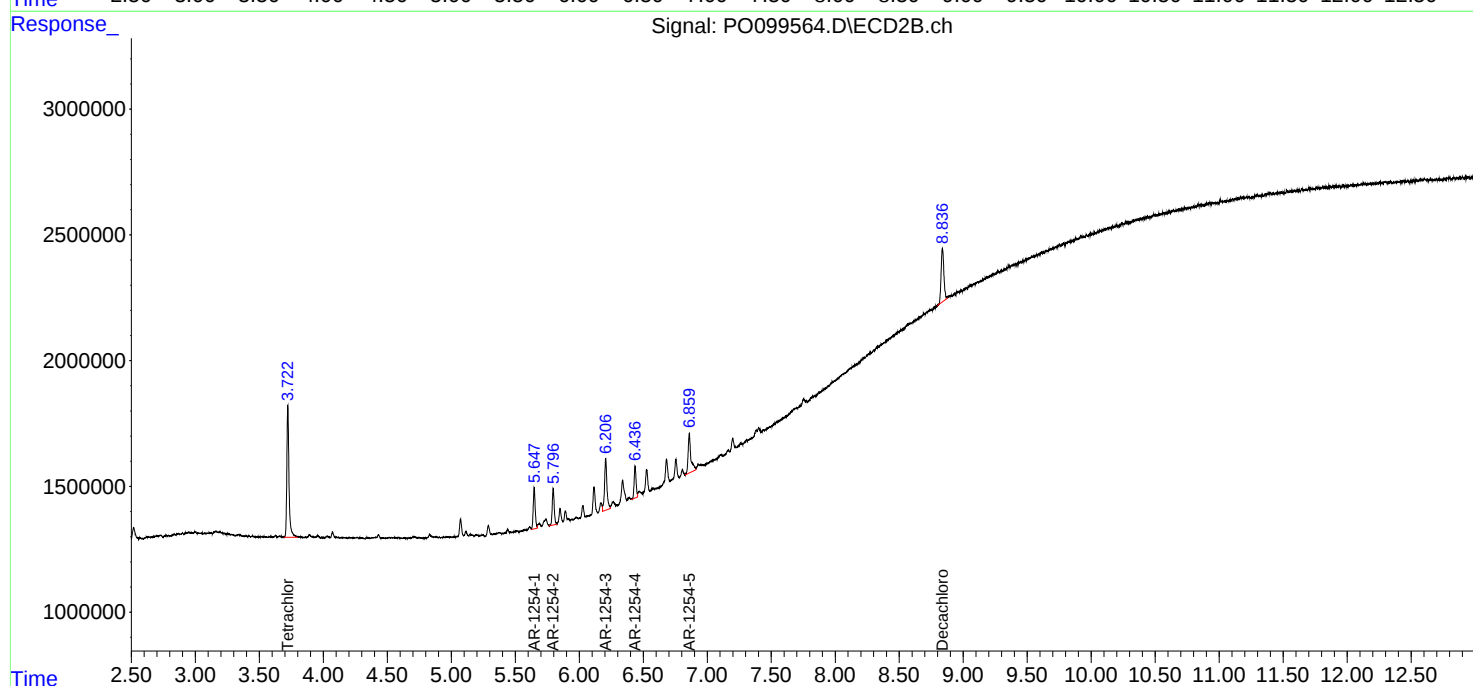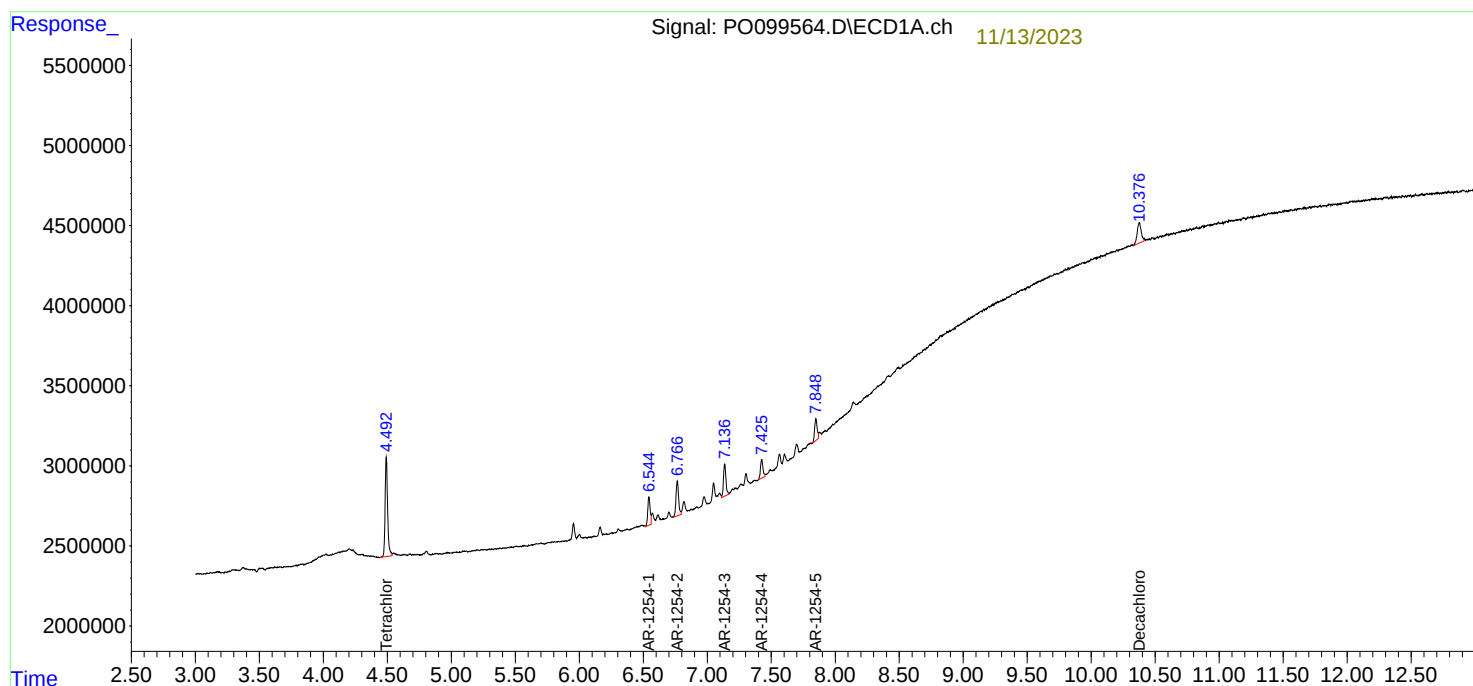

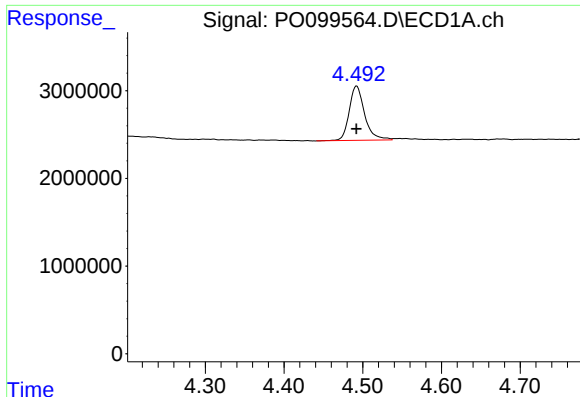


#1 Tetrachloro-m-xylene

R.T.: 4.492 min
Delta R.T.: 0.000 min
Response: 8426421
Conc: 4.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICCO50

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

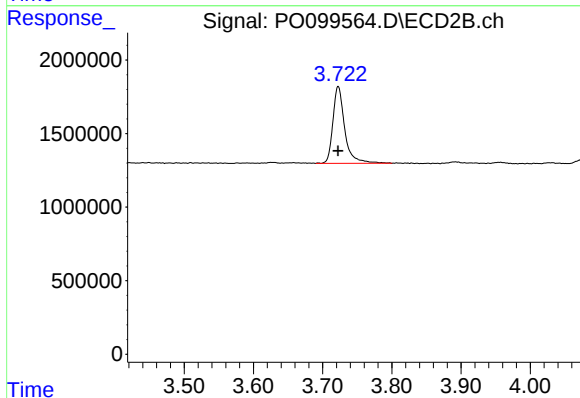


#1 Tetrachloro-m-xylene

R.T.: 3.723 min
Delta R.T.: 0.000 min
Response: 6231408
Conc: 5.02 ng/ml


11/13/2023
Supervised By :Ankita
Jodhani

11/13/2023

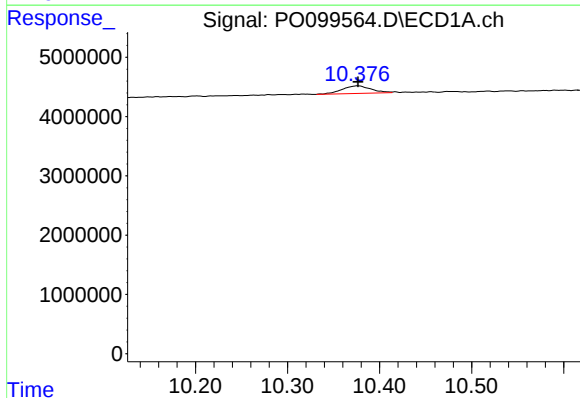


#2 Decachlorobiphenyl

R.T.: 10.377 min
Delta R.T.: 0.000 min
Response: 2798313
Conc: 4.46 ng/ml

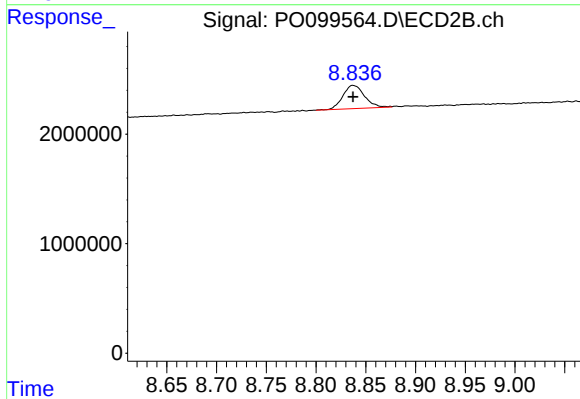

#2 Decachlorobiphenyl

R.T.: 8.837 min
Delta R.T.: 0.000 min
Response: 3207363
Conc: 4.41 ng/ml

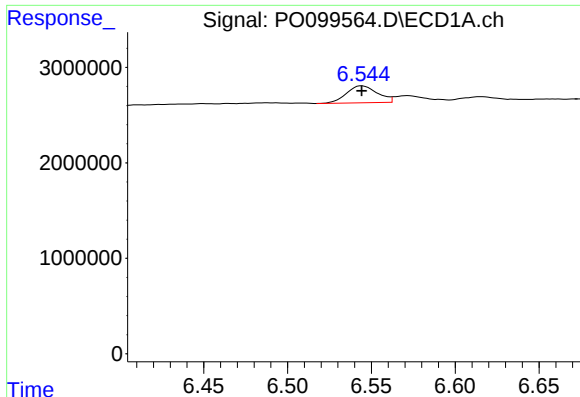


#26 AR-1254-1

R.T.: 6.544 min
Delta R.T.: 0.000 min
Response: 2278954
Conc: 50.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254\ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

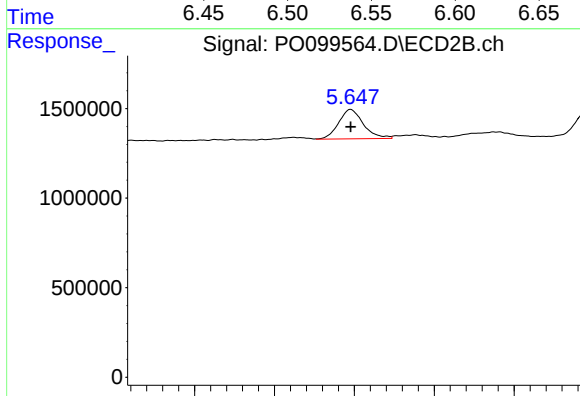


#26 AR-1254-1

R.T.: 5.648 min
Delta R.T.: 0.000 min
Response: 1767771
Conc: 48.60 ng/ml


11/13/2023
Supervised By :Ankita
Jodhani

11/13/2023

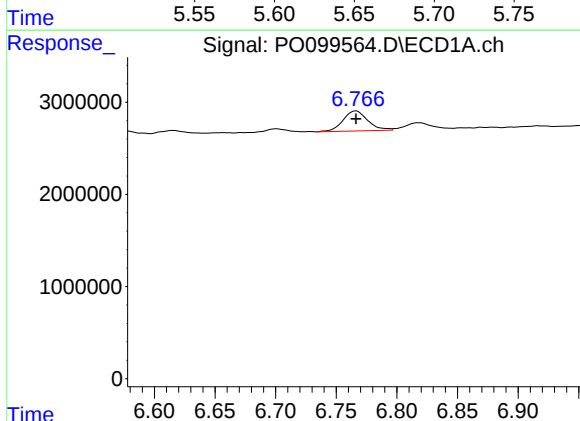


#27 AR-1254-2

R.T.: 6.766 min
Delta R.T.: 0.000 min
Response: 3075537
Conc: 48.77 ng/ml

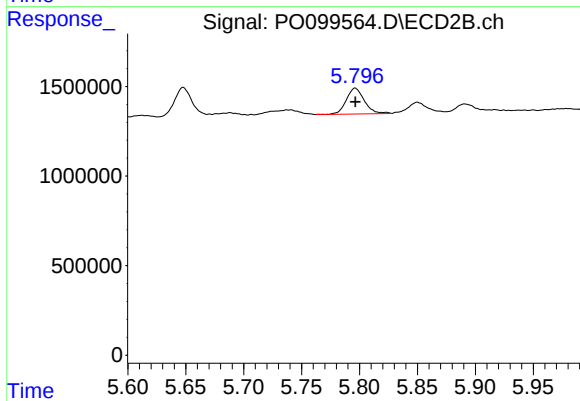

#27 AR-1254-2

R.T.: 5.796 min
Delta R.T.: 0.000 min
Response: 1569732
Conc: 48.32 ng/ml

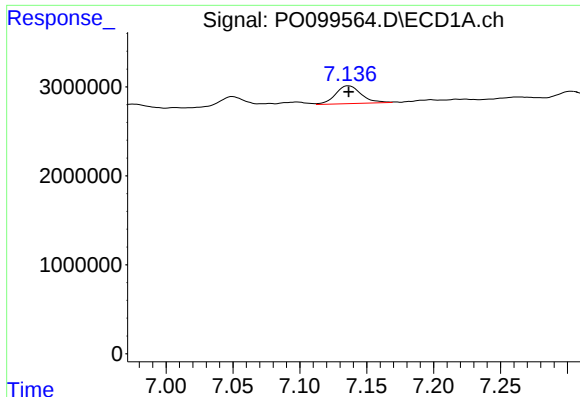


#28 AR-1254-3

R.T.: 7.136 min
Delta R.T.: 0.000 min
Response: 2679314
Conc: 46.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254\ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

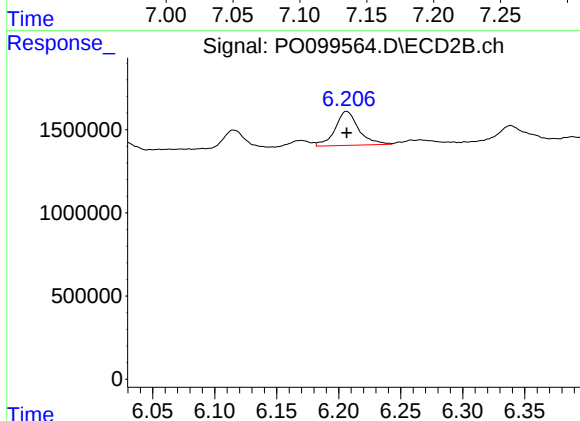


#28 AR-1254-3

R.T.: 6.206 min
Delta R.T.: 0.000 min
Response: 2700528
Conc: 49.80 ng/ml


11/13/2023
Supervised By :Ankita
Jodhani

11/13/2023

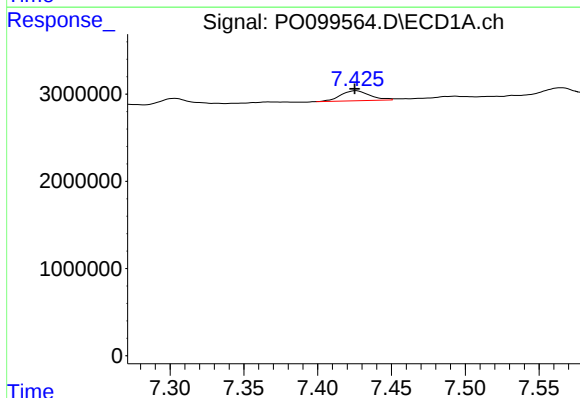


#29 AR-1254-4

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 1581778
Conc: 46.66 ng/ml m

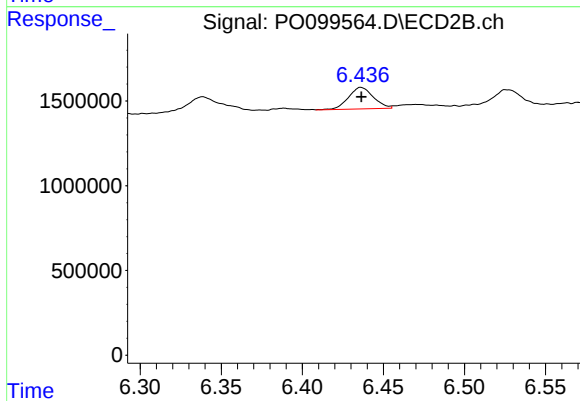

#29 AR-1254-4

R.T.: 6.436 min
Delta R.T.: 0.000 min
Response: 1350980
Conc: 47.97 ng/ml

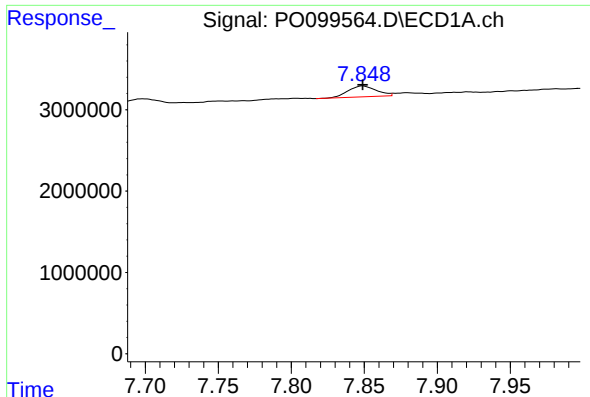


#30 AR-1254-5

R.T.: 7.849 min
Delta R.T.: 0.000 min
Response: 1803305
Conc: 46.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254\ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

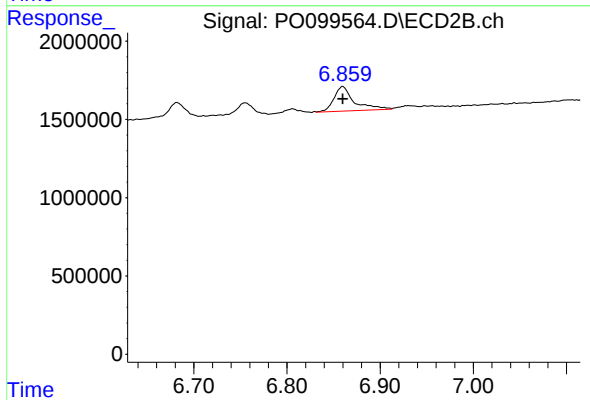

#30 AR-1254-5

R.T.: 6.860 min
Delta R.T.: 0.000 min
Response: 2374157
Conc: 48.73 ng/ml

11/13/2023
Supervised By :Ankita
Jodhani

11/13/2023