

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111018\
Data File : PO051322.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 9:47
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:26:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.334	10119147	4820614	17.949	21.604
2) SA Decachlor...	9.972	8.067	7437113	3906424	20.043	17.625

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111018\
Data File : PO051322.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 9:47
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:26:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

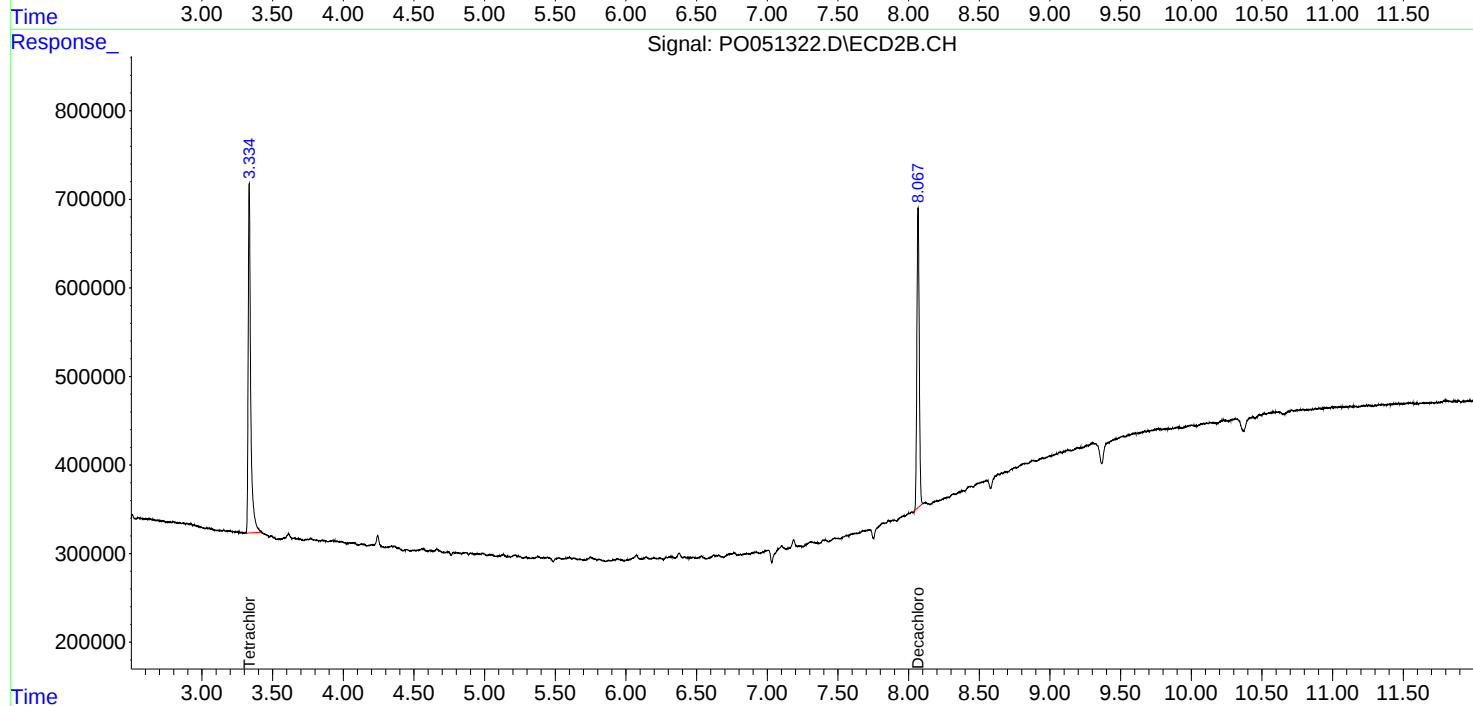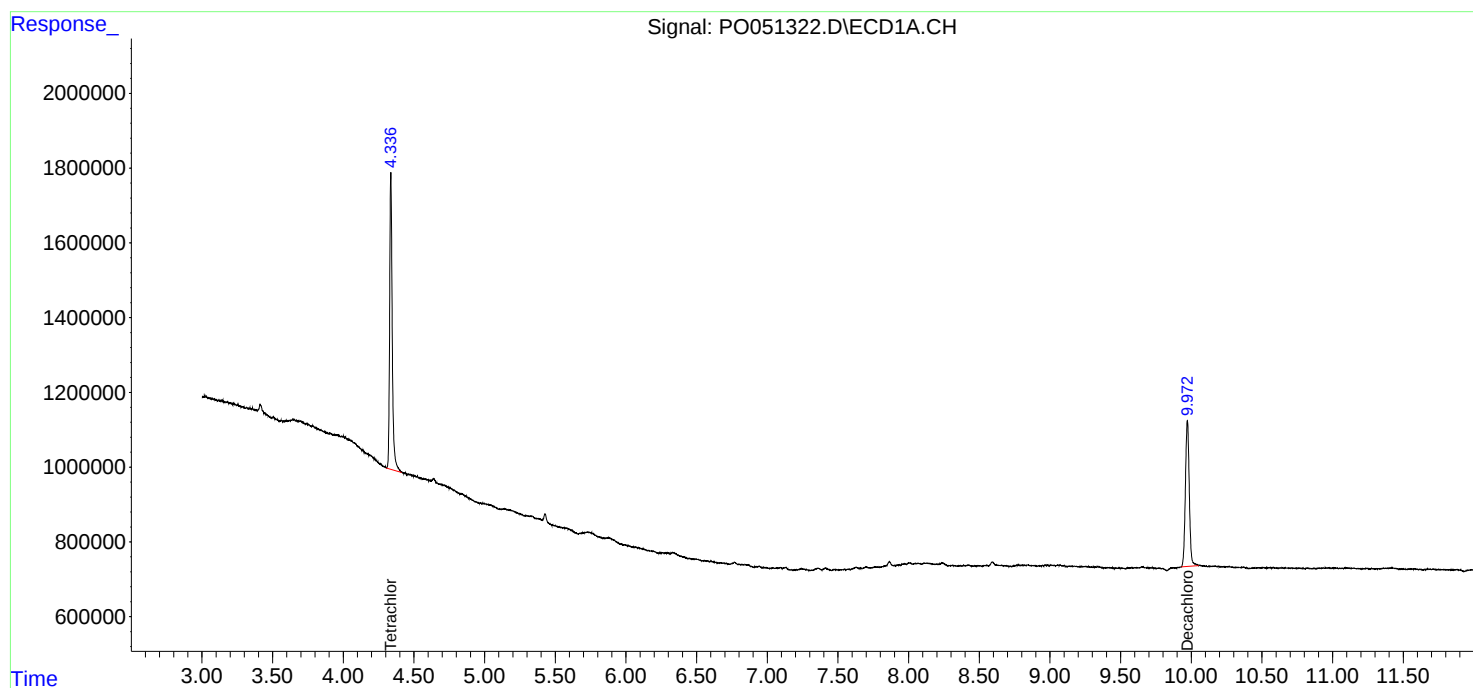


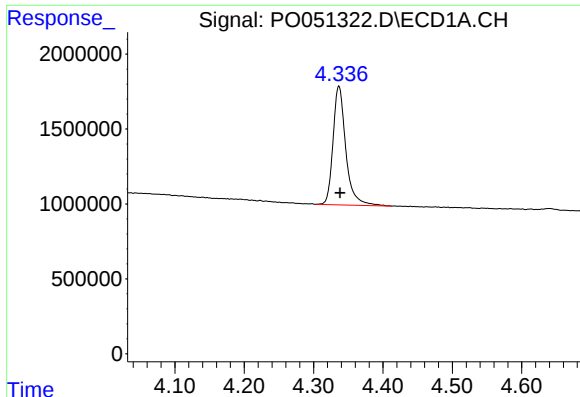

#1 Tetrachloro-m-xylene


R.T.: 4.337 min
Delta R.T.: -0.001 min
Response: 10119147
Conc: 17.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

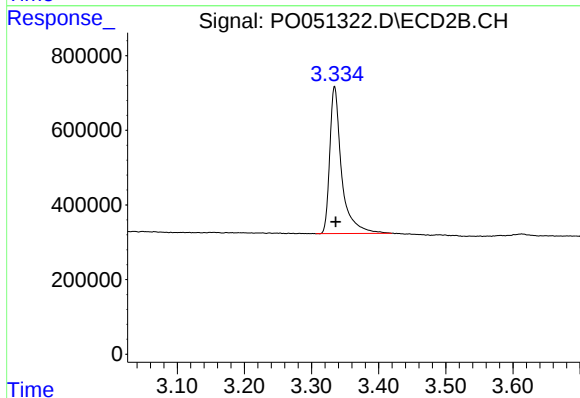


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: -0.002 min
Response: 4820614
Conc: 21.60 ng/ml

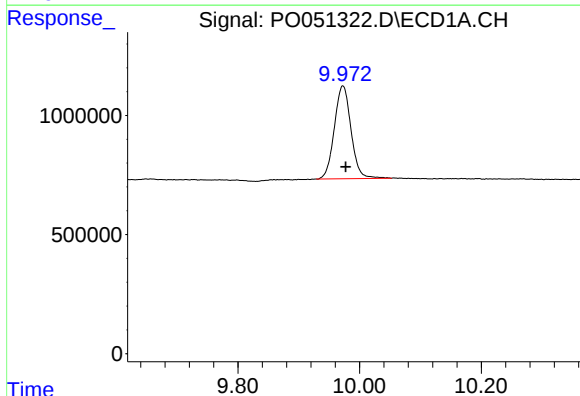

#2 Decachlorobiphenyl

R.T.: 9.972 min
Delta R.T.: -0.005 min
Response: 7437113
Conc: 20.04 ng/ml

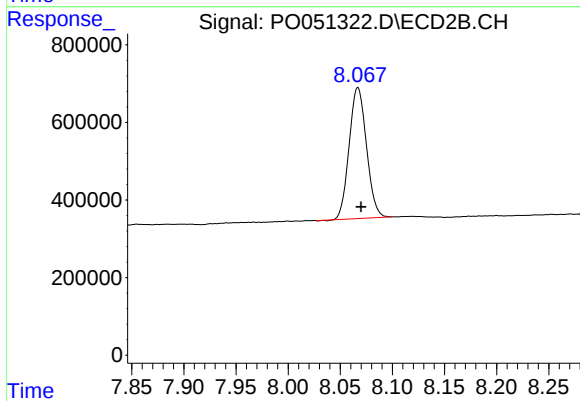

#2 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: -0.003 min
Response: 3906424
Conc: 17.62 ng/ml