

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111018\
 Data File : PO051324.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Nov 2018 11:05
 Operator : SM/SJ
 Sample : J5805-05RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-SAMPLES(21-25)RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 09 11:27:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 08 14:50:13 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.335	8225006	3485002	14.589	15.618
2) SA Decachlor...	9.975	8.068	3869317	1773974	10.428	8.004

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111018\
Data File : PO051324.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Nov 2018 11:05
Operator : SM/SJ
Sample : J5805-05RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLES(21-25)RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 09 11:27:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 08 14:50:13 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

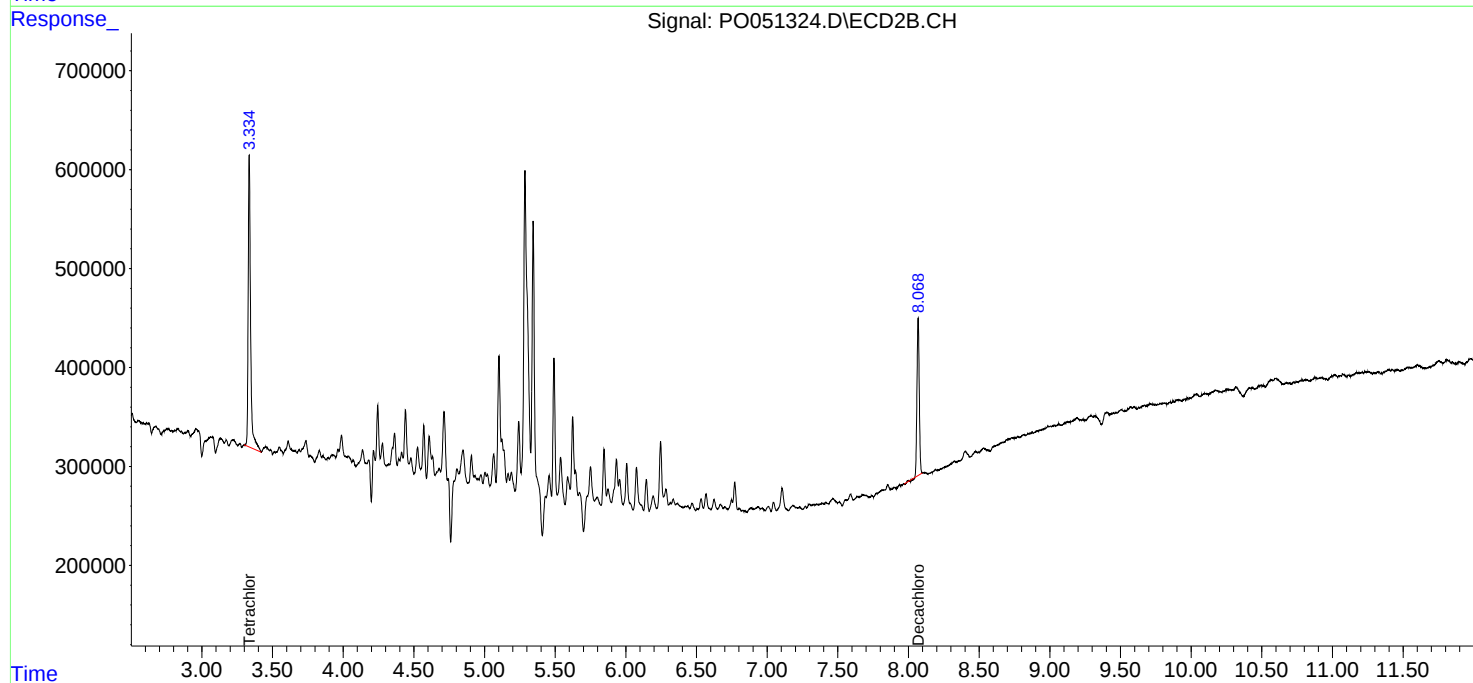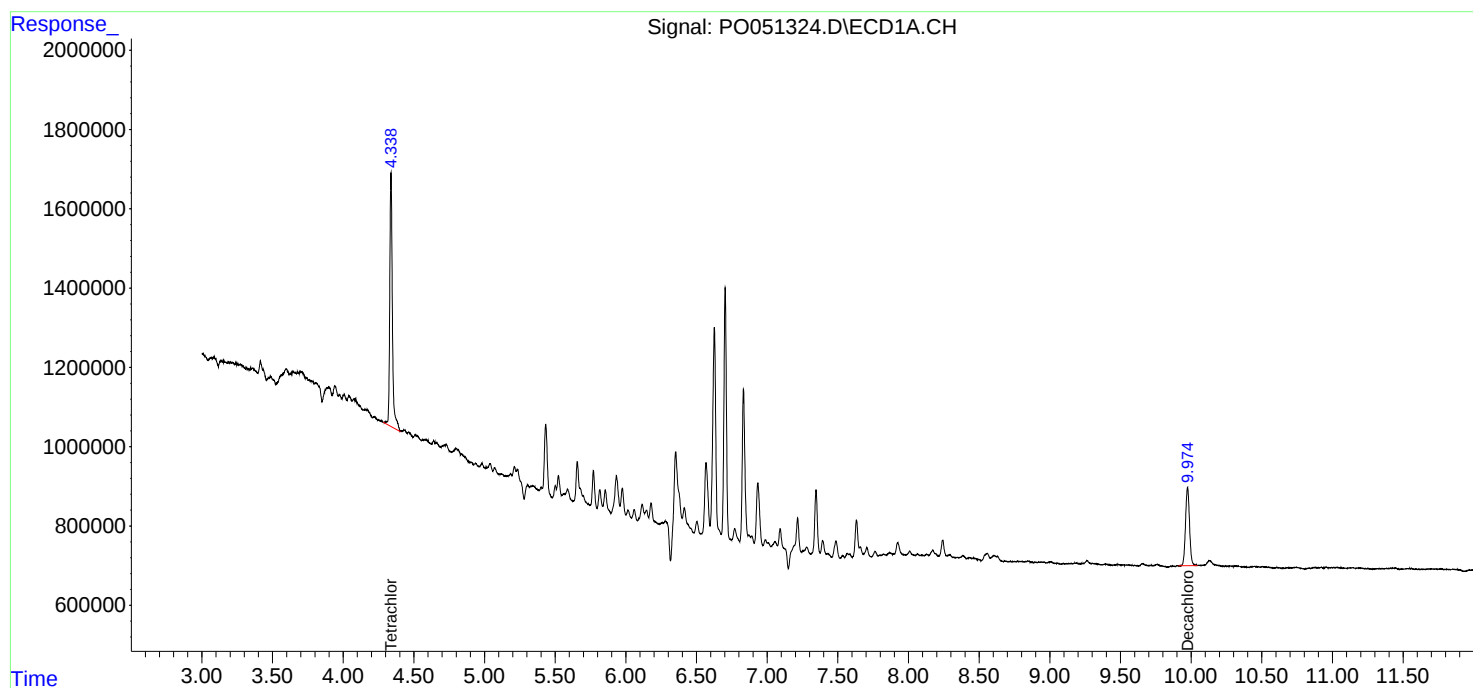


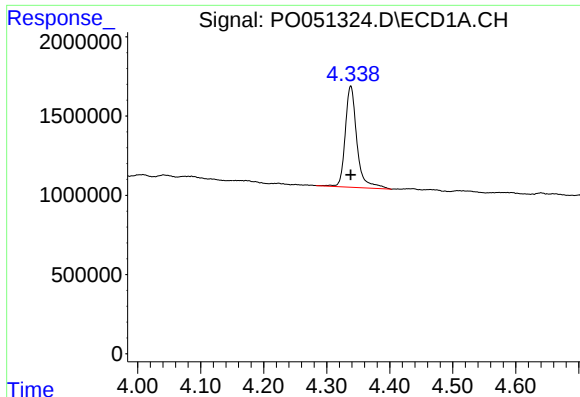

#1 Tetrachloro-m-xylene


R.T.: 4.338 min
Delta R.T.: 0.000 min
Response: 8225006
Conc: 14.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLES(21-25)RE

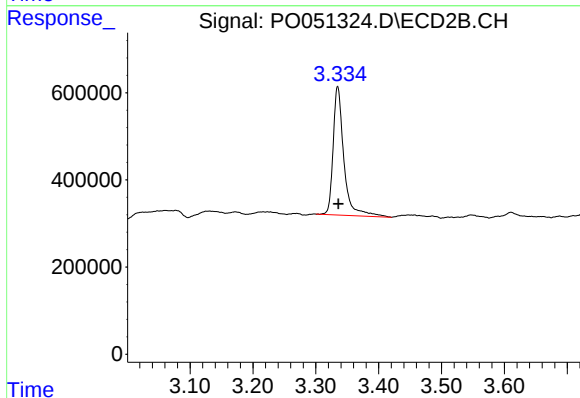


#1 Tetrachloro-m-xylene

R.T.: 3.335 min
Delta R.T.: -0.001 min
Response: 3485002
Conc: 15.62 ng/ml

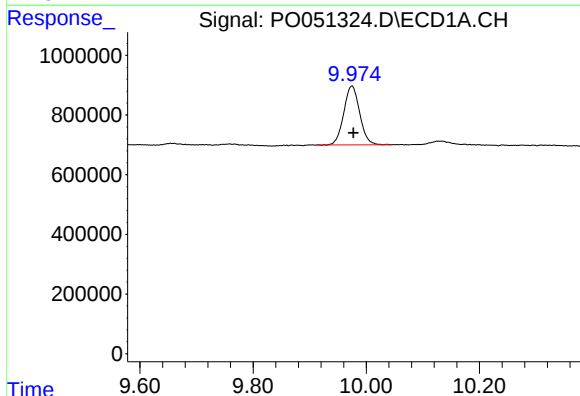

#2 Decachlorobiphenyl

R.T.: 9.975 min
Delta R.T.: -0.003 min
Response: 3869317
Conc: 10.43 ng/ml

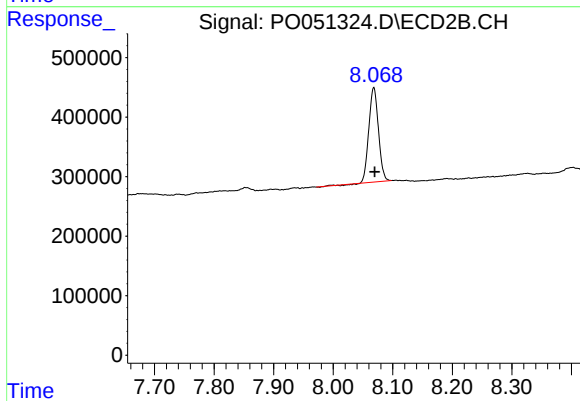

#2 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: -0.002 min
Response: 1773974
Conc: 8.00 ng/ml