

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111020\
 Data File : PO073195.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Nov 2020 10:37
 Operator : DD\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Ankita
 11/11/2020 9:00:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 11:09:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 10 10:22:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.945	4.018	300532	197066	5.463	5.578
2) SA Decachlor...	10.974	9.292	483579	343392	6.096	6.036
Target Compounds						
41) L9 AR-1268-1	9.464	8.212	336342	301245	49.245	59.406
42) L9 AR-1268-2	9.559	8.276	373704	256914	57.111m	57.682
43) L9 AR-1268-3	9.786	8.484	349122	233109	60.339	59.865
44) L9 AR-1268-4	10.226	8.769	98851	99429	46.257	59.630 #
45) L9 AR-1268-5	10.638	9.049	1022108	693961	59.383	57.305

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111020\
Data File : PO073195.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2020 10:37
Operator : DD\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
11/11/2020 9:00:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 11:09:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 10 10:22:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

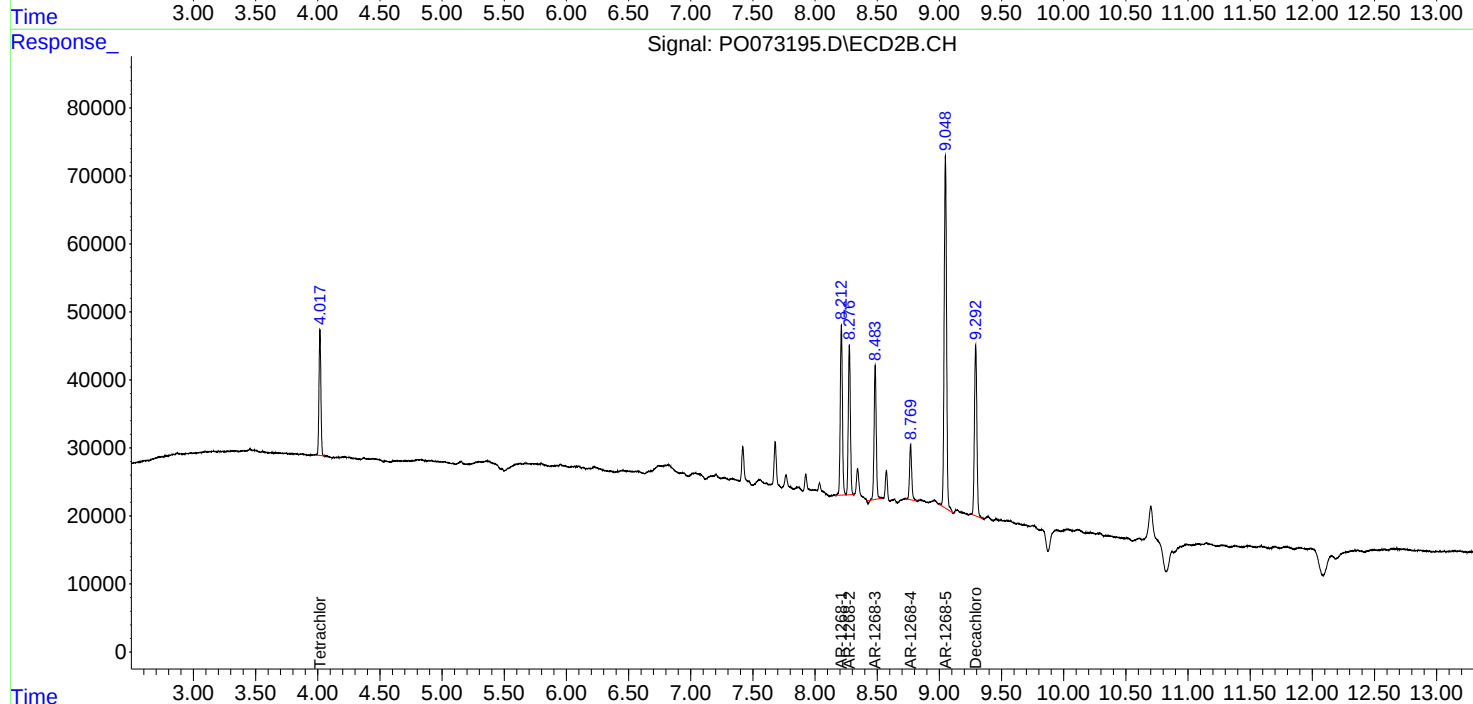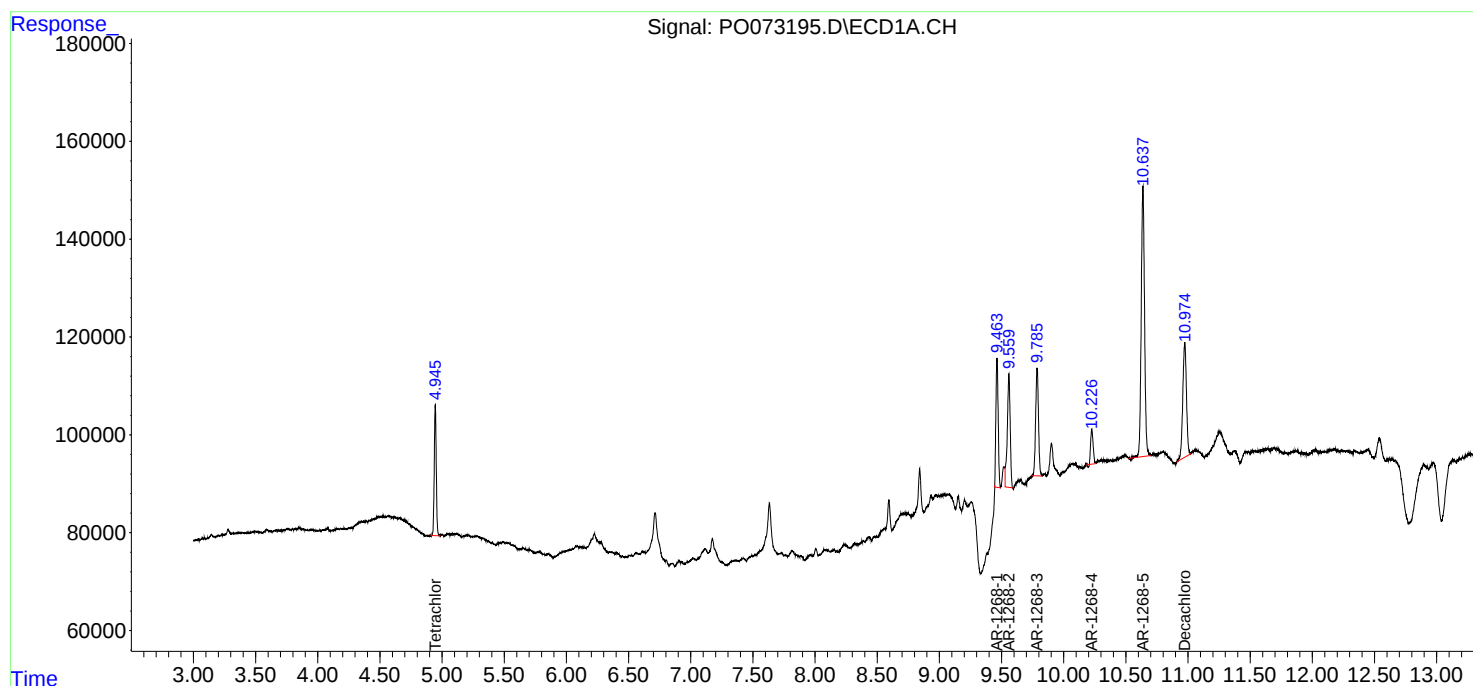

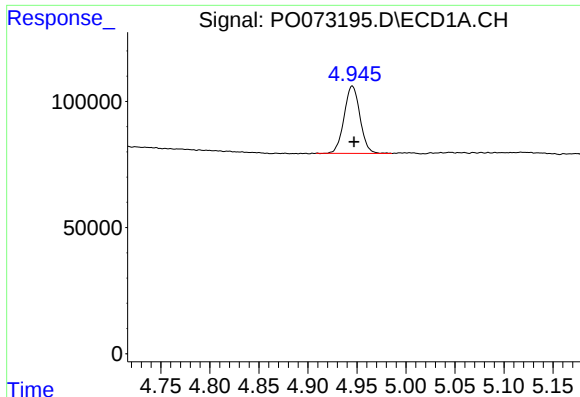


#1 Tetrachloro-m-xylene

R.T.: 4.945 min
Delta R.T.: -0.002 min
Response: 300532
Conc: 5.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
11/11/2020 9:00:28 AM

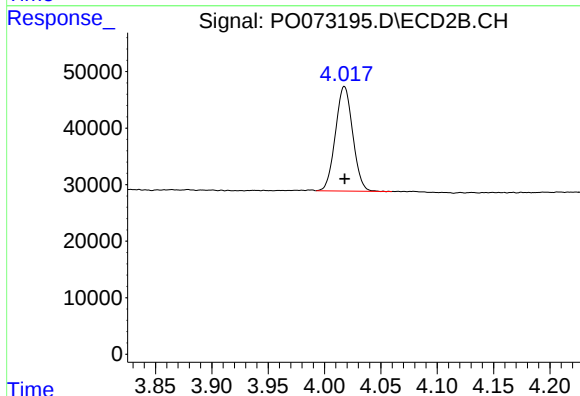


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: 0.000 min
Response: 197066
Conc: 5.58 ng/ml

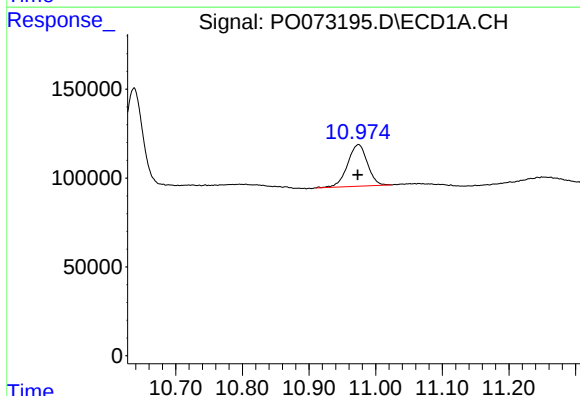


#2 Decachlorobiphenyl

R.T.: 10.974 min
Delta R.T.: 0.001 min
Response: 483579
Conc: 6.10 ng/ml

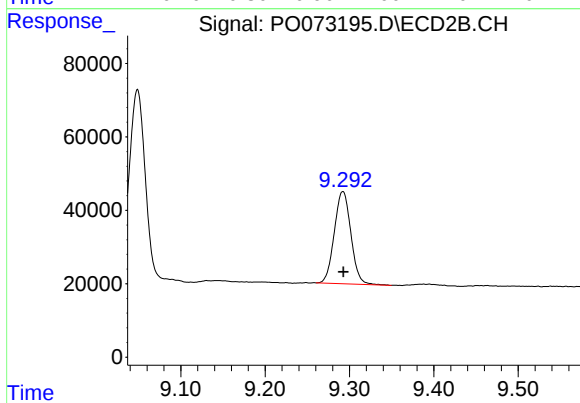

#2 Decachlorobiphenyl

R.T.: 9.292 min
Delta R.T.: 0.000 min
Response: 343392
Conc: 6.04 ng/ml

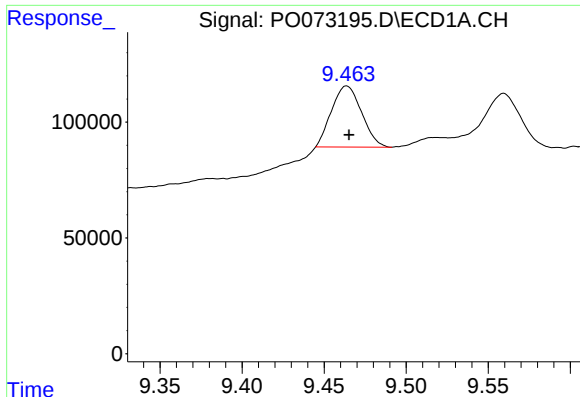


#41 AR-1268-1

R.T.: 9.464 min
Delta R.T.: -0.001 min
Response: 336342
Conc: 49.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
11/11/2020 9:00:28 AM

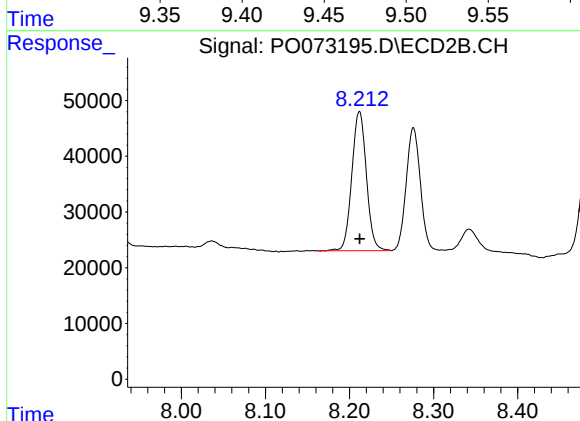


#41 AR-1268-1

R.T.: 8.212 min
Delta R.T.: 0.000 min
Response: 301245
Conc: 59.41 ng/ml

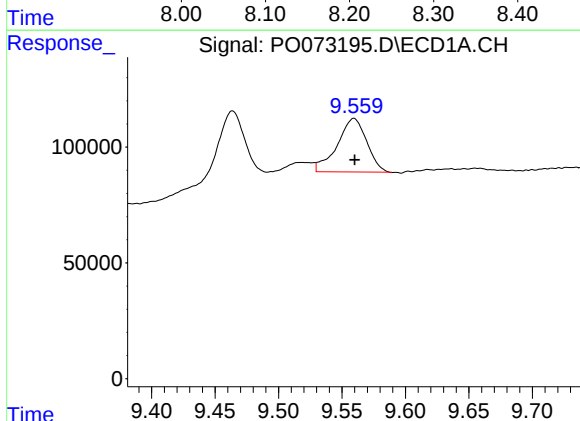


#42 AR-1268-2

R.T.: 9.559 min
Delta R.T.: 0.000 min
Response: 373704
Conc: 57.11 ng/ml m

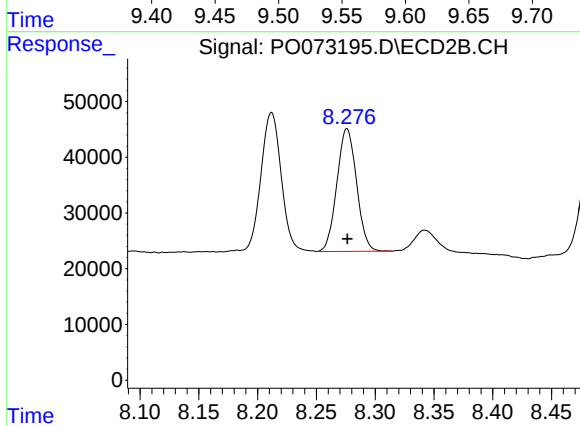

#42 AR-1268-2

R.T.: 8.276 min
Delta R.T.: 0.000 min
Response: 256914
Conc: 57.68 ng/ml

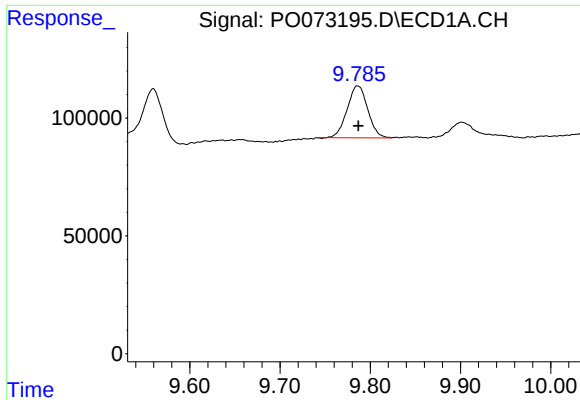


#43 AR-1268-3

R.T.: 9.786 min
Delta R.T.: 0.000 min
Response: 349122
Conc: 60.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
11/11/2020 9:00:28 AM

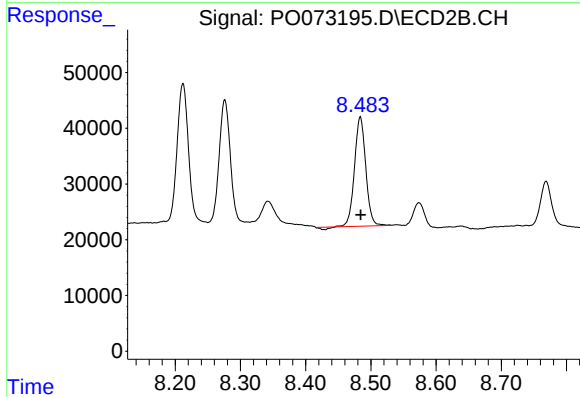


#43 AR-1268-3

R.T.: 8.484 min
Delta R.T.: 0.000 min
Response: 233109
Conc: 59.87 ng/ml

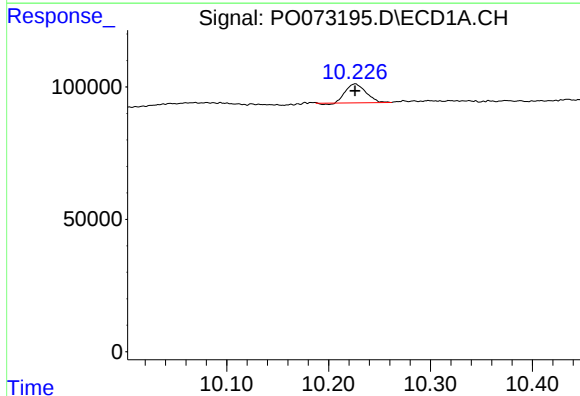


#44 AR-1268-4

R.T.: 10.226 min
Delta R.T.: 0.000 min
Response: 98851
Conc: 46.26 ng/ml

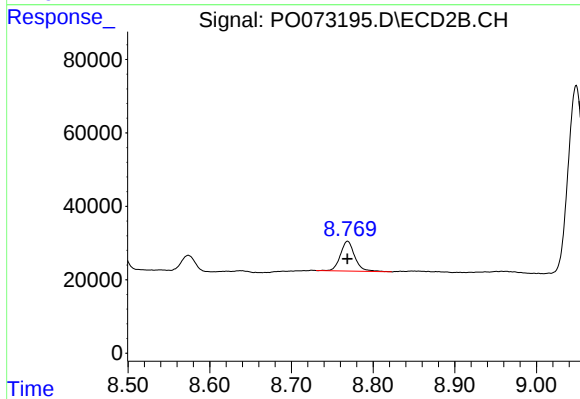

#44 AR-1268-4

R.T.: 8.769 min
Delta R.T.: 0.000 min
Response: 99429
Conc: 59.63 ng/ml

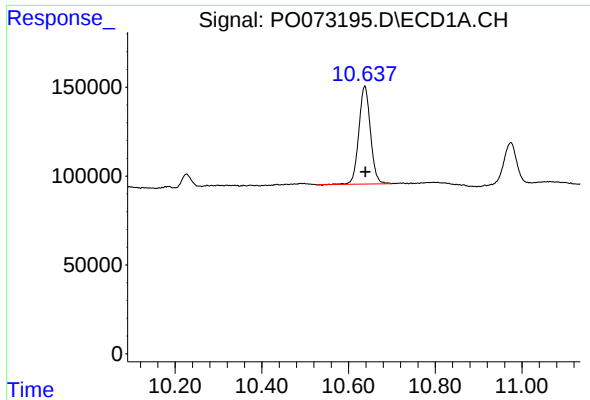


#45 AR-1268-5

R.T.: 10.638 min
Delta R.T.: -0.001 min
Response: 1022108
Conc: 59.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Ankita
11/11/2020 9:00:28 AM

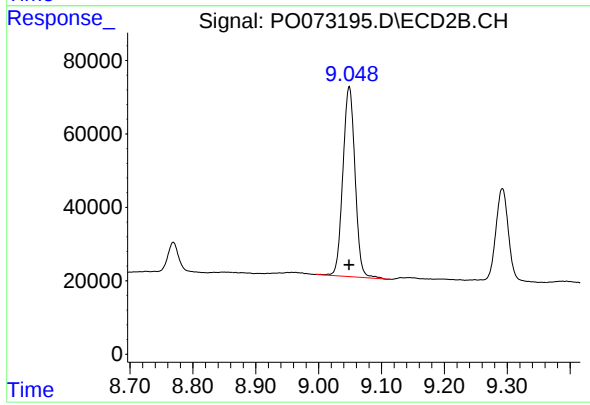

#45 AR-1268-5

R.T.: 9.049 min
Delta R.T.: 0.000 min
Response: 693961
Conc: 57.30 ng/ml