

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111021\
Data File : PO082728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2021 13:55
Operator : AJ\MA
Sample : M4601-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AS-RO-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 05:10:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.962	3.960	1877908	738448	21.455	23.862
2)	SA Decachlor...	11.065	9.274	1351502	660294	21.401	22.933

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111021\
Data File : P0082728.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2021 13:55
Operator : AJ\MA
Sample : M4601-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AS-RO-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 05:10:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110321.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 03 05:20:12 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

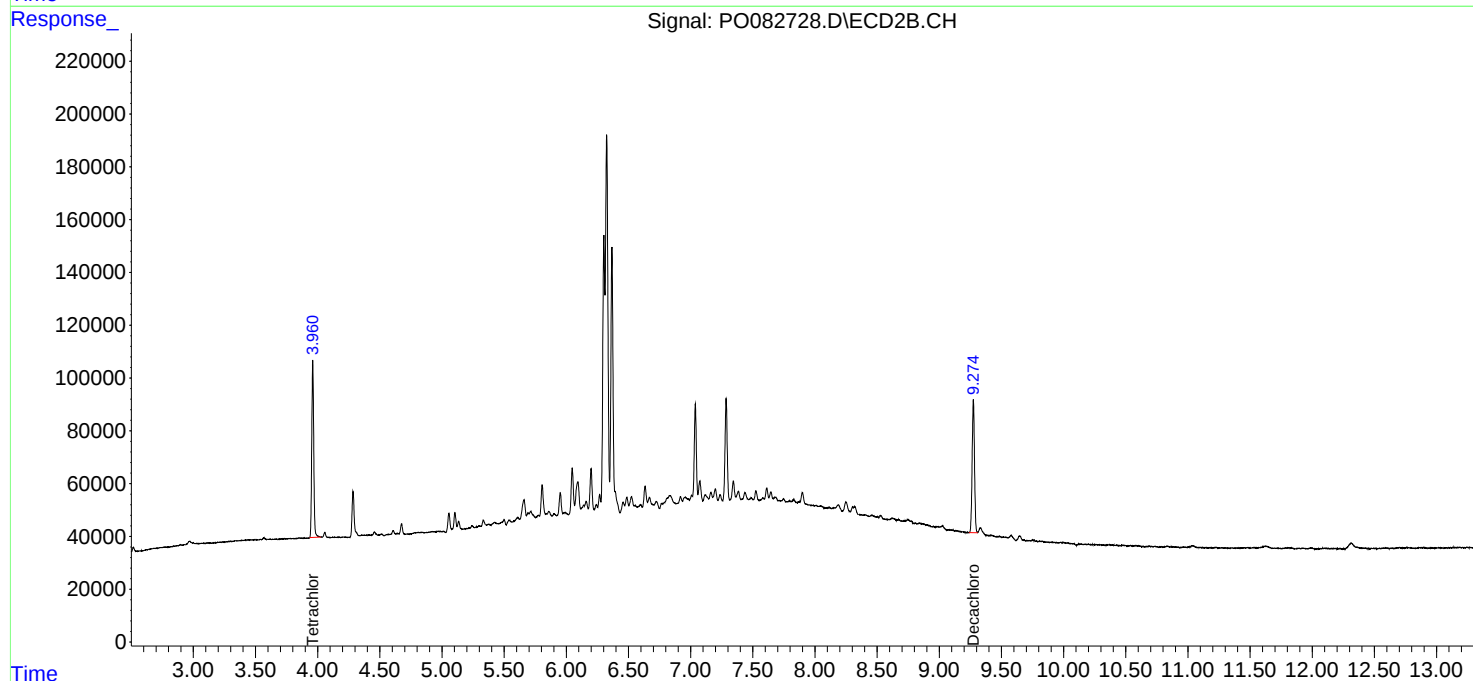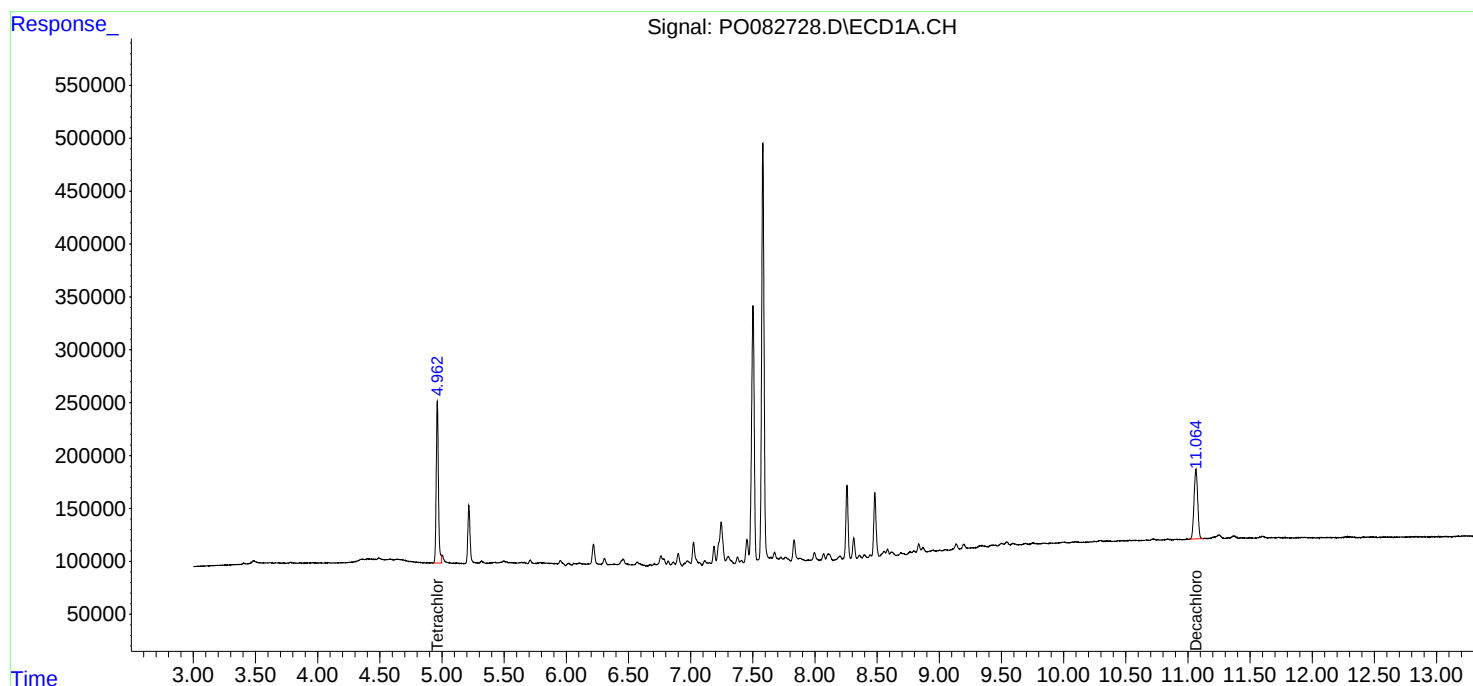


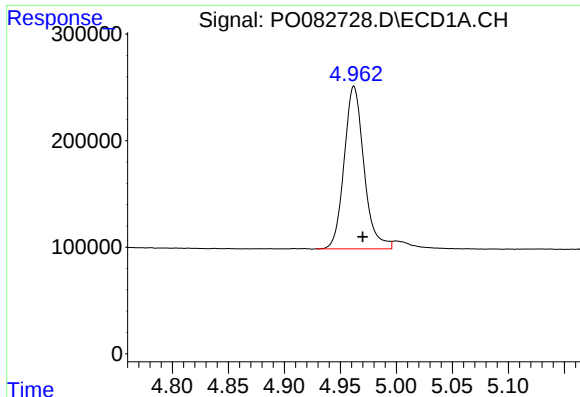

#1 Tetrachloro-m-xylene


R.T.: 4.962 min
Delta R.T.: -0.008 min
Response: 1877908
Conc: 21.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
AS-RO-COMP

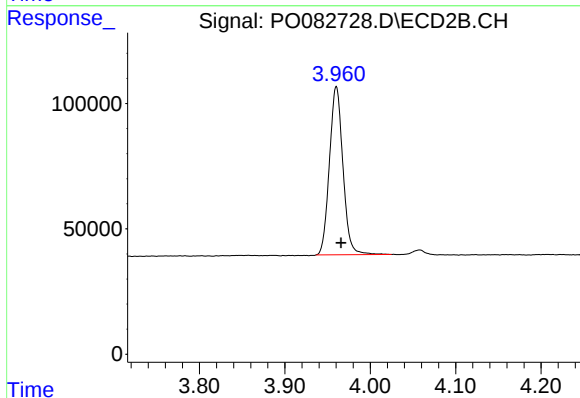


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: -0.006 min
Response: 738448
Conc: 23.86 ng/ml

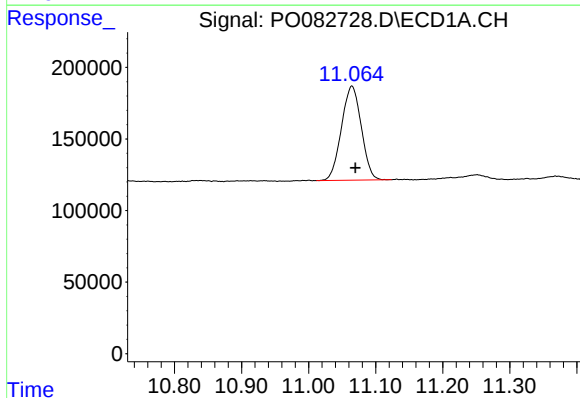

#2 Decachlorobiphenyl

R.T.: 11.065 min
Delta R.T.: -0.005 min
Response: 1351502
Conc: 21.40 ng/ml

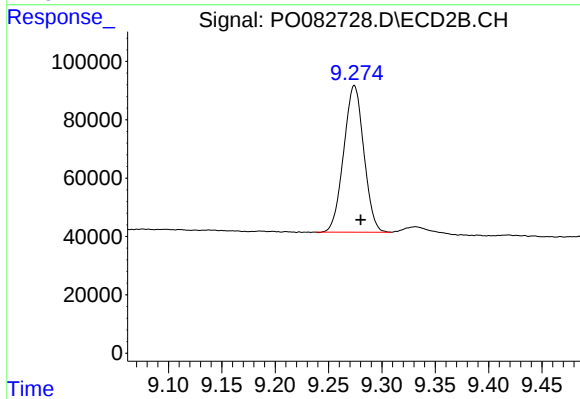

#2 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: -0.006 min
Response: 660294
Conc: 22.93 ng/ml