

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111022\
 Data File : PO090417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 12:27
 Operator : YP/AJ
 Sample : N5526-03DL 50X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 64ADL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2022
 Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 20:57:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
26)	L6	AR-1254-1	6.339	5.371	9424324	6207124	81.316 105.374 #
27)	L6	AR-1254-2	6.559	5.519	21300920	8031146	122.466 149.890
28)	L6	AR-1254-3	6.927	5.924	35731670	18729506	205.821 225.976
29)	L6	AR-1254-4	7.214	6.154	47337619	21312311	371.373 429.126
30)	L6	AR-1254-5	7.636	6.574	83776999	47373801	594.756 632.701

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111022\
Data File : PO090417.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 12:27
Operator : YP/AJ
Sample : N5526-03DL 50X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
64ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 20:57:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

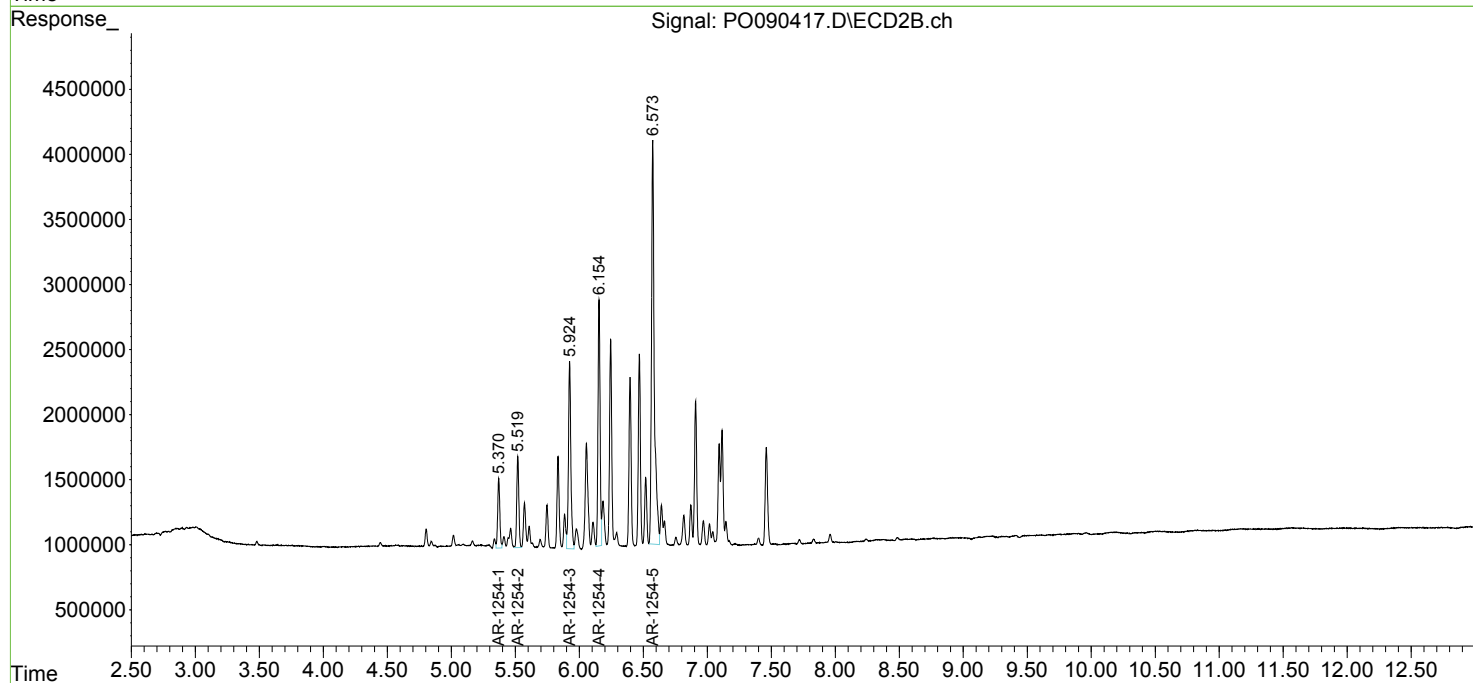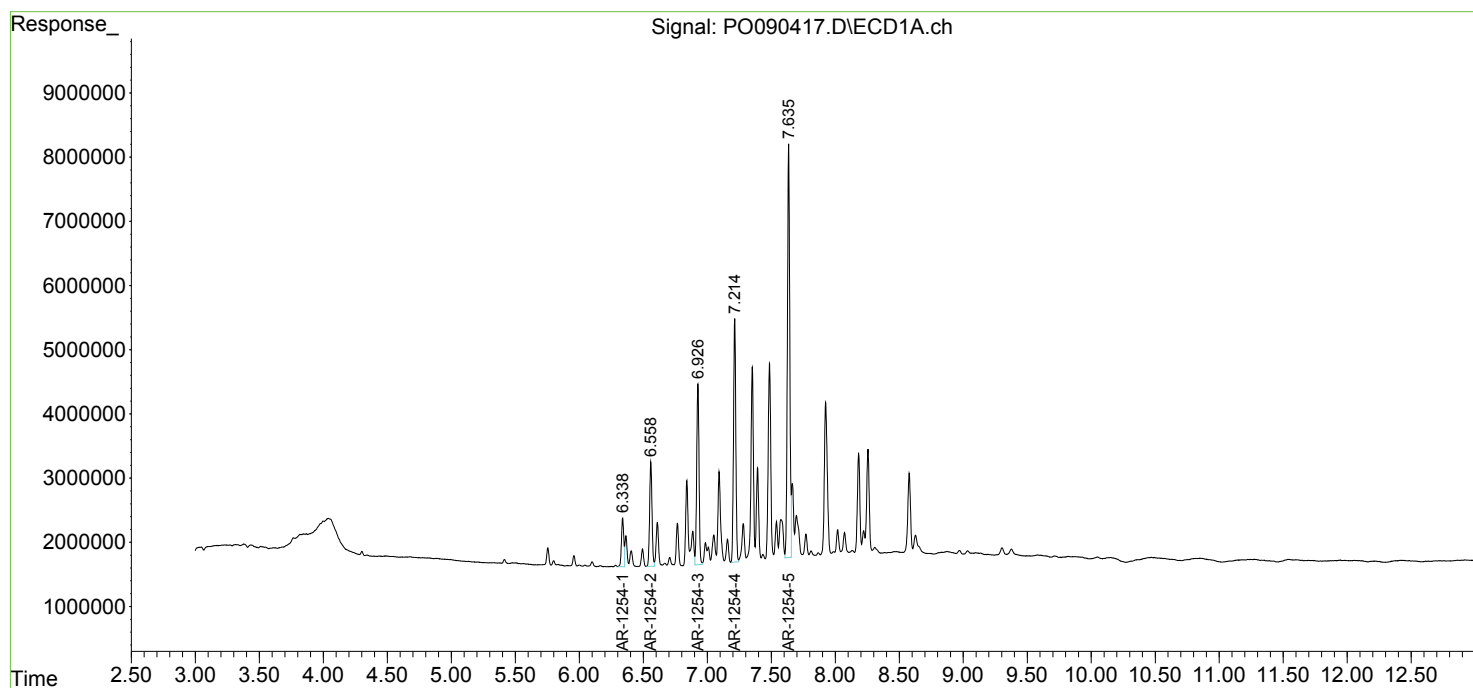

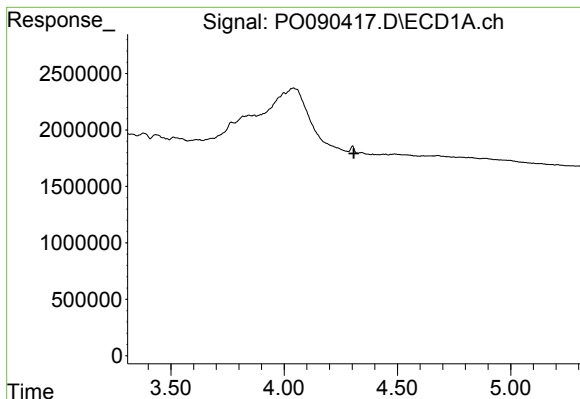


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
64ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

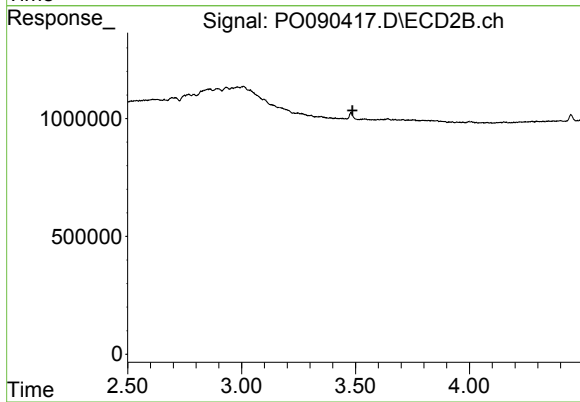


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

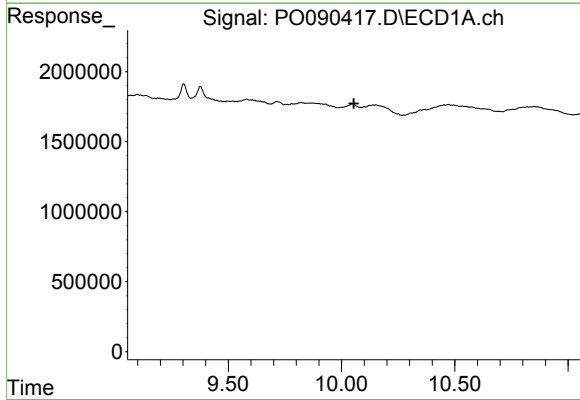


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.054 min
Response: 0
Conc: N.D.

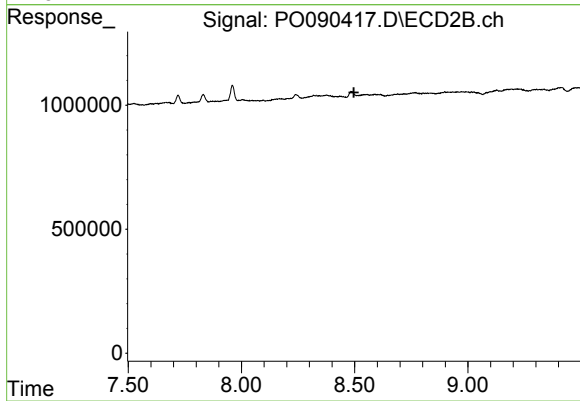

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.496 min
Response: 0
Conc: N.D.

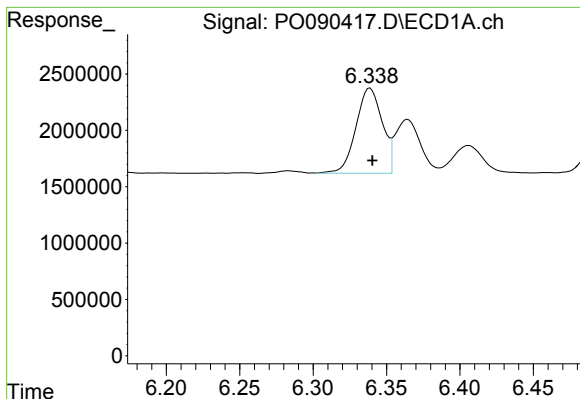


#26 AR-1254-1

R.T.: 6.339 min
Delta R.T.: -0.002 min
Response: 9424324
Conc: 81.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
64ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

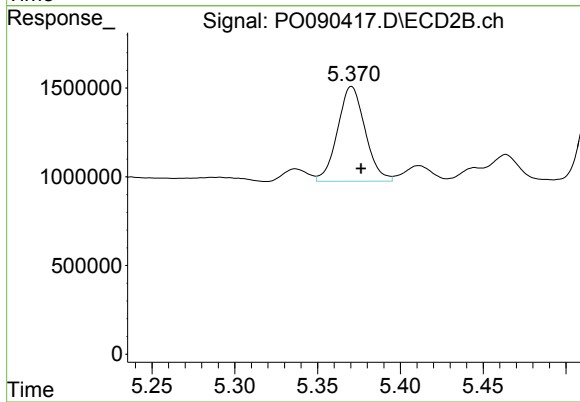


#26 AR-1254-1

R.T.: 5.371 min
Delta R.T.: -0.006 min
Response: 6207124
Conc: 105.37 ng/ml

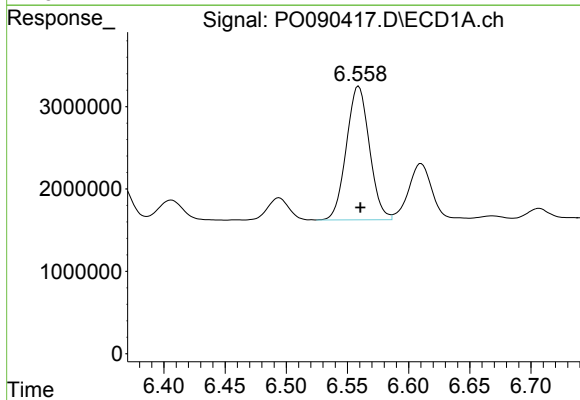


#27 AR-1254-2

R.T.: 6.559 min
Delta R.T.: -0.001 min
Response: 21300920
Conc: 122.47 ng/ml

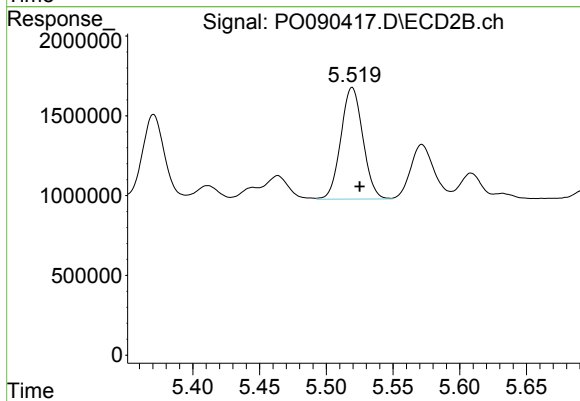

#27 AR-1254-2

R.T.: 5.519 min
Delta R.T.: -0.006 min
Response: 8031146
Conc: 149.89 ng/ml

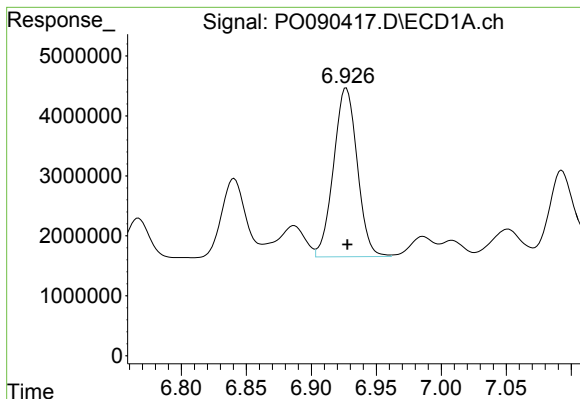


#28 AR-1254-3

R.T.: 6.927 min
Delta R.T.: 0.000 min
Response: 35731670
Conc: 205.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
64ADL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

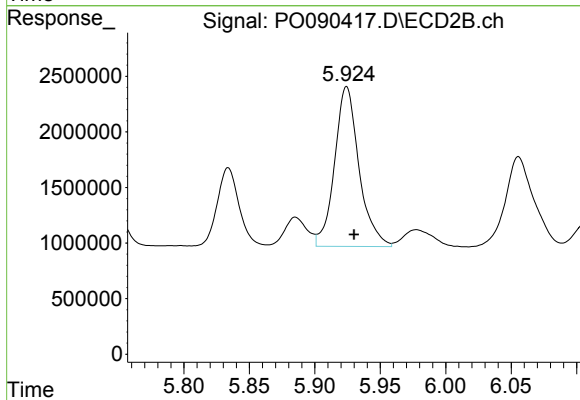


#28 AR-1254-3

R.T.: 5.924 min
Delta R.T.: -0.006 min
Response: 18729506
Conc: 225.98 ng/ml

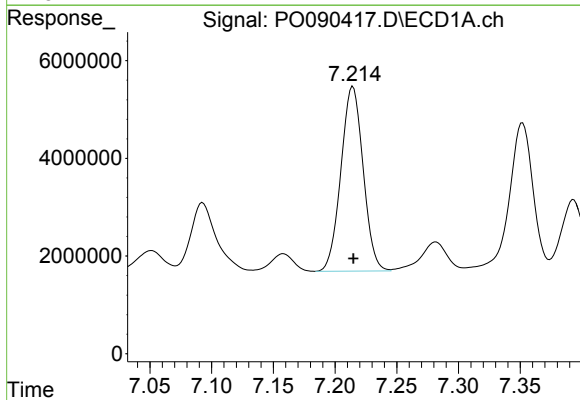


#29 AR-1254-4

R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 47337619
Conc: 371.37 ng/ml

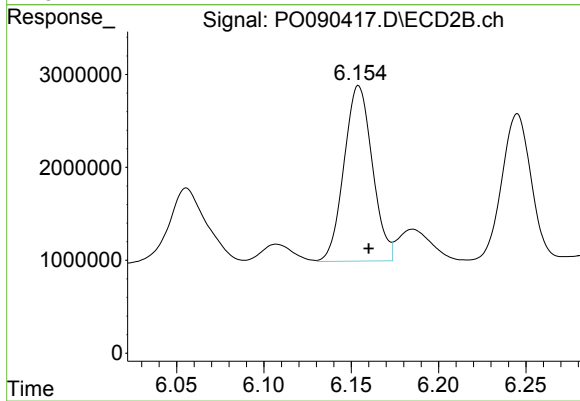

#29 AR-1254-4

R.T.: 6.154 min
Delta R.T.: -0.006 min
Response: 21312311
Conc: 429.13 ng/ml

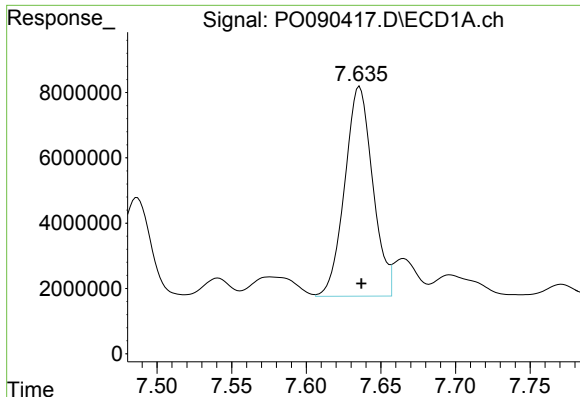


#30 AR-1254-5

R.T.: 7.636 min
Delta R.T.: -0.001 min
Response: 83776999
Conc: 594.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
64ADL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

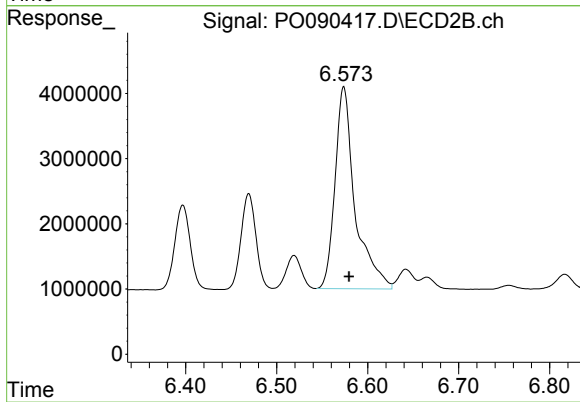

#30 AR-1254-5

R.T.: 6.574 min
Delta R.T.: -0.006 min
Response: 47373801
Conc: 632.70 ng/ml