

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111022\
 Data File : PO090454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 23:54
 Operator : YP/AJ
 Sample : N5538-03
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP-14-B-EAST

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2022
 Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 03:56:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.303	3.481	50089586	17866344	15.585	16.811
2) SA Decachlor...	10.051	8.486	43281811	16384598	17.662	15.908
Target Compounds						
31) L7 AR-1260-1	7.093	6.056	3074074	1429277	21.929	23.742
32) L7 AR-1260-2	7.352	6.247	2518501	1074916	15.567	14.879m
33) L7 AR-1260-3	7.714	6.398	1291856	776516	12.297	11.653m
34) L7 AR-1260-4	7.937	6.873	3019741	564071	24.443	11.088 #
35) L7 AR-1260-5	8.256	7.117	3605659	1260834	15.845	10.855 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111022\
Data File : PO090454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 23:54
Operator : YP/AJ
Sample : N5538-03
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-14-B-EAST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 03:56:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

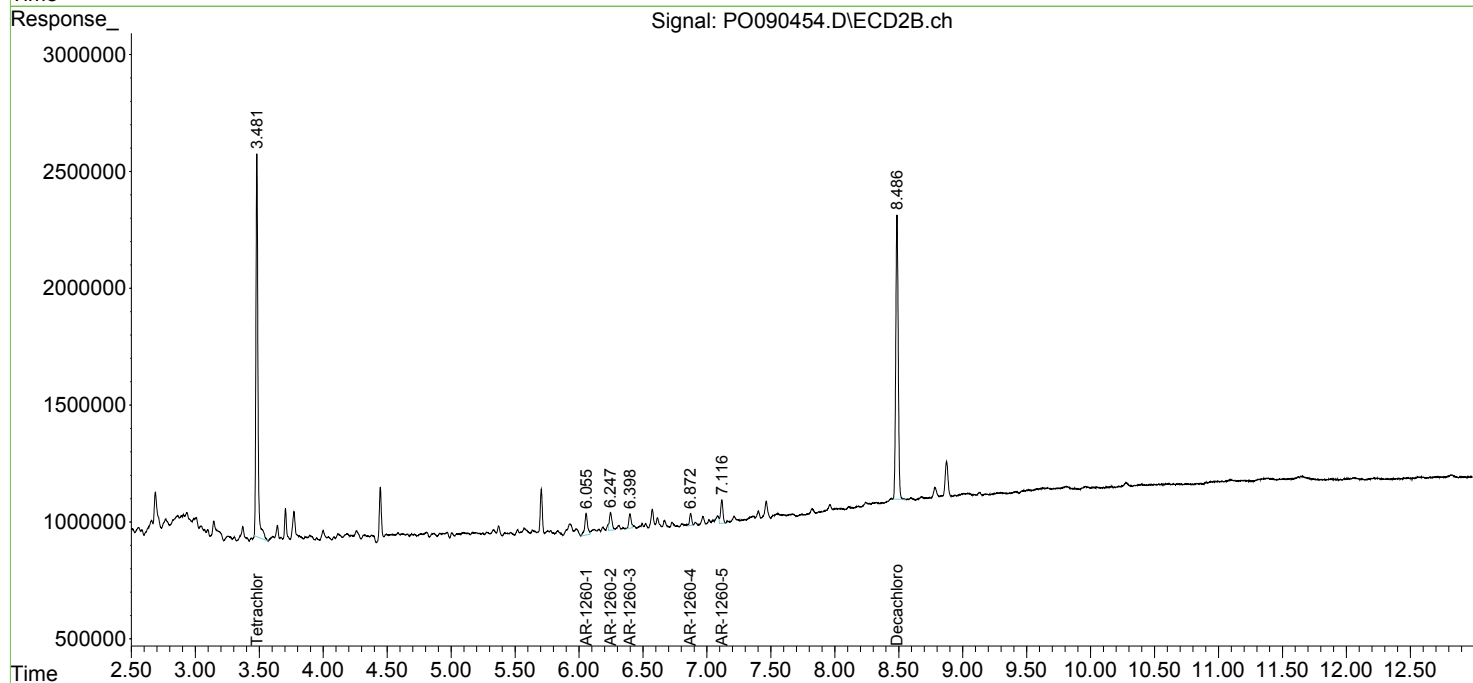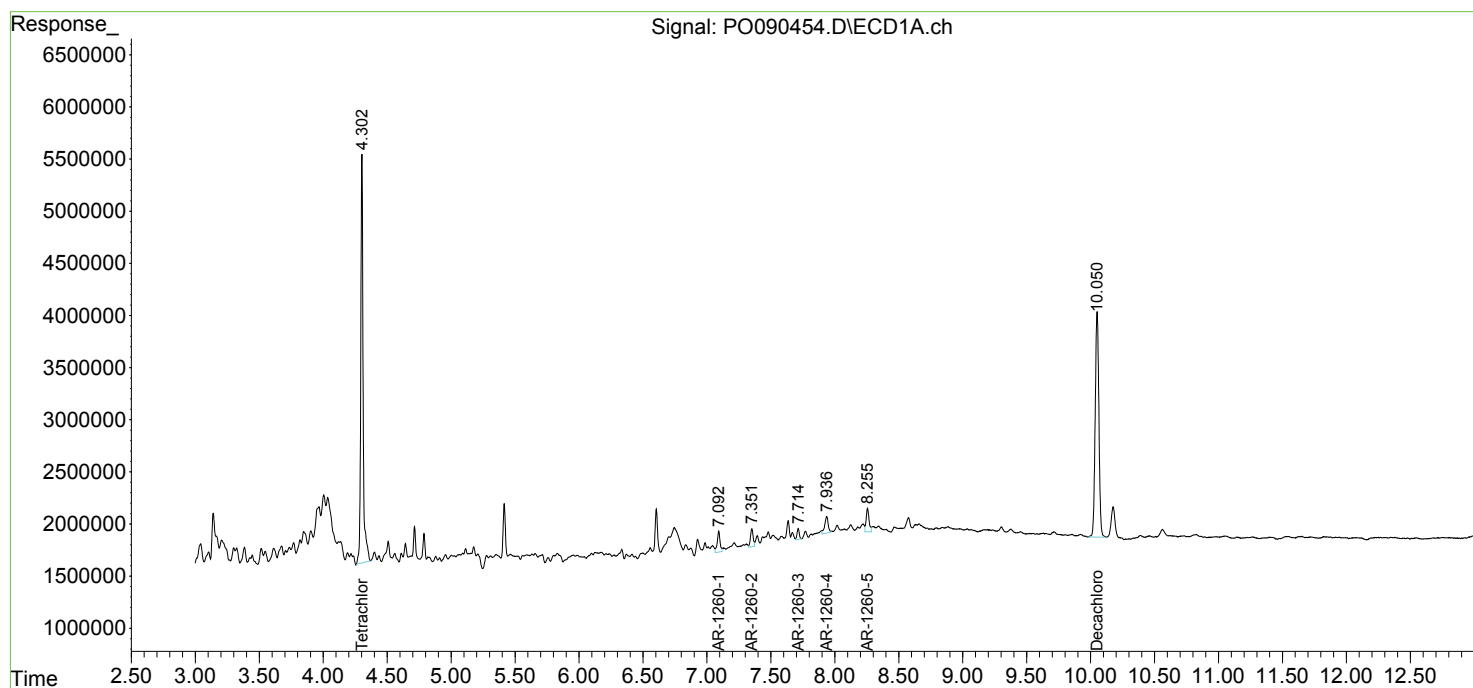

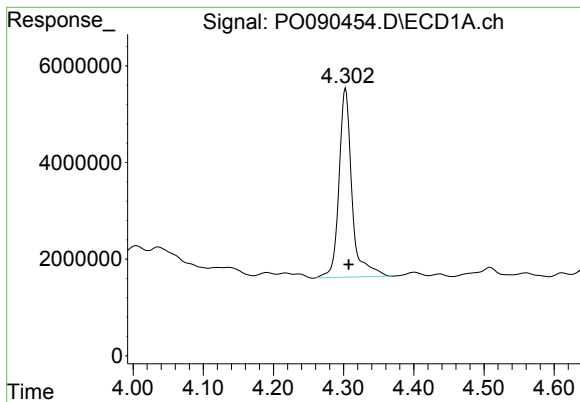


#1 Tetrachloro-m-xylene

R.T.: 4.303 min
Delta R.T.: -0.004 min
Response: 50089586
Conc: 15.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-14-B-EAST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

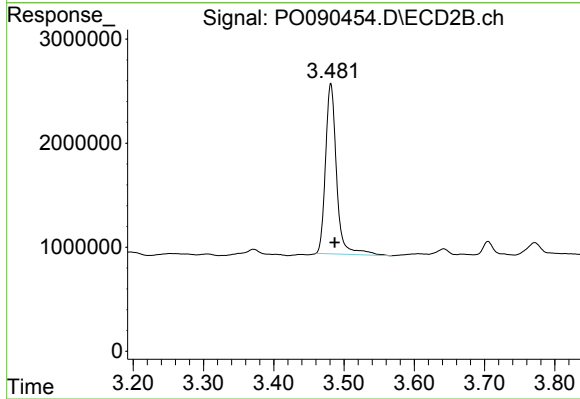


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: -0.005 min
Response: 17866344
Conc: 16.81 ng/ml

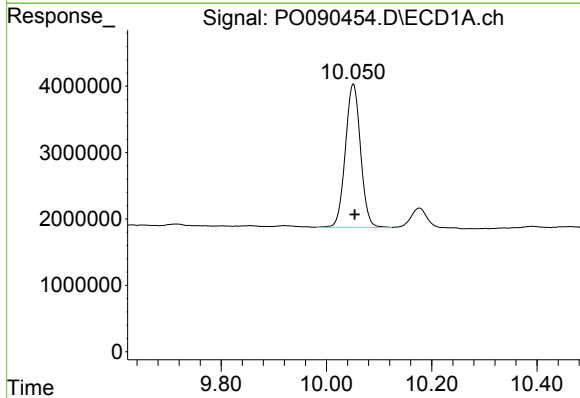


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.003 min
Response: 43281811
Conc: 17.66 ng/ml

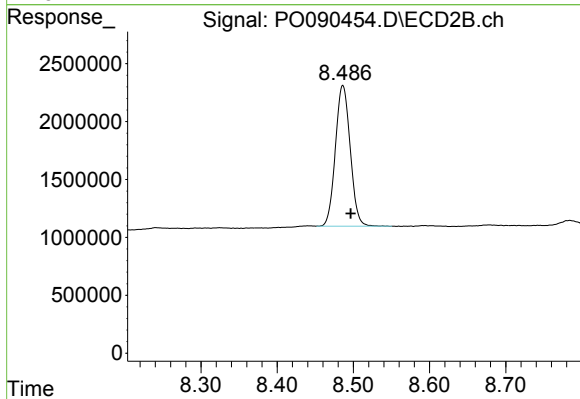

#2 Decachlorobiphenyl

R.T.: 8.486 min
Delta R.T.: -0.010 min
Response: 16384598
Conc: 15.91 ng/ml

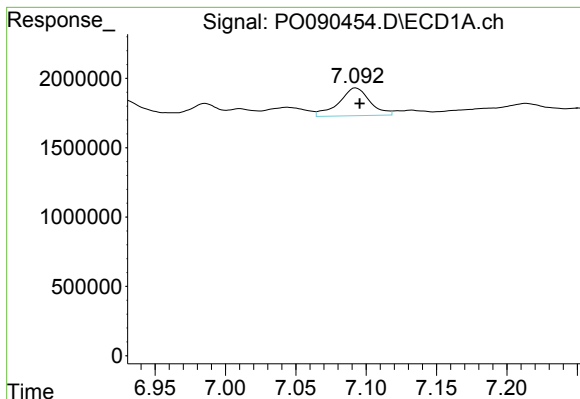


#31 AR-1260-1

R.T.: 7.093 min
Delta R.T.: -0.003 min
Response: 3074074
Conc: 21.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-14-B-EAST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

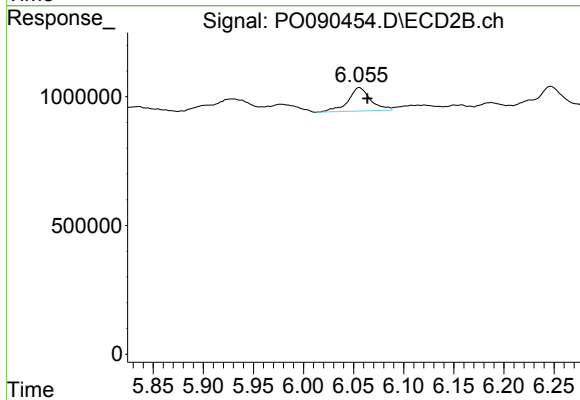


#31 AR-1260-1

R.T.: 6.056 min
Delta R.T.: -0.008 min
Response: 1429277
Conc: 23.74 ng/ml

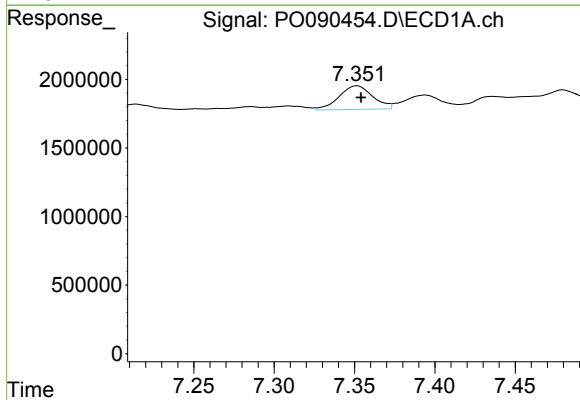


#32 AR-1260-2

R.T.: 7.352 min
Delta R.T.: -0.002 min
Response: 2518501
Conc: 15.57 ng/ml

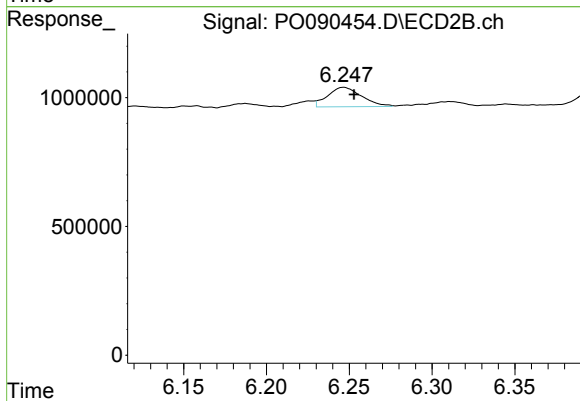

#32 AR-1260-2

R.T.: 6.247 min
Delta R.T.: -0.006 min
Response: 1074916
Conc: 14.88 ng/ml m

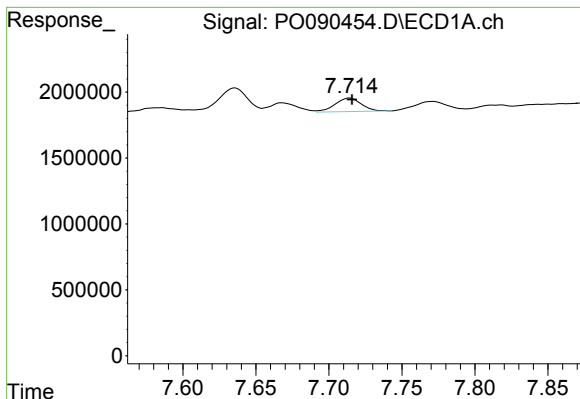


#33 AR-1260-3

R.T.: 7.714 min
Delta R.T.: -0.002 min
Response: 1291856
Conc: 12.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-14-B-EAST


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

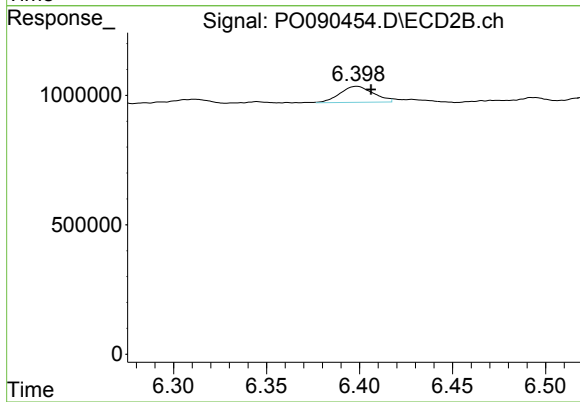


#33 AR-1260-3

R.T.: 6.398 min
Delta R.T.: -0.008 min
Response: 776516
Conc: 11.65 ng/ml m

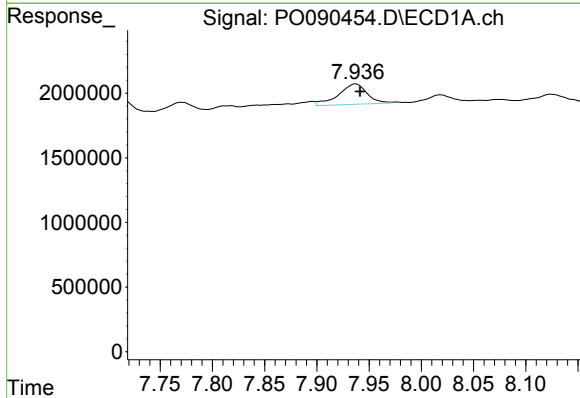


#34 AR-1260-4

R.T.: 7.937 min
Delta R.T.: -0.004 min
Response: 3019741
Conc: 24.44 ng/ml

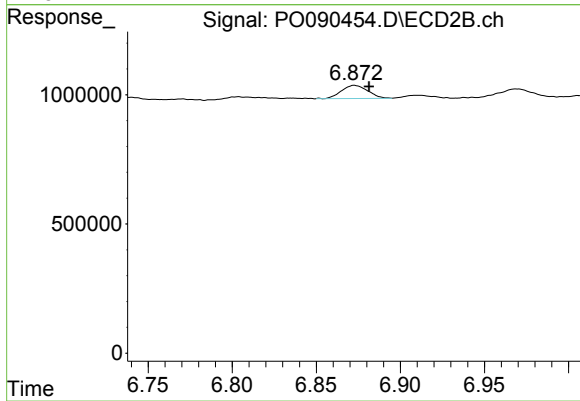

#34 AR-1260-4

R.T.: 6.873 min
Delta R.T.: -0.008 min
Response: 564071
Conc: 11.09 ng/ml

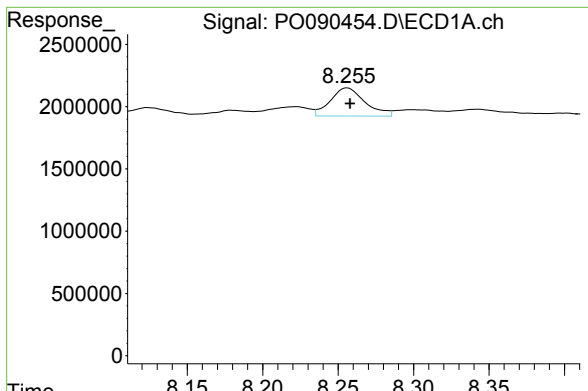

#35 AR-1260-5

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 3605659
Conc: 15.85 ng/ml

Instrument :

ECD_O


ClientSampleId :

TP-14-B-EAST

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

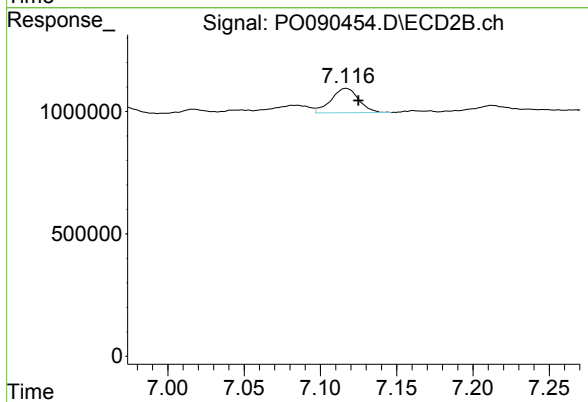

#35 AR-1260-5

R.T.: 7.117 min
Delta R.T.: -0.008 min
Response: 1260834
Conc: 10.86 ng/ml