

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111022\
 Data File : PO090467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2022 04:05
 Operator : YP/AJ
 Sample : N5561-05
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-05

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2022
 Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 05:45:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.302	3.480	64809252	20754308	20.165	19.528
2) SA Decachlor...	10.050	8.486	33924272	14394105	13.843m	13.976

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111022\
Data File : PO090467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2022 04:05
Operator : YP/AJ
Sample : N5561-05
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 05:45:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

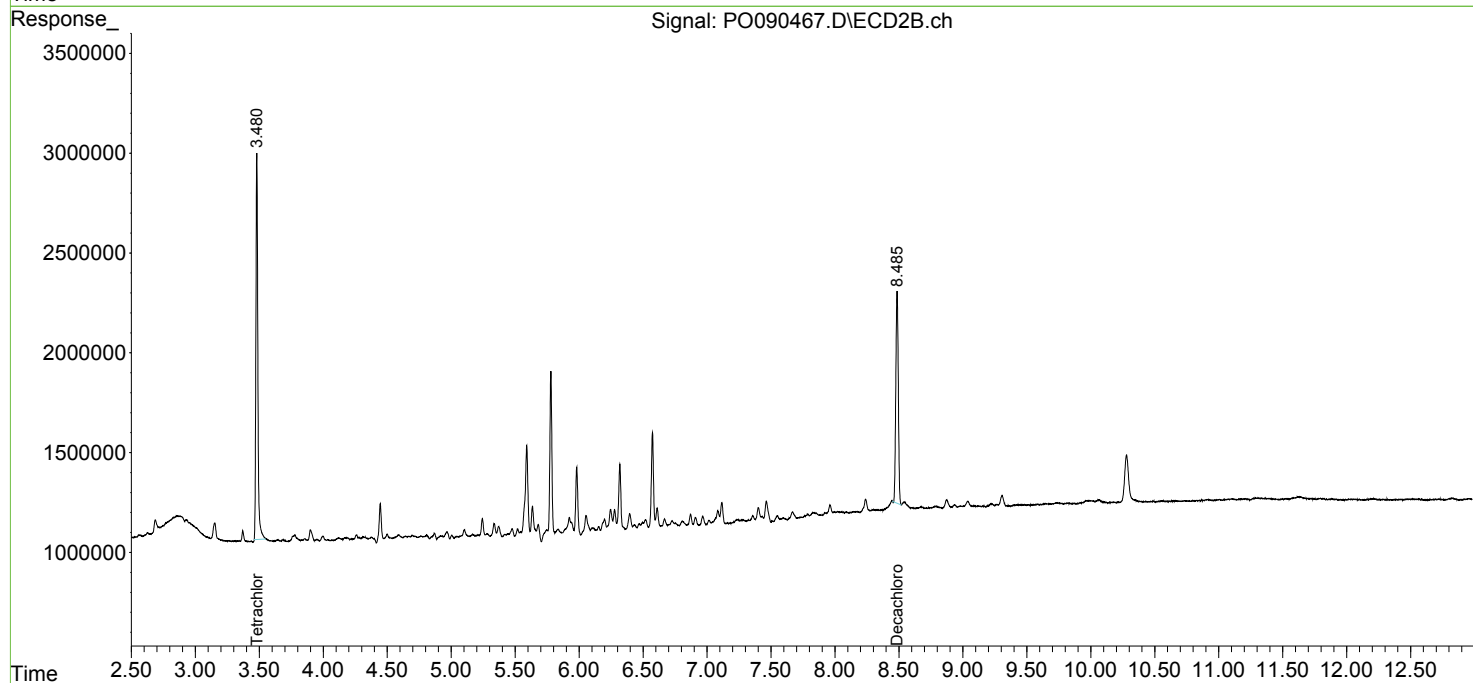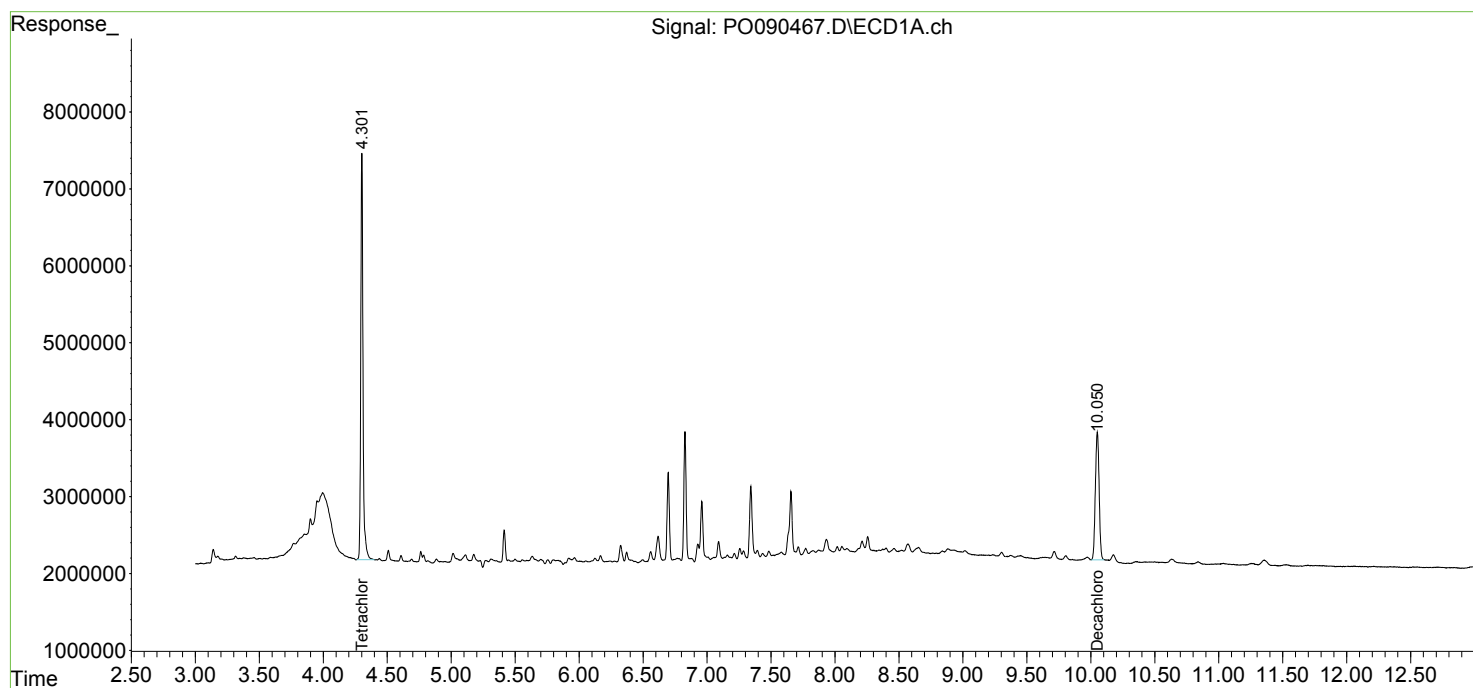

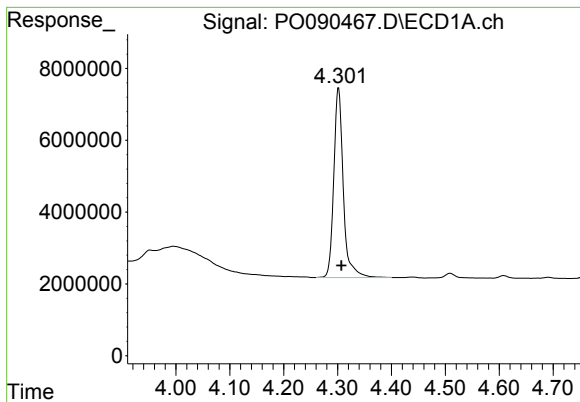


#1 Tetrachloro-m-xylene

R.T.: 4.302 min
Delta R.T.: -0.005 min
Response: 64809252
Conc: 20.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-05


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

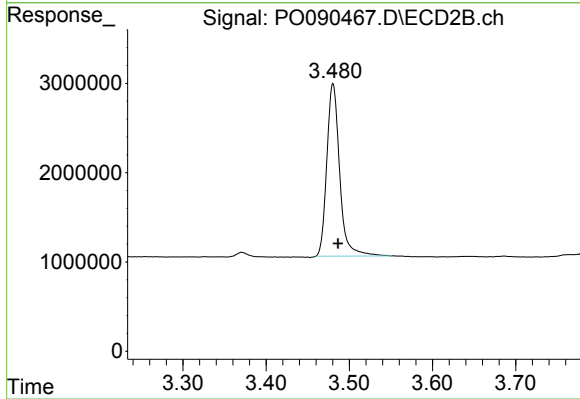


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: -0.006 min
Response: 20754308
Conc: 19.53 ng/ml

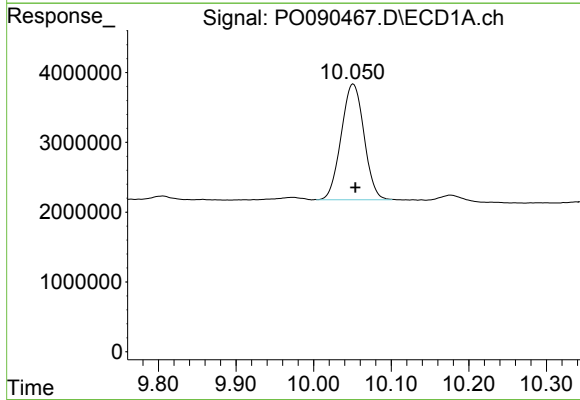

#2 Decachlorobiphenyl

R.T.: 10.050 min
Delta R.T.: -0.004 min
Response: 33924272
Conc: 13.84 ng/ml m

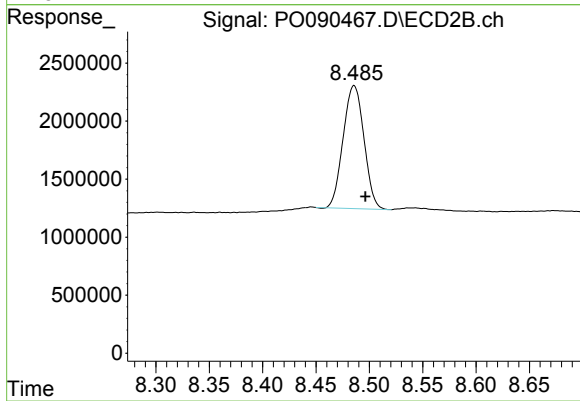

#2 Decachlorobiphenyl

R.T.: 8.486 min
Delta R.T.: -0.011 min
Response: 14394105
Conc: 13.98 ng/ml