

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111023\
 Data File : PO099603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2023 20:29
 Operator : YP/AJ
 Sample : 05351-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-241

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2023
 Supervised By :Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 22:35:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 10 11:13:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.494	3.722	34201735	24035613	19.867	19.826
2) SA Decachlor...	10.378	8.833	18601925	19285850	29.142m	26.257m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111023\
Data File : PO099603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2023 20:29
Operator : YP/AJ
Sample : 05351-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-241


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 22:35:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 10 11:13:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

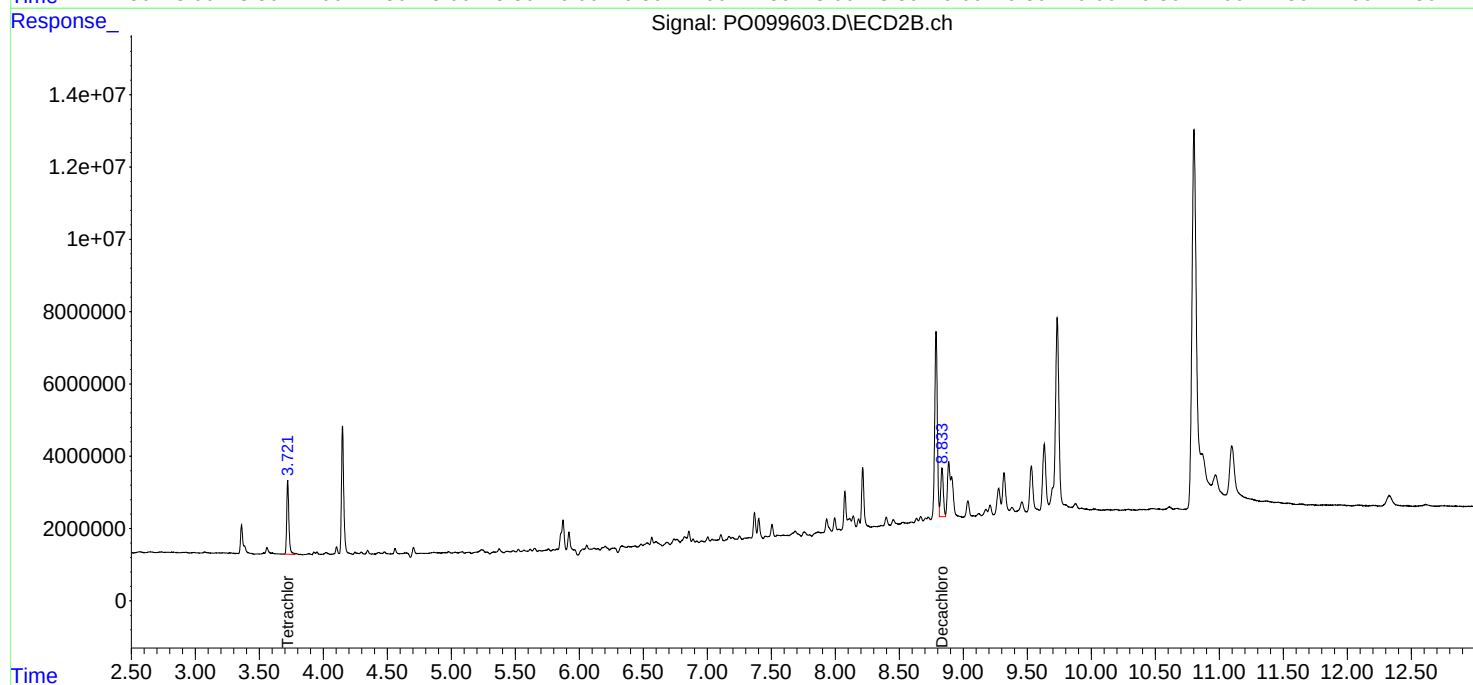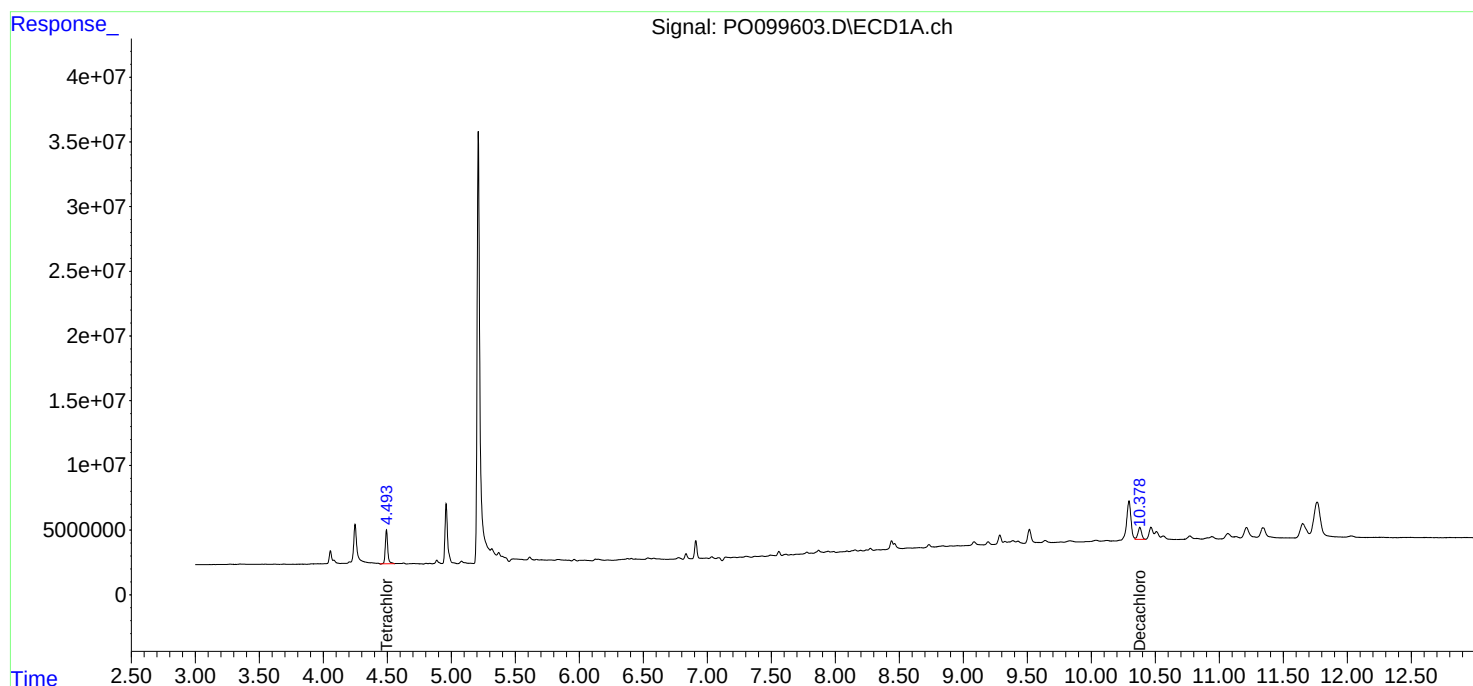

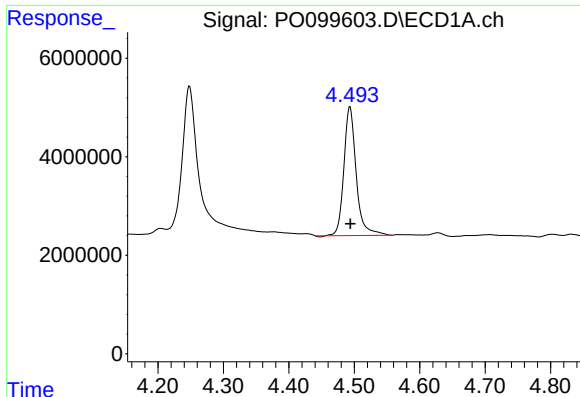


#1 Tetrachloro-m-xylene

R.T.: 4.494 min
Delta R.T.: 0.000 min
Response: 34201735
Conc: 19.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-241


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

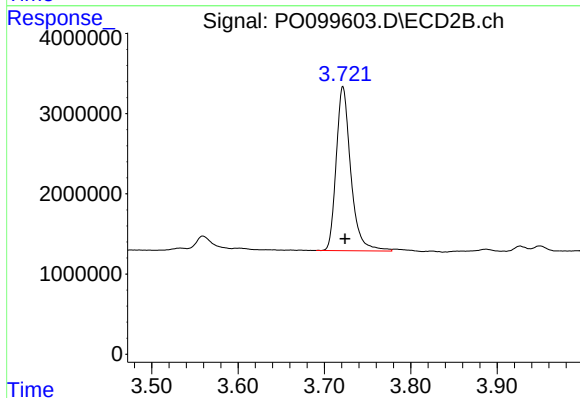


#1 Tetrachloro-m-xylene

R.T.: 3.722 min
Delta R.T.: -0.003 min
Response: 24035613
Conc: 19.83 ng/ml

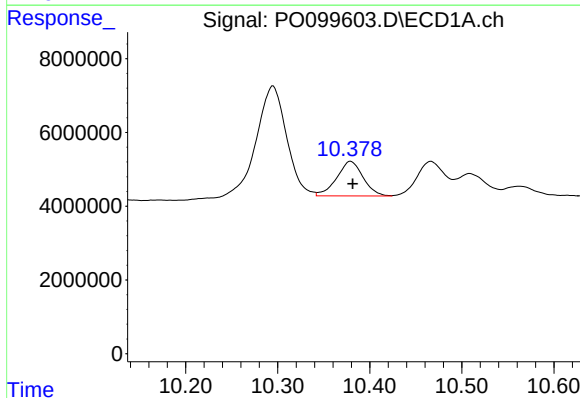

#2 Decachlorobiphenyl

R.T.: 10.378 min
Delta R.T.: -0.003 min
Response: 18601925
Conc: 29.14 ng/ml m

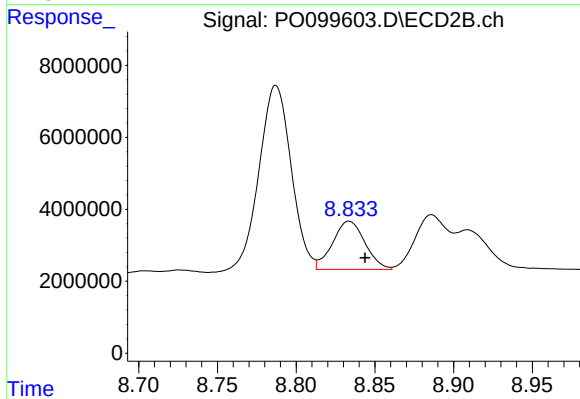

#2 Decachlorobiphenyl

R.T.: 8.833 min
Delta R.T.: -0.011 min
Response: 19285850
Conc: 26.26 ng/ml m