

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111023\
 Data File : PO099633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2023 06:20
 Operator : YP/AJ
 Sample : 05353-06 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 BC258874-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2023
 Supervised By :Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 23:28:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO110923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 10 11:13:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.493	3.721	2989443	2034508	1.737	1.678
2) SA Decachlor...	10.374	8.833	1684168	1545692	2.638	2.104
Target Compounds						
26) L6 AR-1254-1	6.544	5.643	531055	437479	11.800m	12.027m
27) L6 AR-1254-2	6.767	5.791	910092	501244	14.432	15.430m
28) L6 AR-1254-3	7.135	6.202	1064278	671498	18.273	12.384m#
29) L6 AR-1254-4	7.425	6.432	687744	472233	20.179	16.768m
30) L6 AR-1254-5	7.847	6.855	946435	748009	24.188	15.352m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111023\
Data File : PO099633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2023 06:20
Operator : YP/AJ
Sample : 05353-06 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC258874-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 23:28:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 10 11:13:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

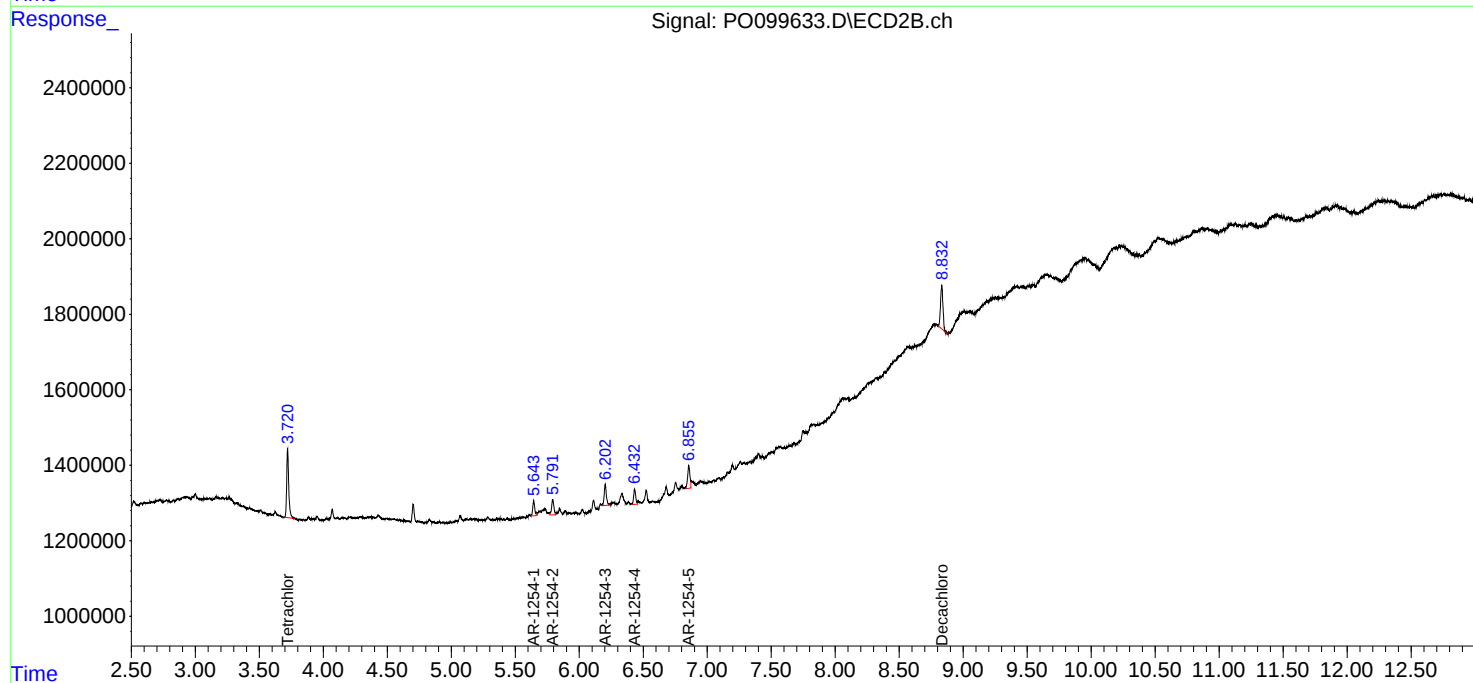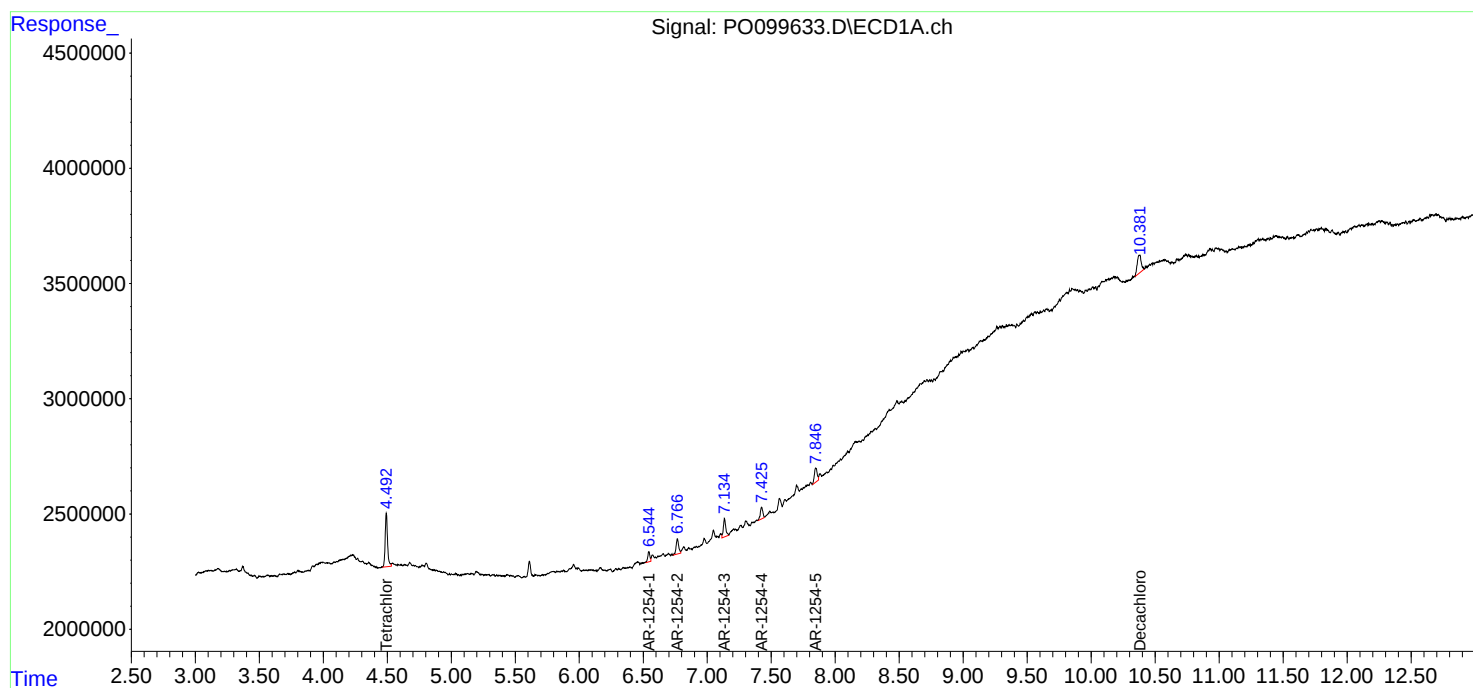

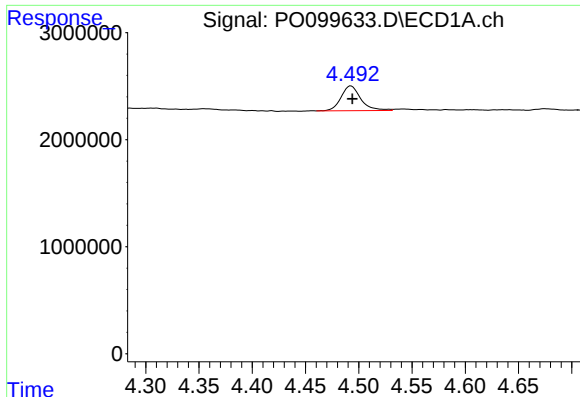


#1 Tetrachloro-m-xylene

R.T.: 4.493 min
Delta R.T.: -0.001 min
Response: 2989443
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC258874-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

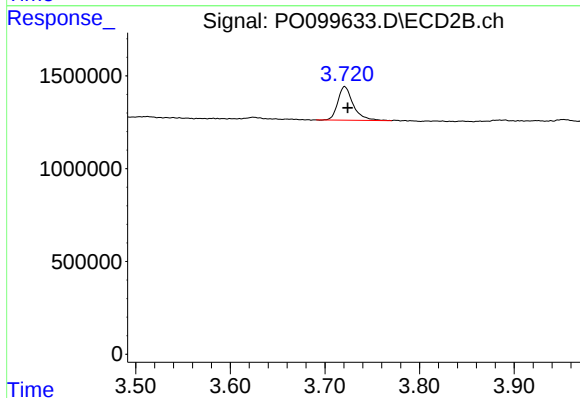


#1 Tetrachloro-m-xylene

R.T.: 3.721 min
Delta R.T.: -0.003 min
Response: 2034508
Conc: 1.68 ng/ml

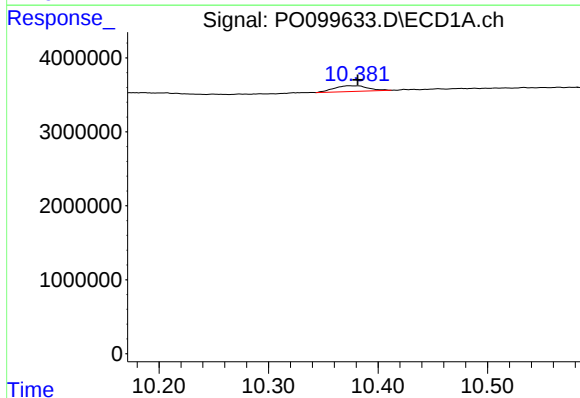


#2 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: -0.008 min
Response: 1684168
Conc: 2.64 ng/ml

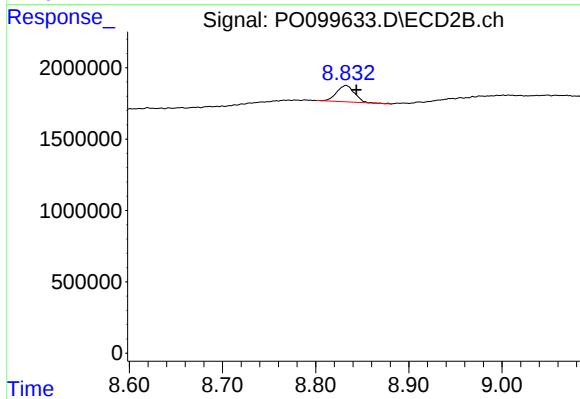

#2 Decachlorobiphenyl

R.T.: 8.833 min
Delta R.T.: -0.011 min
Response: 1545692
Conc: 2.10 ng/ml

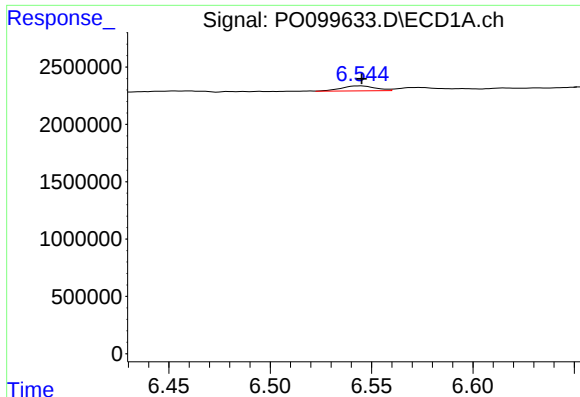


#26 AR-1254-1

R.T.: 6.544 min
Delta R.T.: -0.001 min
Response: 531055
Conc: 11.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC258874-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

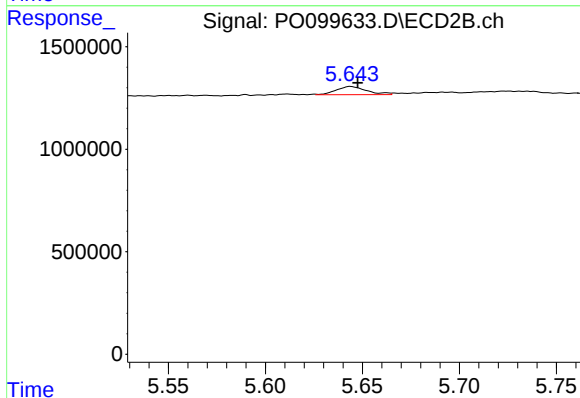


#26 AR-1254-1

R.T.: 5.643 min
Delta R.T.: -0.004 min
Response: 437479
Conc: 12.03 ng/ml m

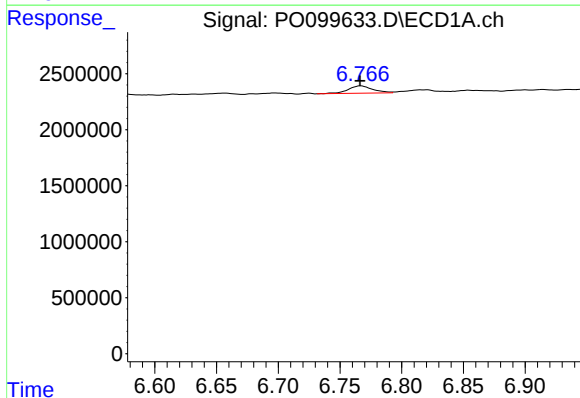


#27 AR-1254-2

R.T.: 6.767 min
Delta R.T.: 0.000 min
Response: 910092
Conc: 14.43 ng/ml

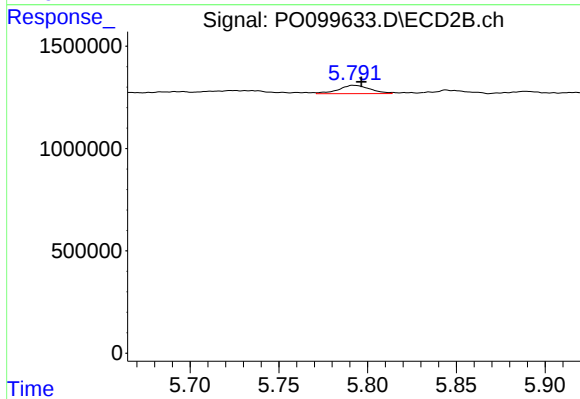

#27 AR-1254-2

R.T.: 5.791 min
Delta R.T.: -0.005 min
Response: 501244
Conc: 15.43 ng/ml m

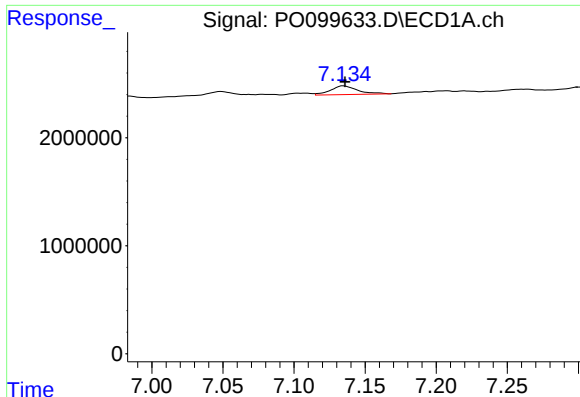


#28 AR-1254-3

R.T.: 7.135 min
Delta R.T.: -0.001 min
Response: 1064278
Conc: 18.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC258874-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

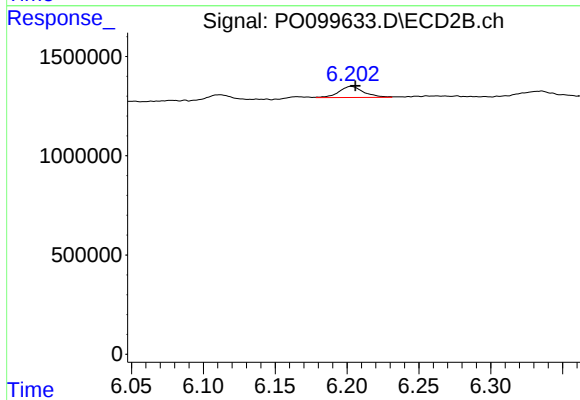


#28 AR-1254-3

R.T.: 6.202 min
Delta R.T.: -0.004 min
Response: 671498
Conc: 12.38 ng/ml m

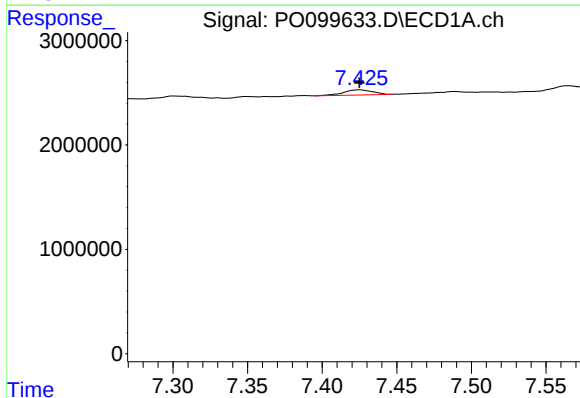


#29 AR-1254-4

R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 687744
Conc: 20.18 ng/ml

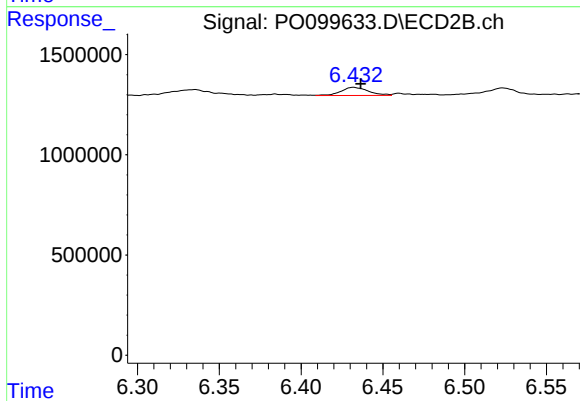

#29 AR-1254-4

R.T.: 6.432 min
Delta R.T.: -0.004 min
Response: 472233
Conc: 16.77 ng/ml m

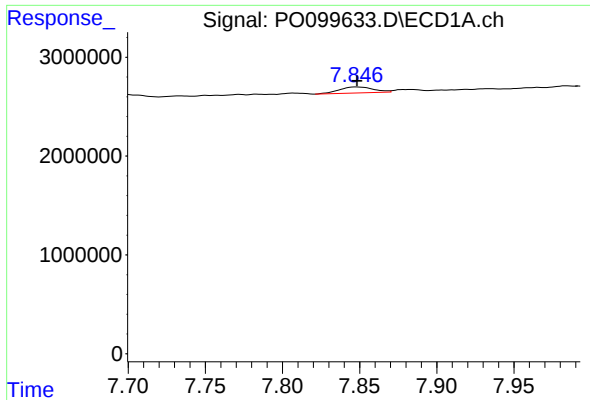


#30 AR-1254-5

R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 946435
Conc: 24.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC258874-1-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

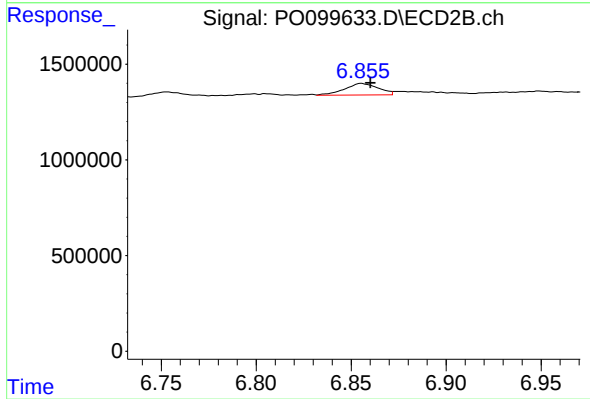

#30 AR-1254-5

R.T.: 6.855 min
Delta R.T.: -0.005 min
Response: 748009
Conc: 15.35 ng/ml m