

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111023\
 Data File : PO099643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2023 10:06
 Operator : YP/AJ
 Sample : 05355-04 10X
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH2650-2-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2023
 Supervised By :Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 23:31:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110923.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 10 11:13:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.491	3.721	2468345	1859428	1.434m	1.534
2) SA Decachlor...	10.373	8.832	1702093	1737953	2.667	2.366

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111023\
Data File : PO099643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2023 10:06
Operator : YP/AJ
Sample : 05355-04 10X
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH2650-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 23:31:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110923.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 10 11:13:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

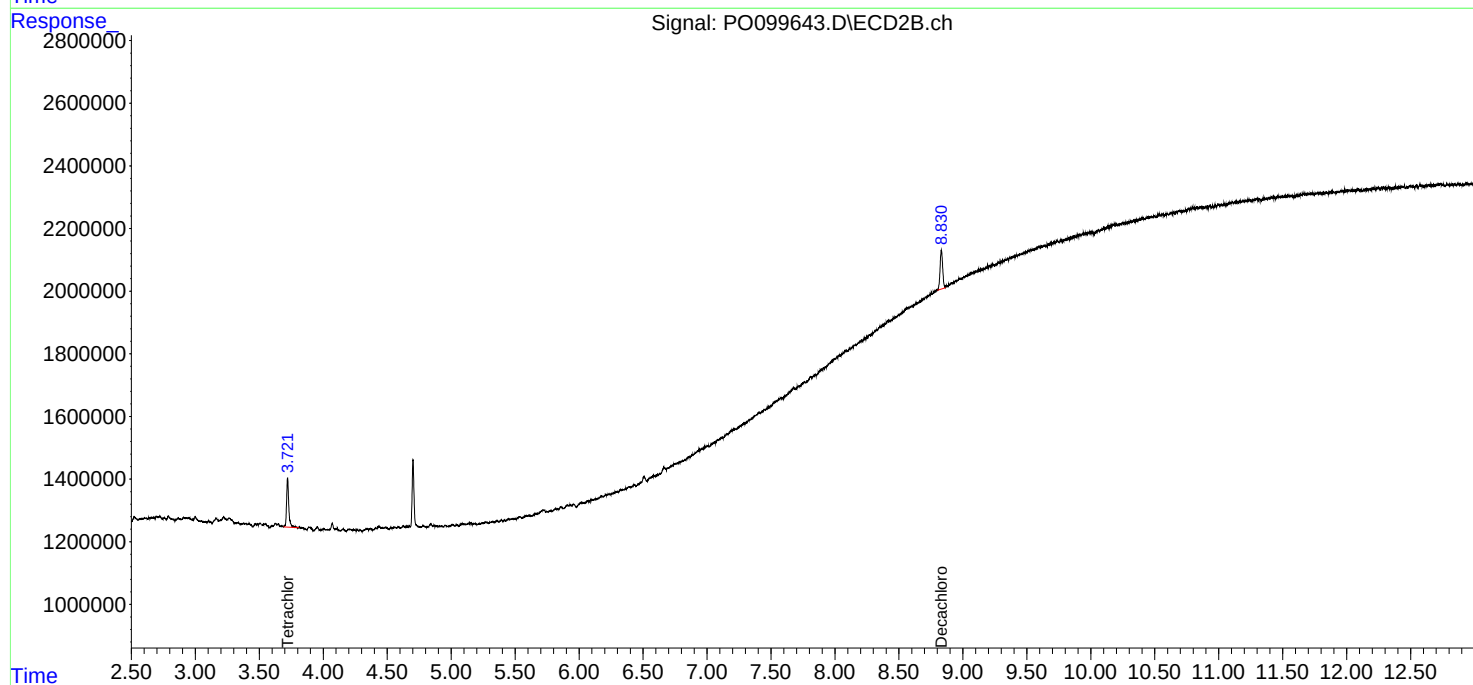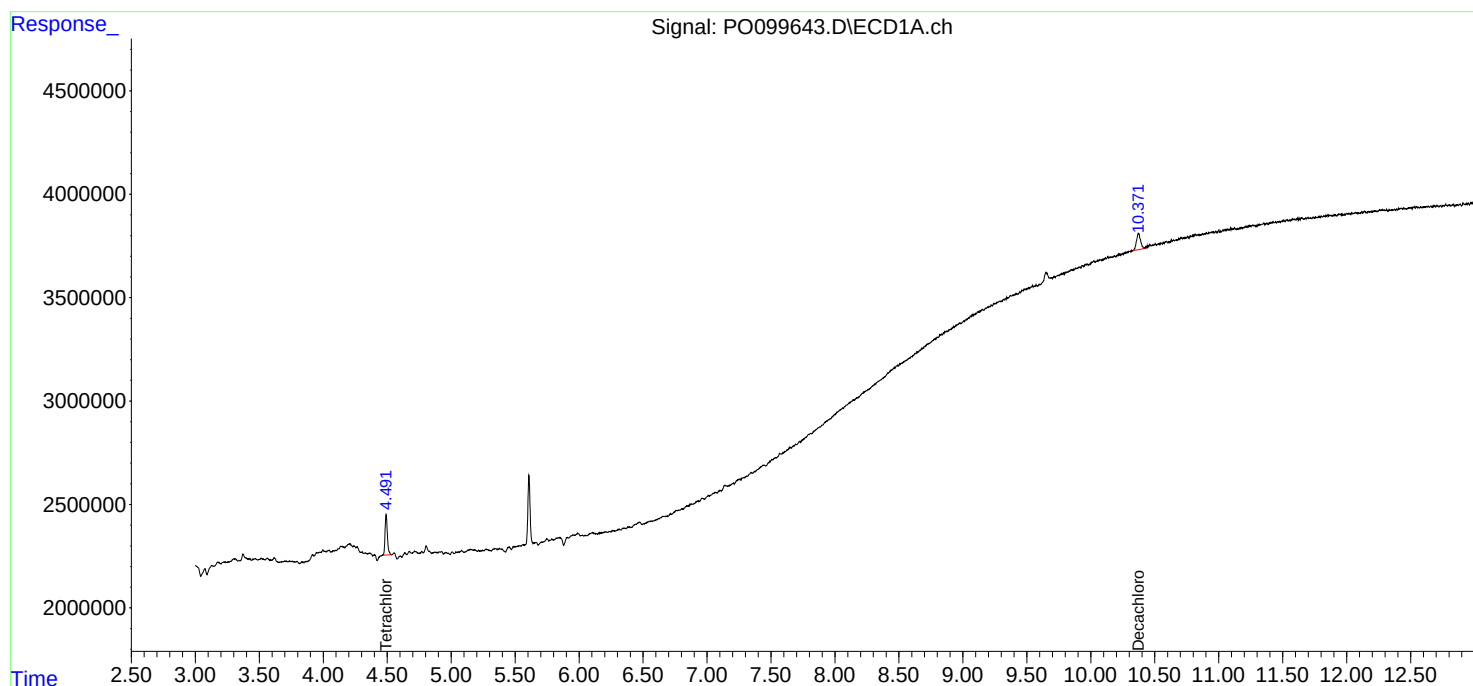

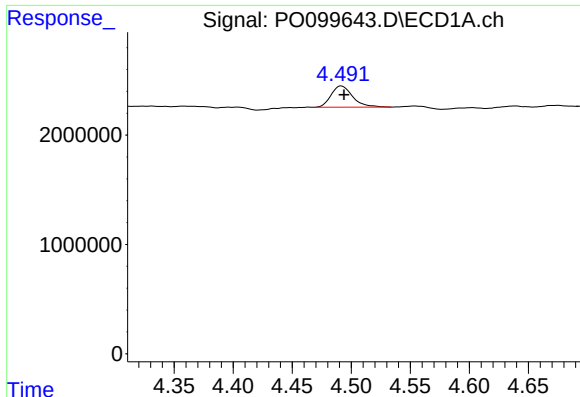


#1 Tetrachloro-m-xylene

R.T.: 4.491 min
Delta R.T.: -0.003 min
Response: 2468345
Conc: 1.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH2650-2-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2023
Supervised By :Ankita Jodhani 11/13/2023

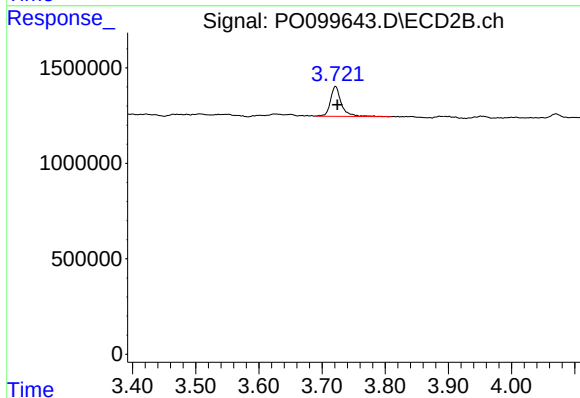


#1 Tetrachloro-m-xylene

R.T.: 3.721 min
Delta R.T.: -0.003 min
Response: 1859428
Conc: 1.53 ng/ml

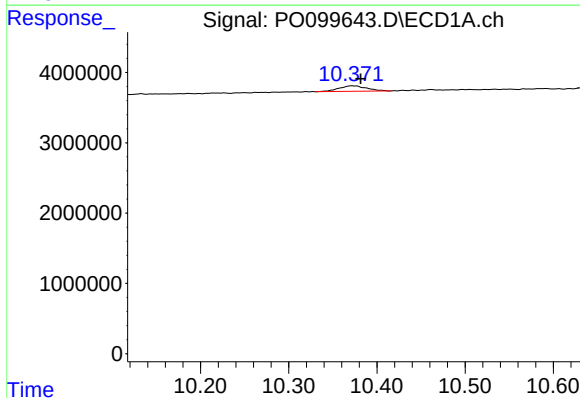

#2 Decachlorobiphenyl

R.T.: 10.373 min
Delta R.T.: -0.009 min
Response: 1702093
Conc: 2.67 ng/ml

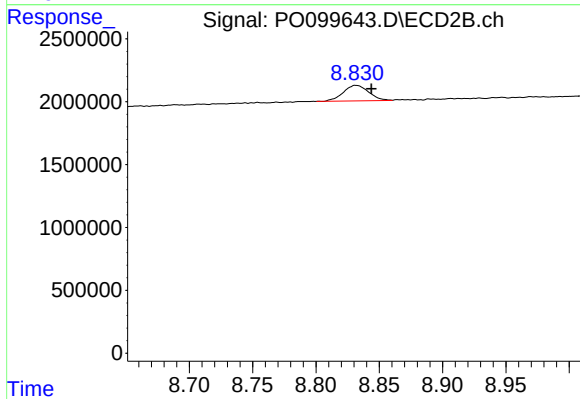

#2 Decachlorobiphenyl

R.T.: 8.832 min
Delta R.T.: -0.012 min
Response: 1737953
Conc: 2.37 ng/ml