

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0111119\
 Data File : P0063632.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2019 19:07
 Operator : SM/AJ
 Sample : K5763-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP-34-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:39:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0110719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 04:54:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.320	3.575	770207	559308	23.276	26.527
2)	SA Decachlor...	9.947	8.550	733083	461823	13.360	15.580
Target Compounds							
27)	L6 AR-1254-2	6.554	0.000	85584	0	30.963	N.D. #
34)	L7 AR-1260-4	7.928	0.000	252760	0	91.079	N.D. #
35)	L7 AR-1260-5	8.218	7.144	48250	151738	8.697	45.042 #
37)	L8 AR-1262-2	8.218	7.144	48250	151738	8.053	42.863 #
38)	L8 AR-1262-3	0.000	7.431	0	29395	N.D.	21.168 #
39)	L8 AR-1262-4	0.000	7.540	0	48603	N.D.	18.561 #
41)	L9 AR-1268-1	0.000	7.431	0	29395	N.D.	7.233 #
42)	L9 AR-1268-2	0.000	7.540	0	48603	N.D.	13.191 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111119\
Data File : PO063632.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2019 19:07
Operator : SM/AJ
Sample : K5763-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-34-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:39:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

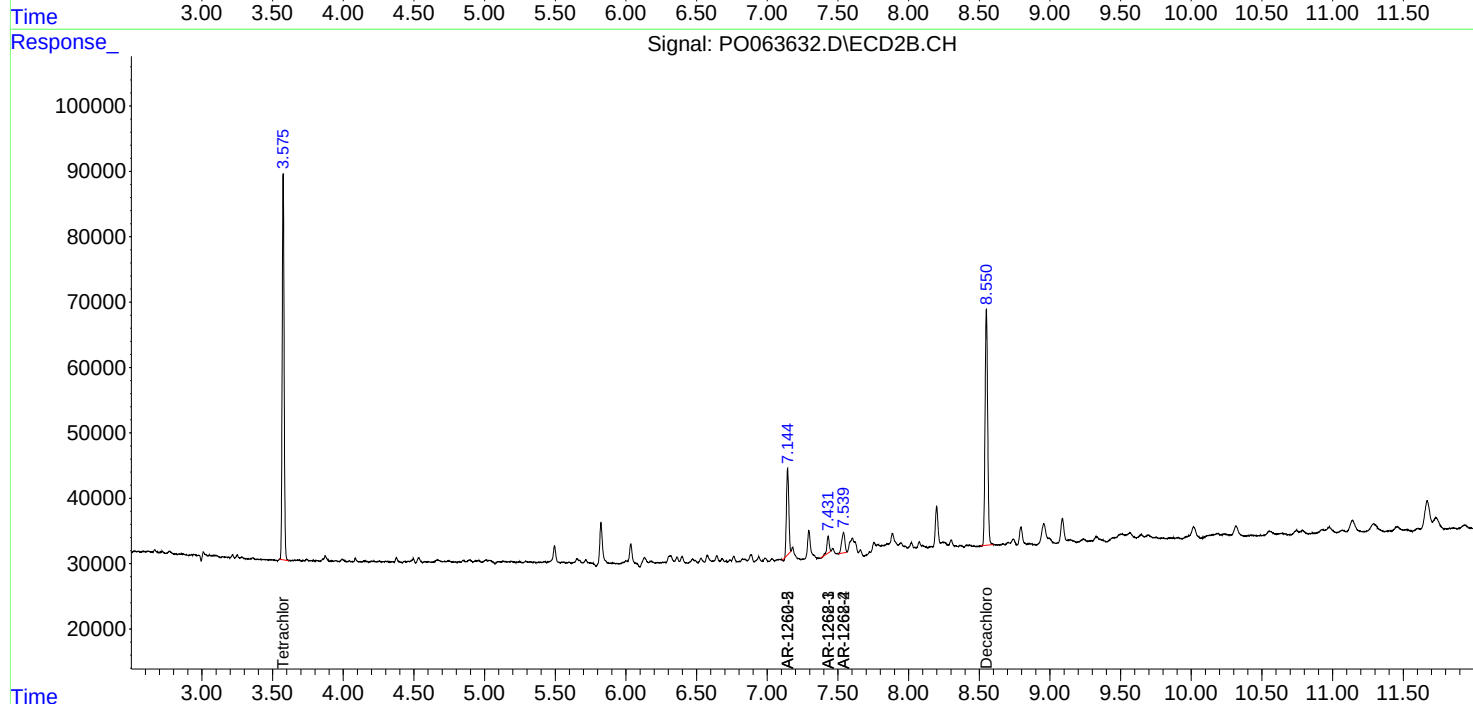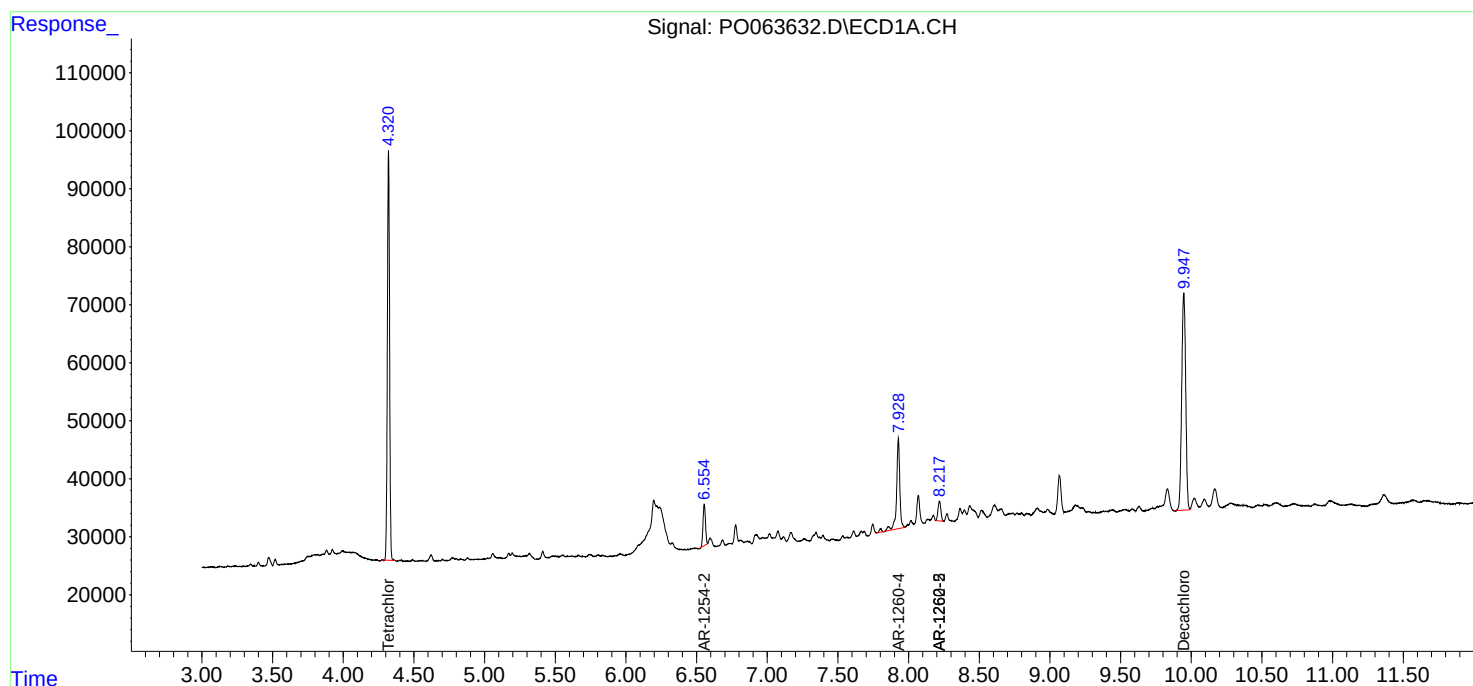


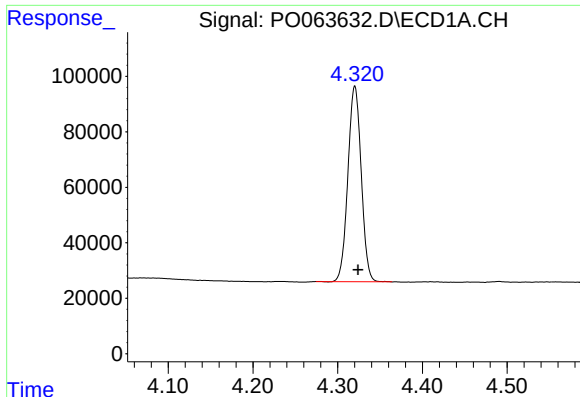

#1 Tetrachloro-m-xylene


R.T.: 4.320 min
Delta R.T.: -0.004 min
Response: 770207
Conc: 23.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-34-S

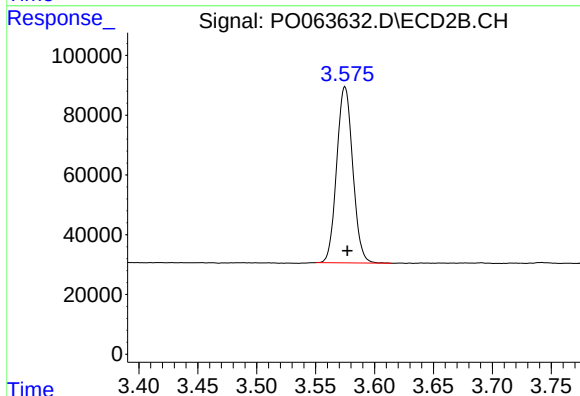


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: -0.002 min
Response: 559308
Conc: 26.53 ng/ml

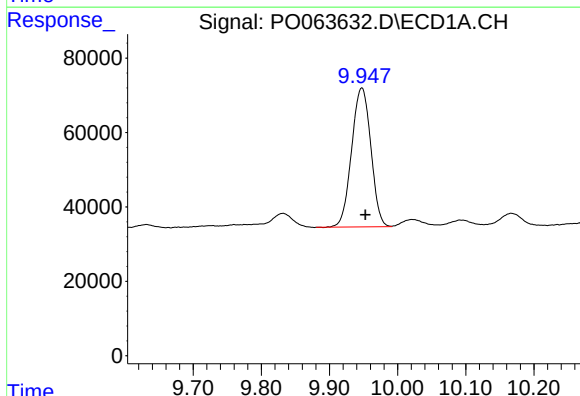


#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.005 min
Response: 733083
Conc: 13.36 ng/ml

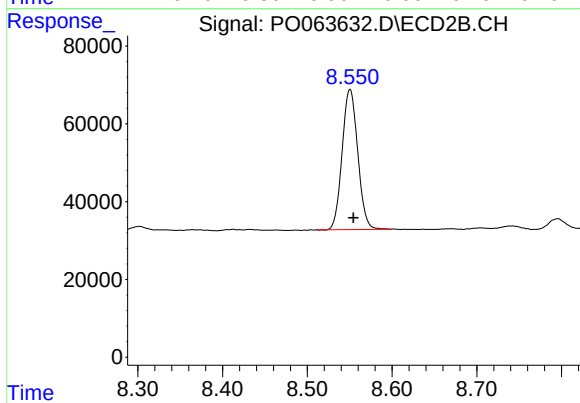

#2 Decachlorobiphenyl


R.T.: 8.550 min
Delta R.T.: -0.004 min
Response: 461823
Conc: 15.58 ng/ml

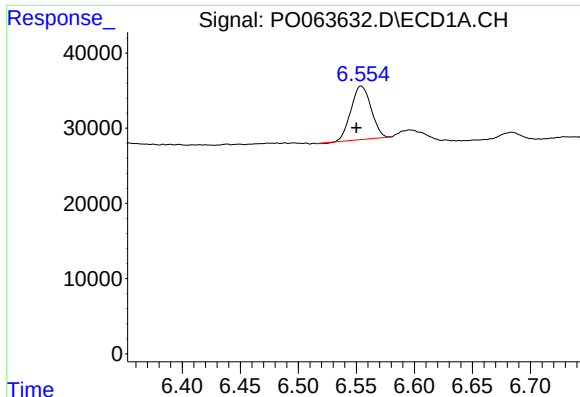

#27 AR-1254-2


R.T.: 6.554 min
Delta R.T.: 0.004 min
Response: 85584
Conc: 30.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-34-S

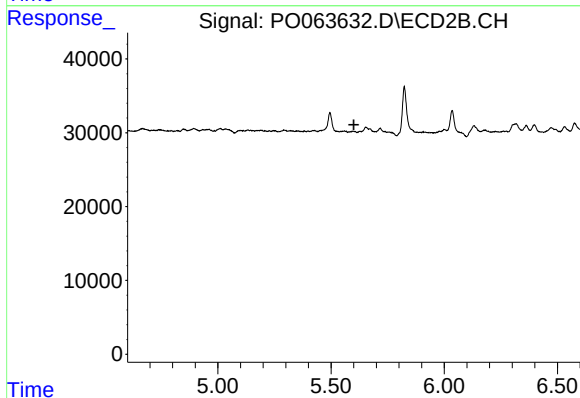


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.600 min
Response: 0
Conc: N.D.

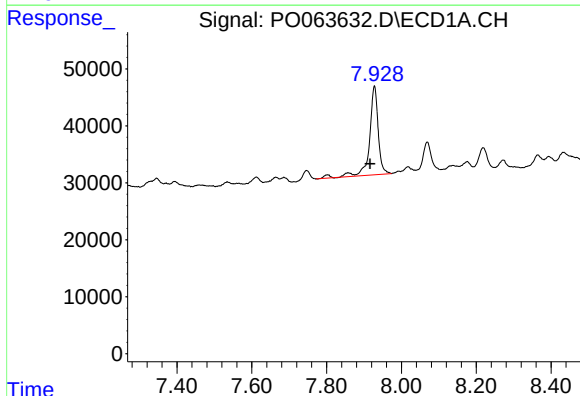


#34 AR-1260-4

R.T.: 7.928 min
Delta R.T.: 0.012 min
Response: 252760
Conc: 91.08 ng/ml

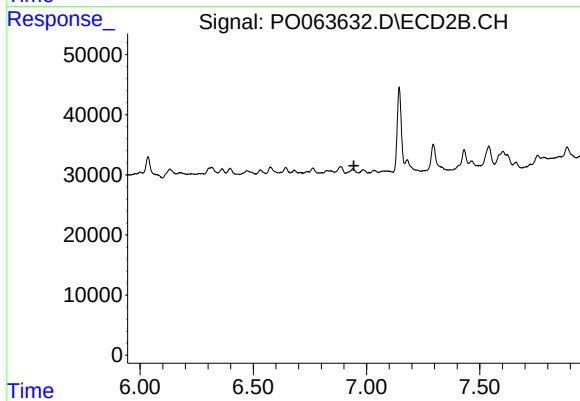

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 6.944 min
Response: 0
Conc: N.D.

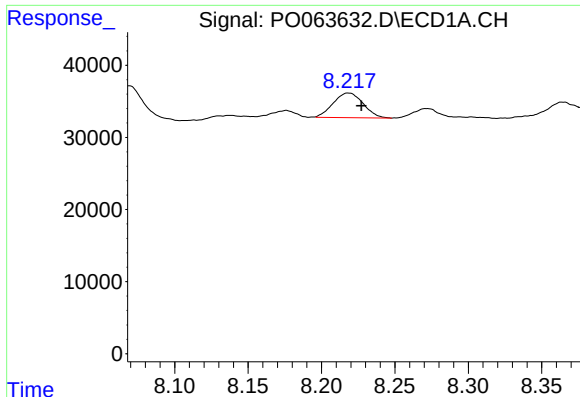

#35 AR-1260-5


R.T.: 8.218 min
Delta R.T.: -0.009 min
Response: 48250
Conc: 8.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-34-S

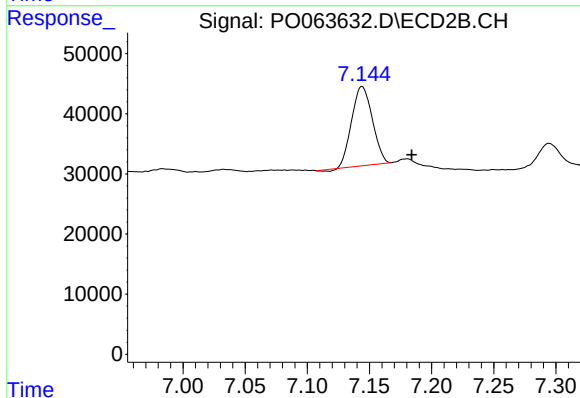


#35 AR-1260-5

R.T.: 7.144 min
Delta R.T.: -0.040 min
Response: 151738
Conc: 45.04 ng/ml

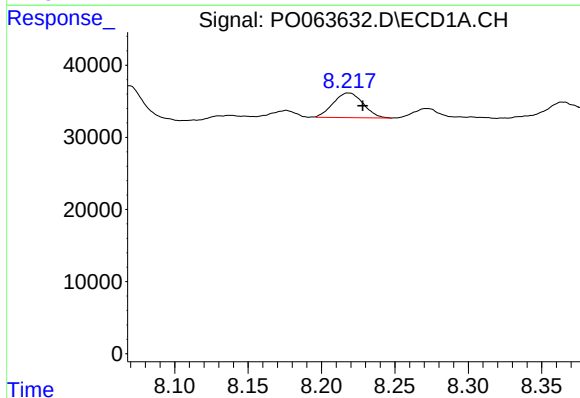


#37 AR-1262-2

R.T.: 8.218 min
Delta R.T.: -0.010 min
Response: 48250
Conc: 8.05 ng/ml

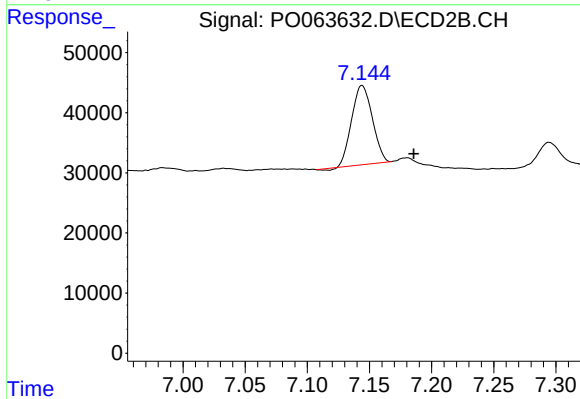

#37 AR-1262-2


R.T.: 7.144 min
Delta R.T.: -0.042 min
Response: 151738
Conc: 42.86 ng/ml

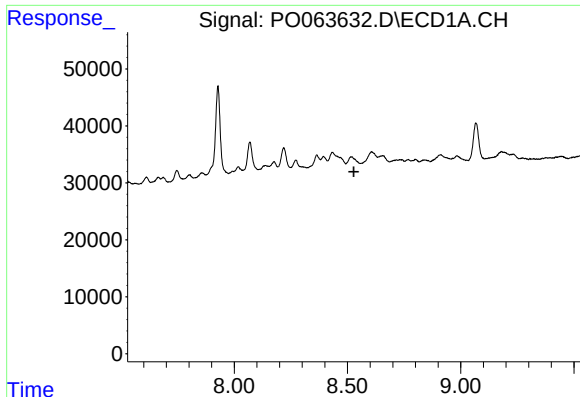

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-34-S

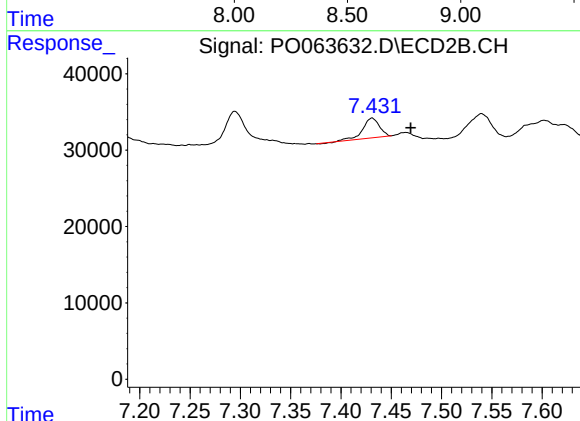


#38 AR-1262-3

R.T.: 7.431 min
Delta R.T.: -0.038 min
Response: 29395
Conc: 21.17 ng/ml

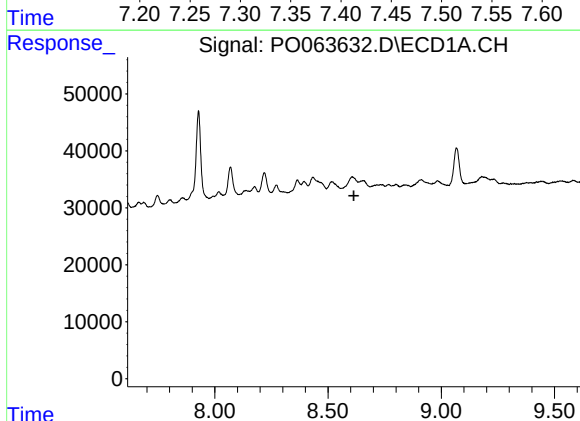


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.614 min
Response: 0
Conc: N.D.

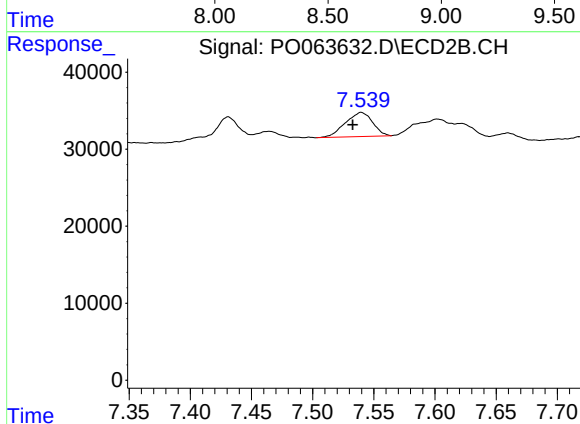

#39 AR-1262-4


R.T.: 7.540 min
Delta R.T.: 0.007 min
Response: 48603
Conc: 18.56 ng/ml

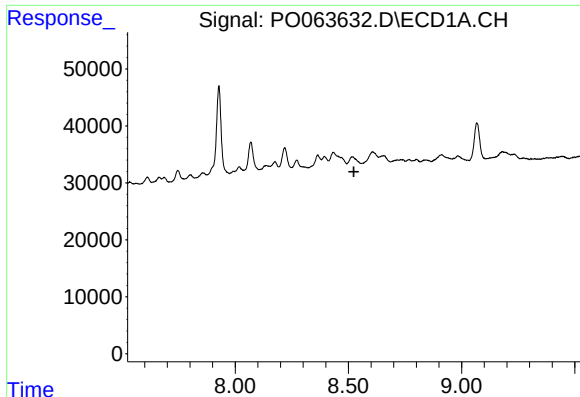

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-34-S

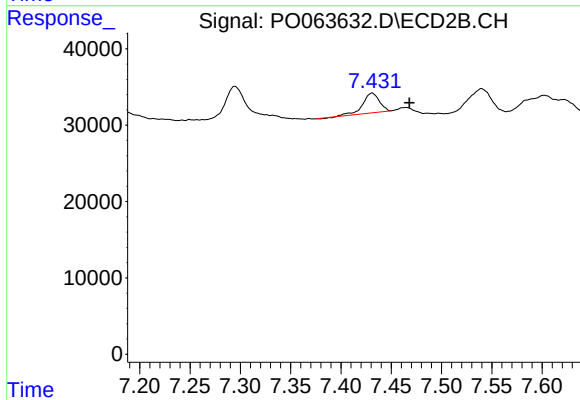


#41 AR-1268-1

R.T.: 7.431 min
Delta R.T.: -0.037 min
Response: 29395
Conc: 7.23 ng/ml

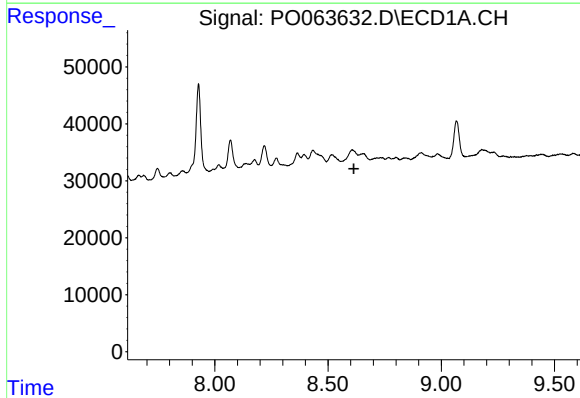

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.614 min
Response: 0
Conc: N.D.

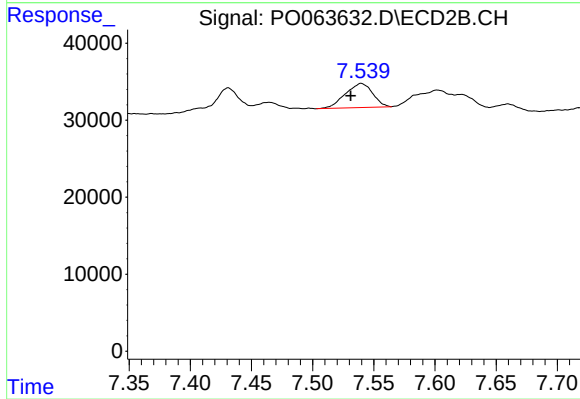

#42 AR-1268-2

R.T.: 7.540 min
Delta R.T.: 0.009 min
Response: 48603
Conc: 13.19 ng/ml