

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111119\
 Data File : PO063611.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2019 12:44
 Operator : SM/AJ
 Sample : K5765-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-009-IDWGW-20191107

Manual Integrations
 APPROVED

Ankita
 11/12/2019 11:51:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 13:34:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 04:54:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.575	456801	312742	13.805	14.833
2) SA Decachlor...	9.945	8.549	167214	103489	3.047	3.491m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111119\
Data File : PO063611.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2019 12:44
Operator : SM/AJ
Sample : K5765-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TT-009-IDWGW-20191107


Manual Integrations
APPROVED

Ankita
11/12/2019 11:51:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 13:34:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

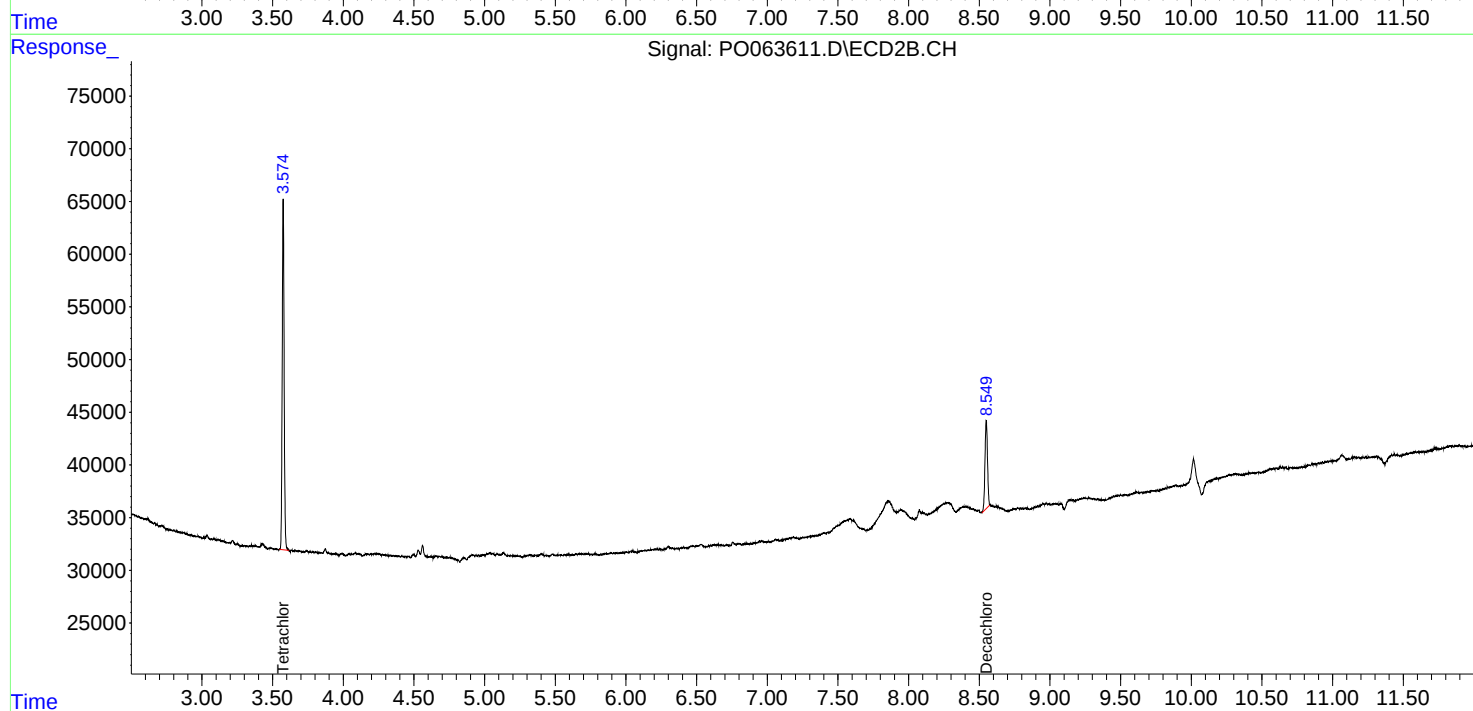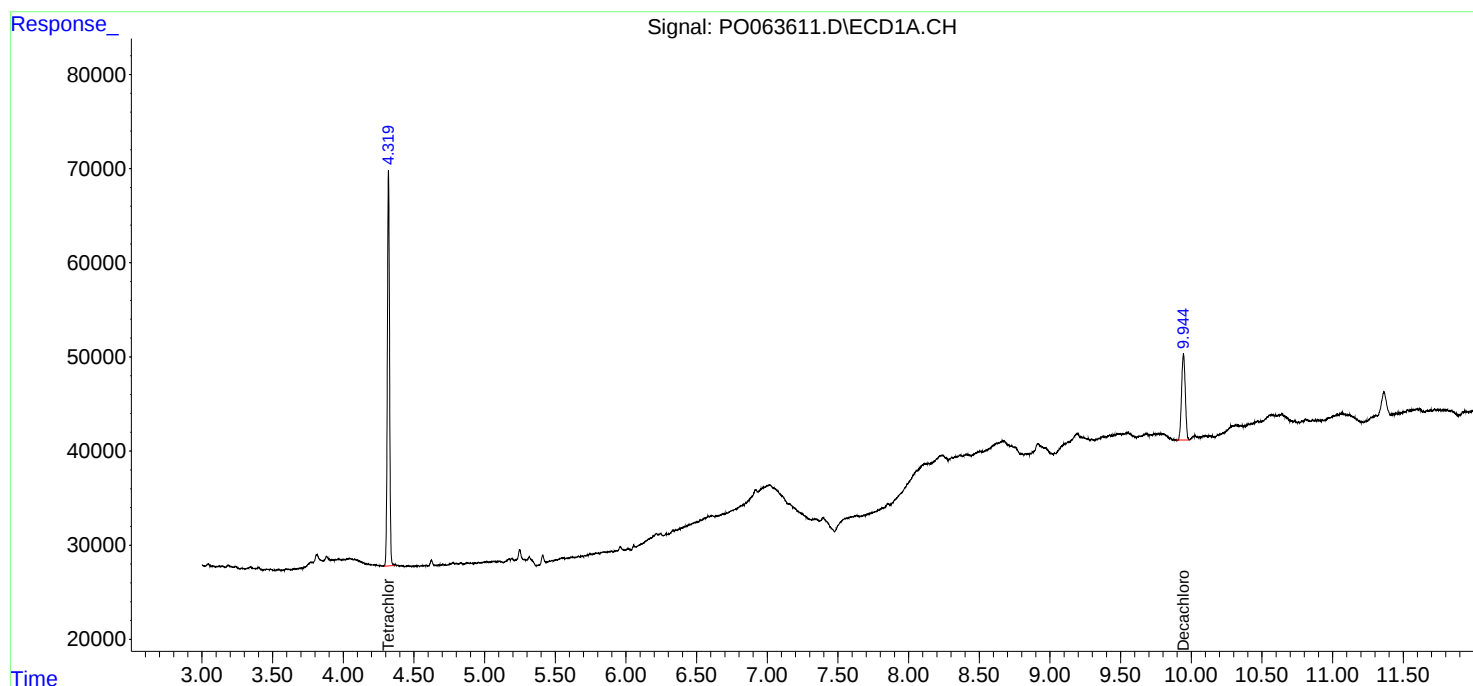

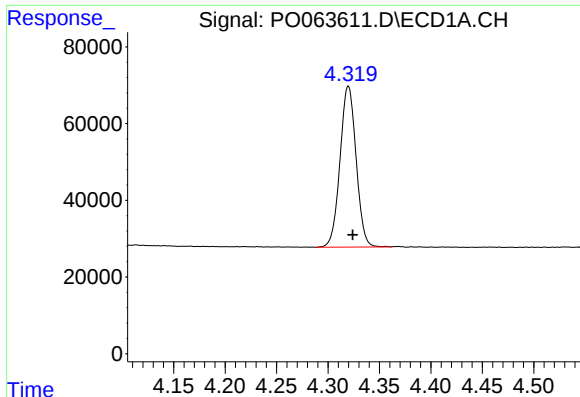


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: -0.004 min
Response: 456801
Conc: 13.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-009-IDW/GW-20191107


Manual Integrations
APPROVED

Ankita
11/12/2019 11:51:52 AM

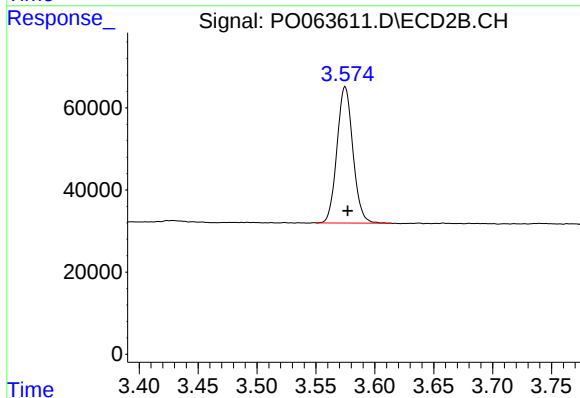


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: -0.002 min
Response: 312742
Conc: 14.83 ng/ml

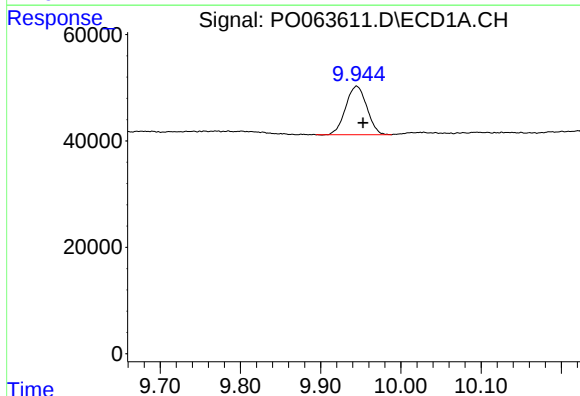

#2 Decachlorobiphenyl

R.T.: 9.945 min
Delta R.T.: -0.008 min
Response: 167214
Conc: 3.05 ng/ml

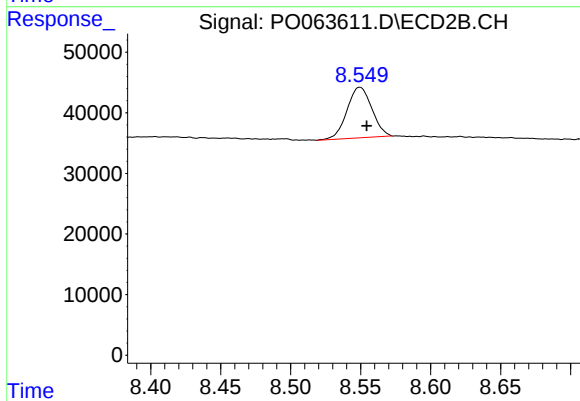

#2 Decachlorobiphenyl

R.T.: 8.549 min
Delta R.T.: -0.006 min
Response: 103489
Conc: 3.49 ng/ml m