

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111120\
 Data File : PO073228.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2020 15:02
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:13:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 10 11:30:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.947	4.019	1590932	940053	30.018	26.307
2)	SA Decachlor...	10.978	9.294	1116243	775109	26.974	23.233
Target Compounds							
24)	L5 AR-1248-4	7.184f	0.000	52431	0	21.686	N.D. #
26)	L6 AR-1254-1	7.184	0.000	52431	0	22.409	N.D. #
33)	L7 AR-1260-3	8.615f	0.000	634175	0	308.093	N.D. #
35)	L7 AR-1260-5	9.155	0.000	27455	0	6.224	N.D. #
36)	L8 AR-1262-1	8.615f	0.000	634175	0	186.094	N.D. #
37)	L8 AR-1262-2	9.155	0.000	27455	0	4.729	N.D. #
45)	L9 AR-1268-5	10.634	0.000	49574	0	2.880	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111120\
Data File : PO073228.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2020 15:02
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:13:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 10 11:30:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

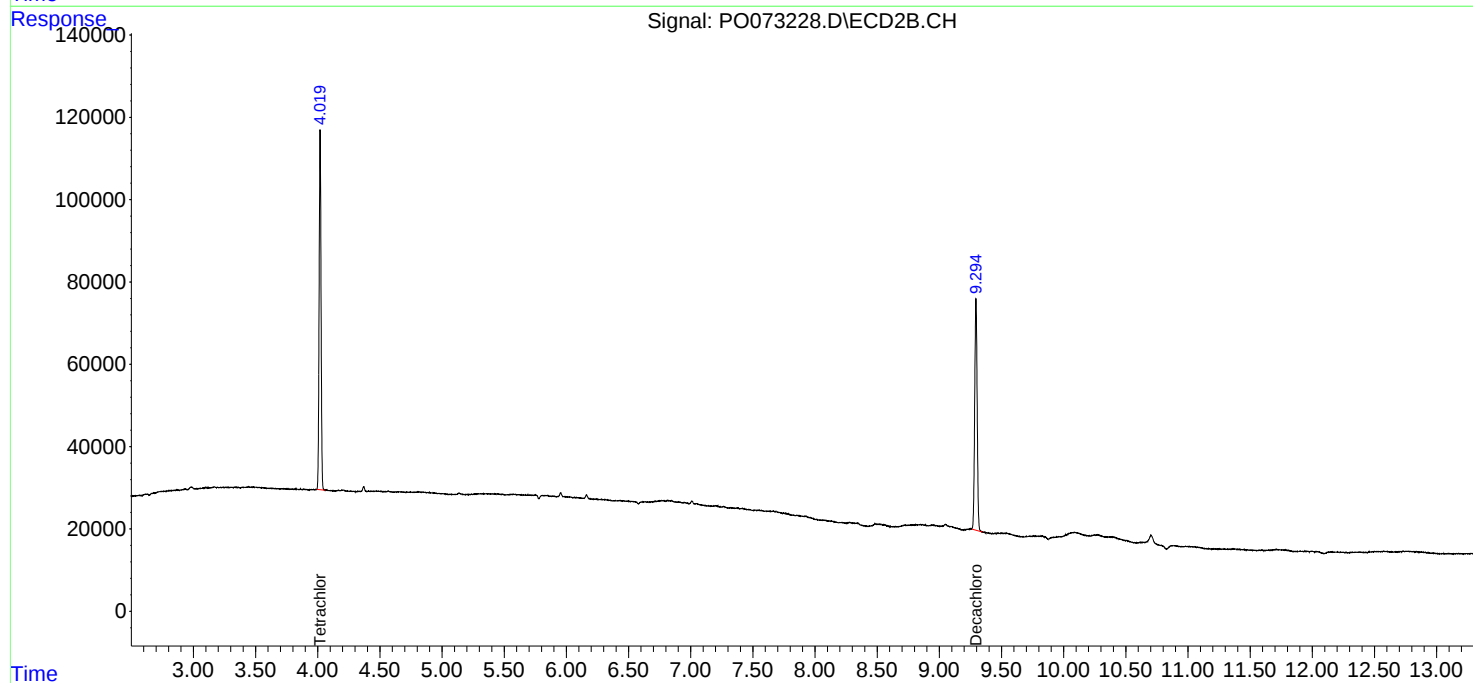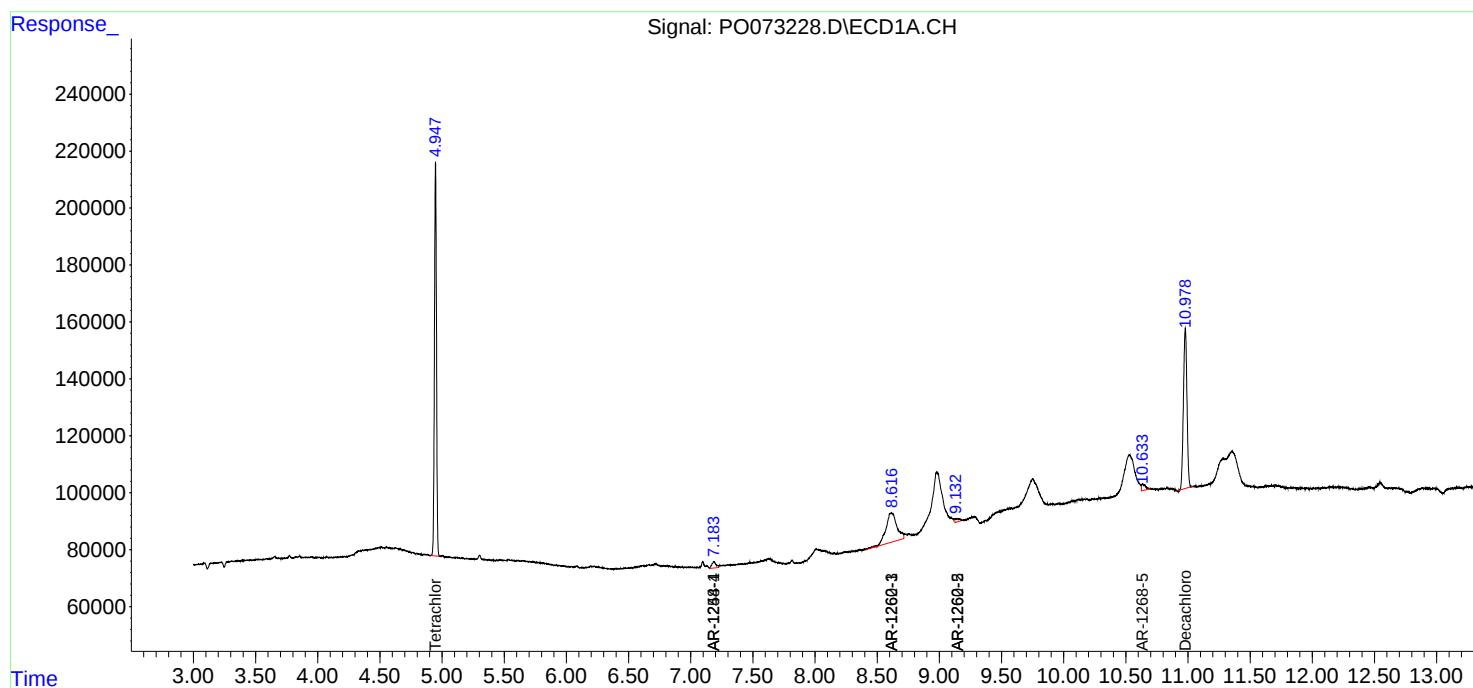


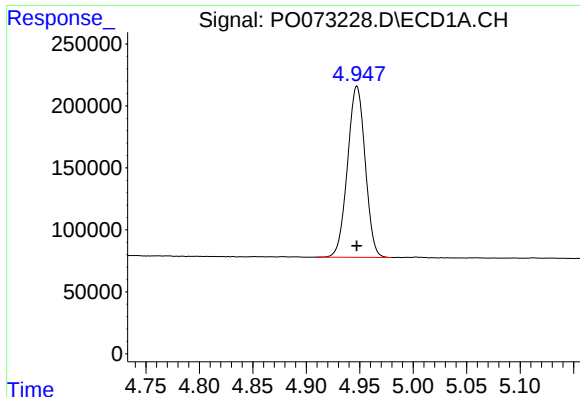

#1 Tetrachloro-m-xylene


R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 1590932
Conc: 30.02 ng/ml

Instrument :
ECD_O
ClientSampleId :

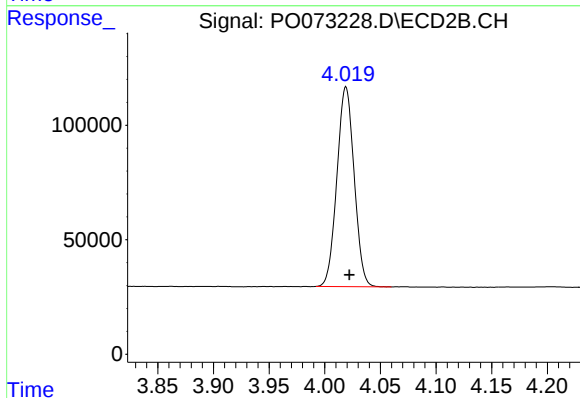


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.003 min
Response: 940053
Conc: 26.31 ng/ml

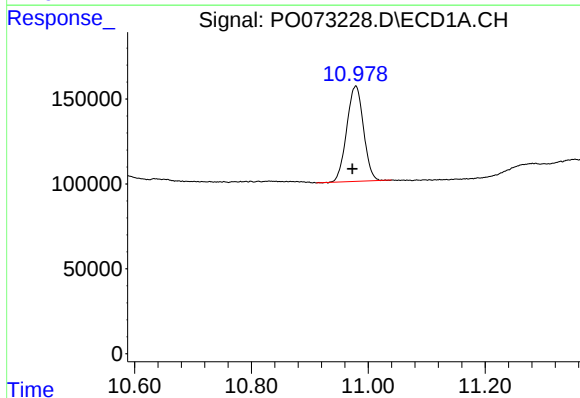


#2 Decachlorobiphenyl

R.T.: 10.978 min
Delta R.T.: 0.006 min
Response: 1116243
Conc: 26.97 ng/ml

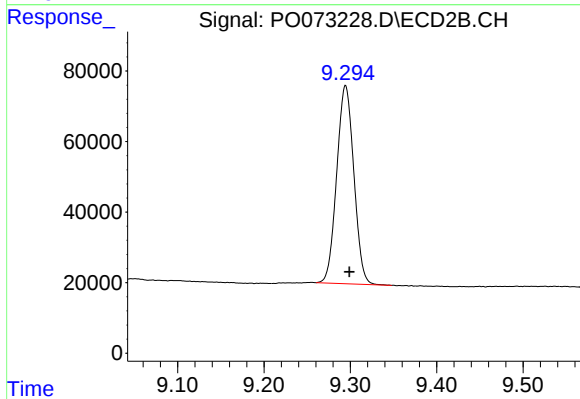

#2 Decachlorobiphenyl


R.T.: 9.294 min
Delta R.T.: -0.004 min
Response: 775109
Conc: 23.23 ng/ml

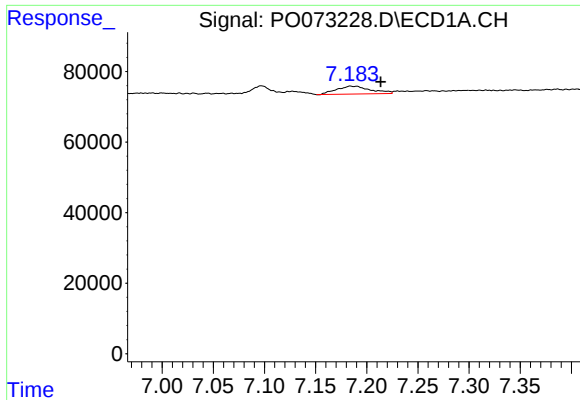

#24 AR-1248-4


R.T.: 7.184 min
Delta R.T.: -0.029 min
Response: 52431
Conc: 21.69 ng/ml

Instrument :
ECD_O
ClientSampleId :

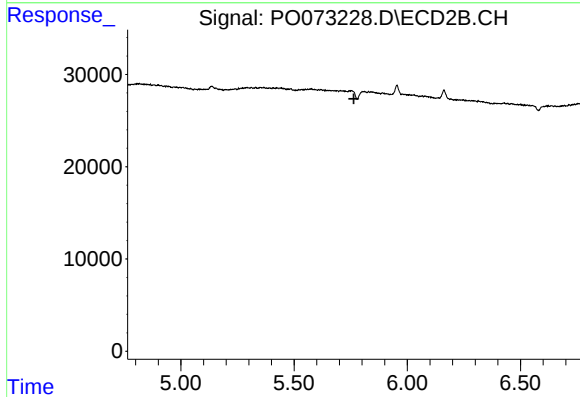


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.764 min
Response: 0
Conc: N.D.

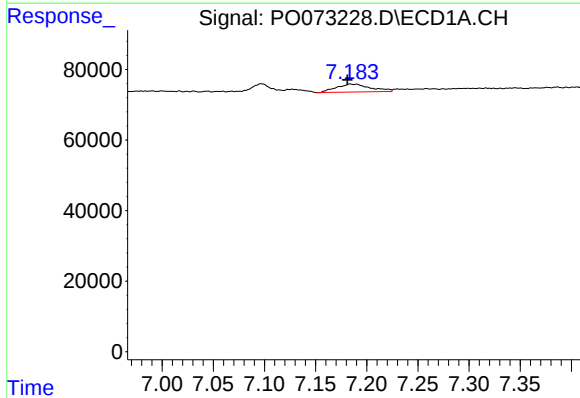


#26 AR-1254-1

R.T.: 7.184 min
Delta R.T.: 0.003 min
Response: 52431
Conc: 22.41 ng/ml

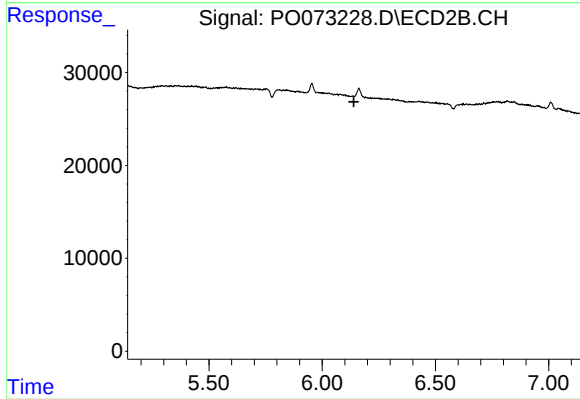

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

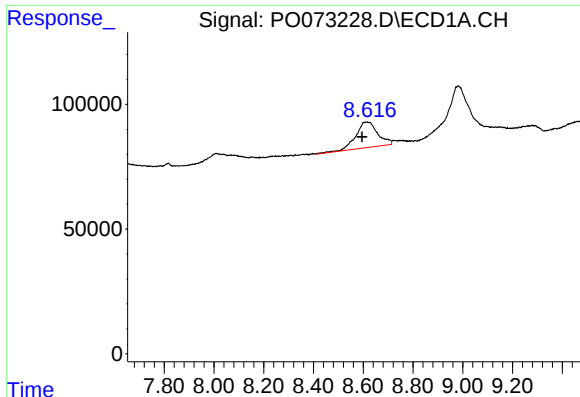

#33 AR-1260-3


R.T.: 8.615 min
Delta R.T.: 0.020 min
Response: 634175
Conc: 308.09 ng/ml

Instrument :
ECD_O
ClientSampleId :

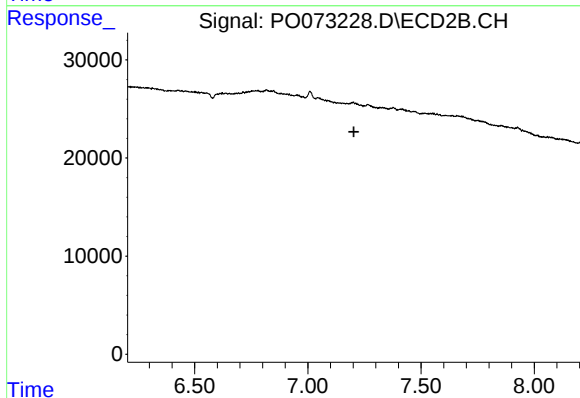


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

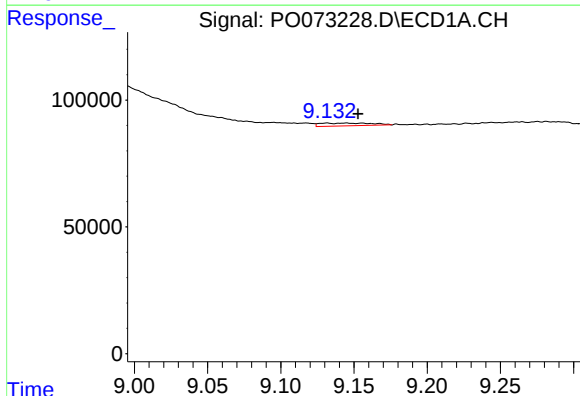


#35 AR-1260-5

R.T.: 9.155 min
Delta R.T.: 0.002 min
Response: 27455
Conc: 6.22 ng/ml

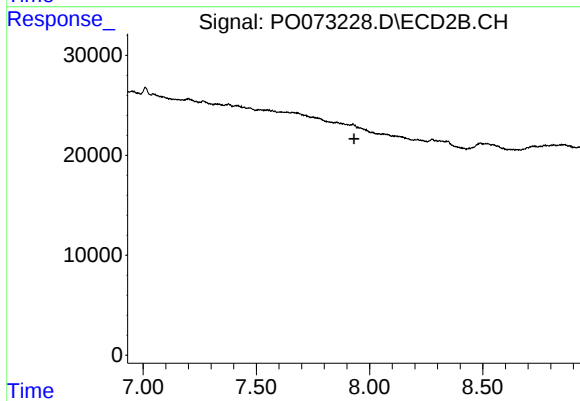

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.931 min
Response: 0
Conc: N.D.

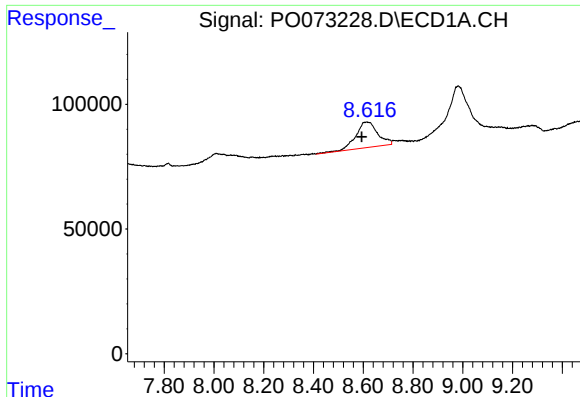

#36 AR-1262-1


R.T.: 8.615 min
Delta R.T.: 0.020 min
Response: 634175
Conc: 186.09 ng/ml

Instrument :
ECD_O
ClientSampleId :

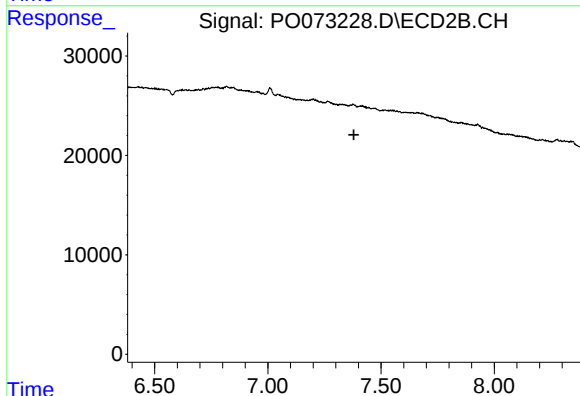


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.380 min
Response: 0
Conc: N.D.

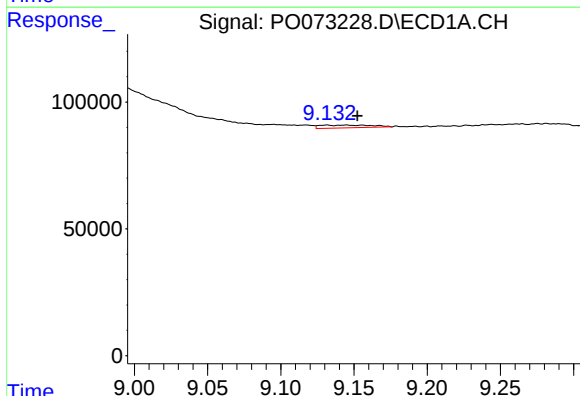


#37 AR-1262-2

R.T.: 9.155 min
Delta R.T.: 0.003 min
Response: 27455
Conc: 4.73 ng/ml

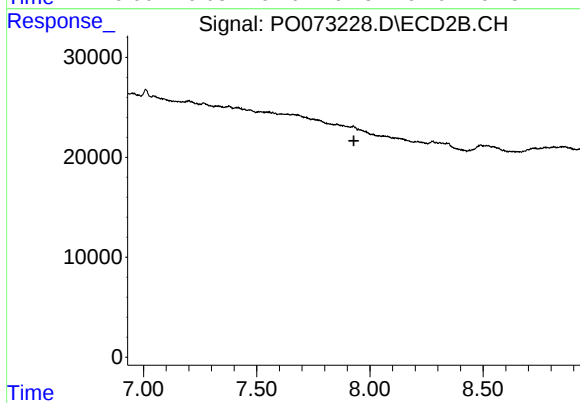

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.929 min
Response: 0
Conc: N.D.

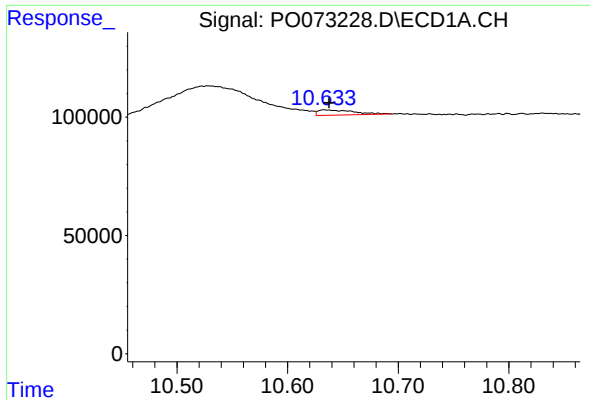

#45 AR-1268-5

R.T.: 10.634 min
Delta R.T.: -0.003 min
Response: 49574
Conc: 2.88 ng/ml

Instrument :
ECD_O
ClientSampleId :

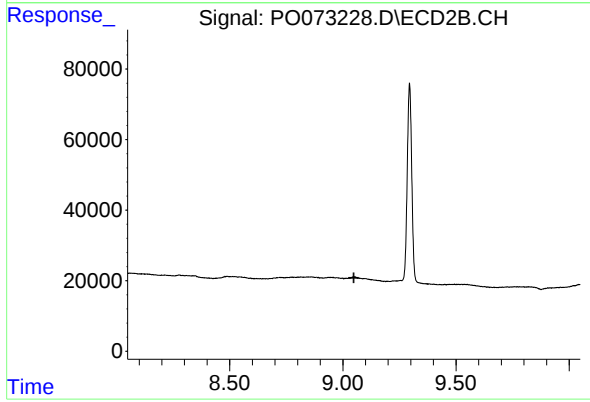

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.049 min
Response: 0
Conc: N.D.