

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111122\
 Data File : PO090508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2022 20:22
 Operator : YP/AJ
 Sample : N5552-01 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MOO-2022-40A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2022
 Supervised By :Ankita Jodhani 11/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 01:56:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.305	3.483	5820278	1764838	1.811	1.661
2) SA Decachlor...	10.058	8.491	4326427	1670022	1.765m	1.621m
Target Compounds						
26) L6 AR-1254-1	6.342	5.374	2634083	1100051	22.728m	18.675m
27) L6 AR-1254-2	6.562	5.520	3406599	697099	19.586m	13.010m#
28) L6 AR-1254-3	6.930	5.927	3469462	1672943	19.985m	20.184m
29) L6 AR-1254-4	7.218	6.157	2458670	1103897	19.289m	22.227m
30) L6 AR-1254-5	7.640	6.578	3062886	1828432	21.744m	24.420

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111122\
Data File : PO090508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2022 20:22
Operator : YP/AJ
Sample : N5552-01 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MOO-2022-40A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2022
Supervised By :Ankita Jodhani 11/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 01:56:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

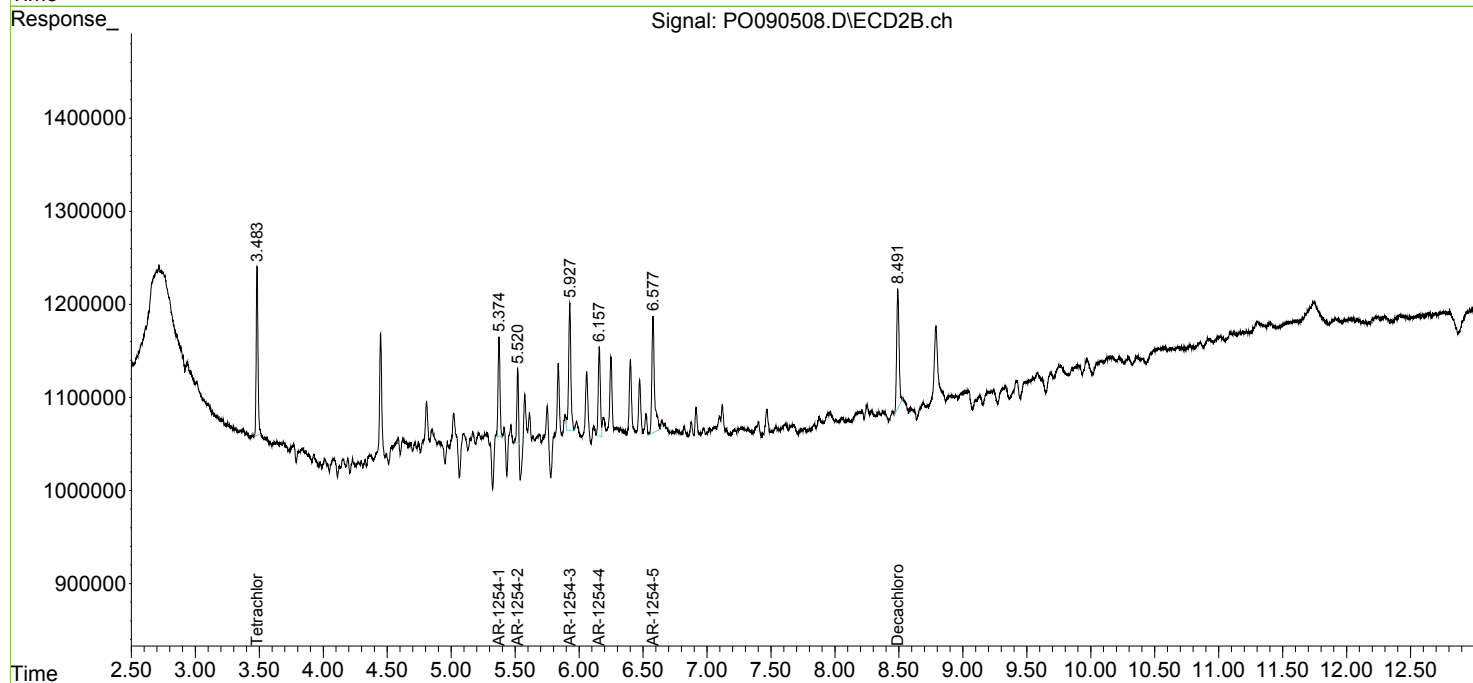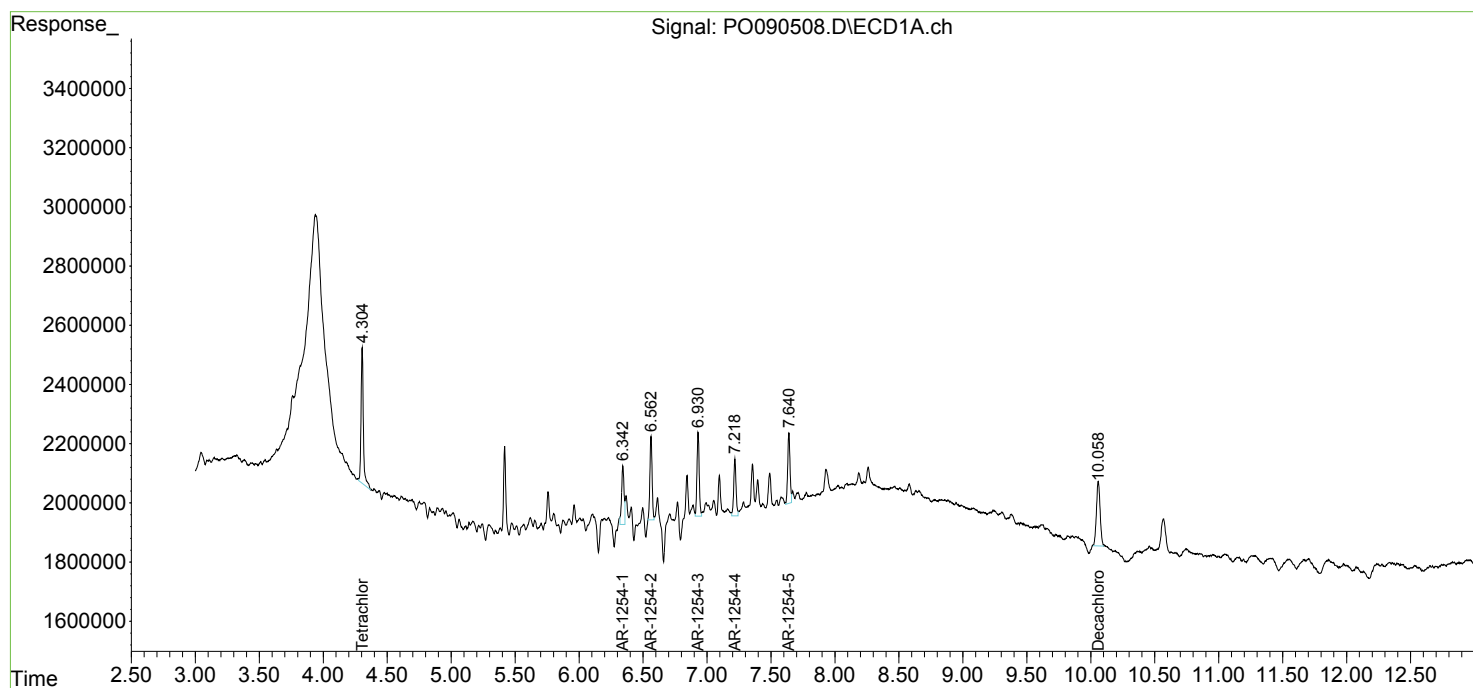

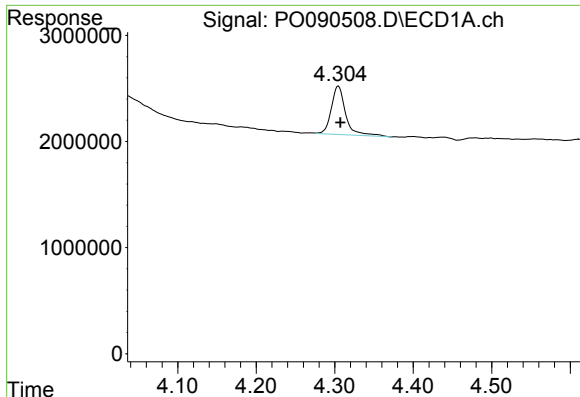


#1 Tetrachloro-m-xylene

R.T.: 4.305 min
Delta R.T.: -0.002 min
Response: 5820278
Conc: 1.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2022-40A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2022
Supervised By :Ankita Jodhani 11/14/2022

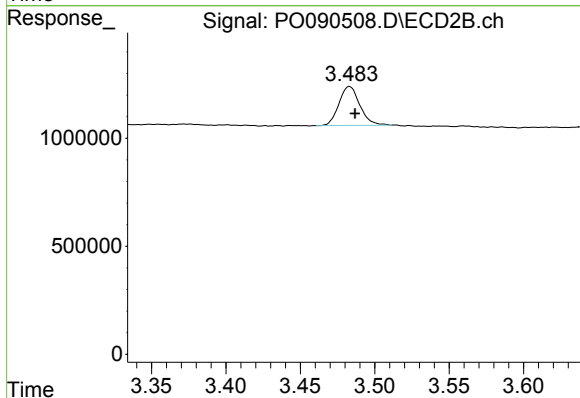


#1 Tetrachloro-m-xylene

R.T.: 3.483 min
Delta R.T.: -0.004 min
Response: 1764838
Conc: 1.66 ng/ml

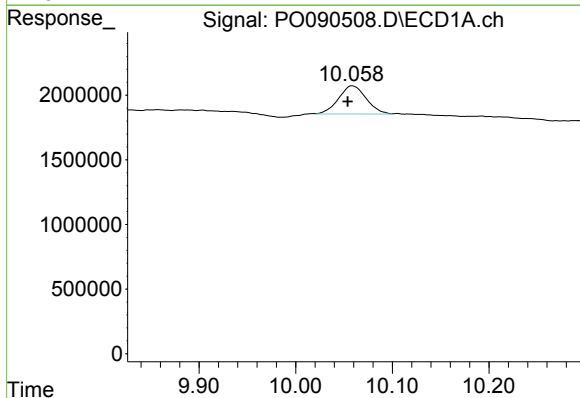


#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: 0.004 min
Response: 4326427
Conc: 1.77 ng/ml m

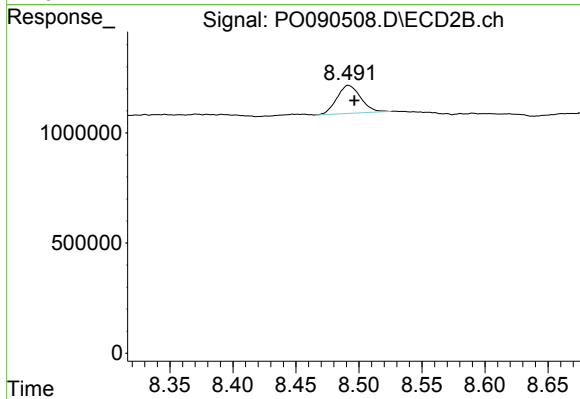

#2 Decachlorobiphenyl

R.T.: 8.491 min
Delta R.T.: -0.006 min
Response: 1670022
Conc: 1.62 ng/ml m

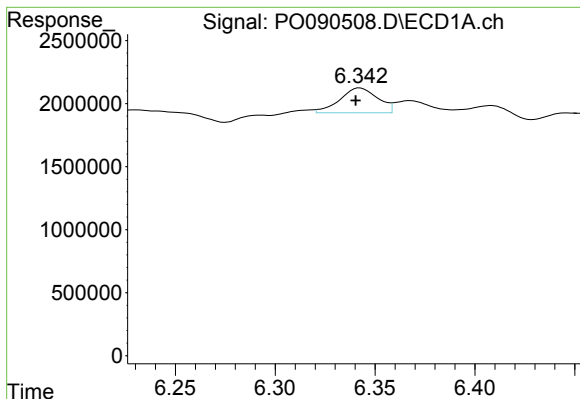


#26 AR-1254-1

R.T.: 6.342 min
Delta R.T.: 0.001 min
Response: 2634083
Conc: 22.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2022-40A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2022
Supervised By :Ankita Jodhani 11/14/2022

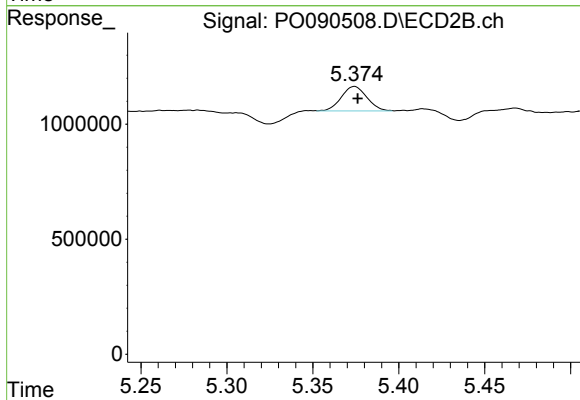


#26 AR-1254-1

R.T.: 5.374 min
Delta R.T.: -0.002 min
Response: 1100051
Conc: 18.67 ng/ml m

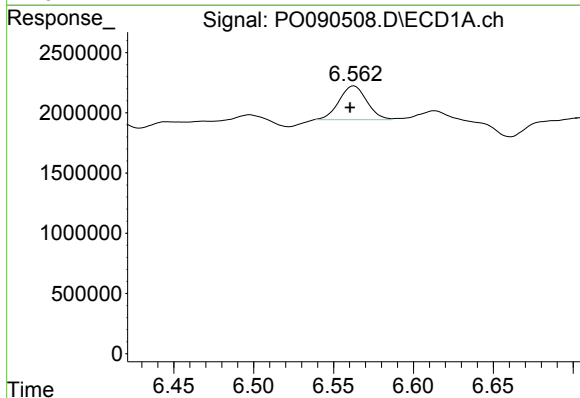


#27 AR-1254-2

R.T.: 6.562 min
Delta R.T.: 0.002 min
Response: 3406599
Conc: 19.59 ng/ml m

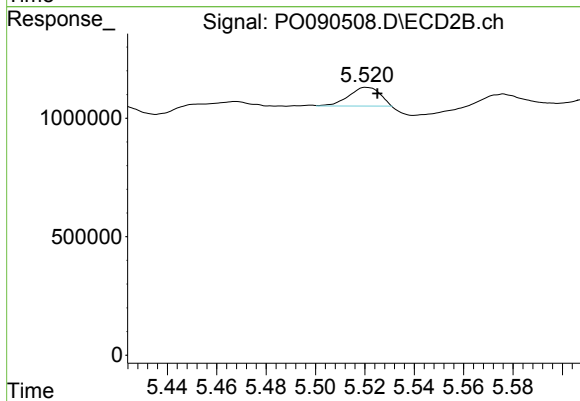

#27 AR-1254-2

R.T.: 5.520 min
Delta R.T.: -0.005 min
Response: 697099
Conc: 13.01 ng/ml m

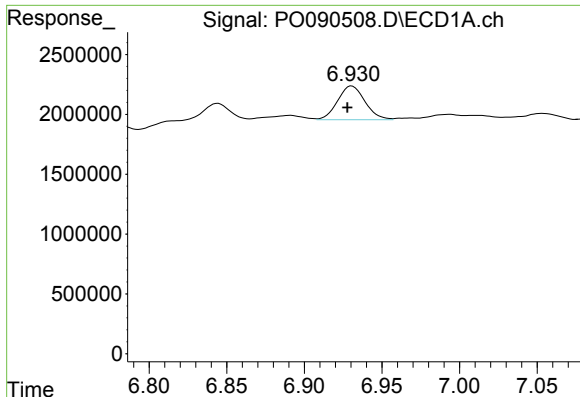


#28 AR-1254-3

R.T.: 6.930 min
Delta R.T.: 0.002 min
Response: 3469462
Conc: 19.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2022-40A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2022
Supervised By :Ankita Jodhani 11/14/2022

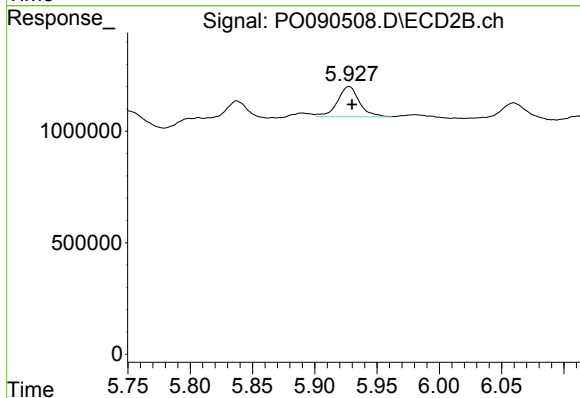


#28 AR-1254-3

R.T.: 5.927 min
Delta R.T.: -0.003 min
Response: 1672943
Conc: 20.18 ng/ml m

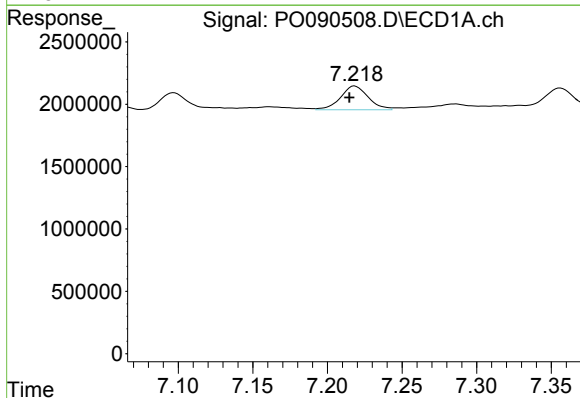


#29 AR-1254-4

R.T.: 7.218 min
Delta R.T.: 0.003 min
Response: 2458670
Conc: 19.29 ng/ml m

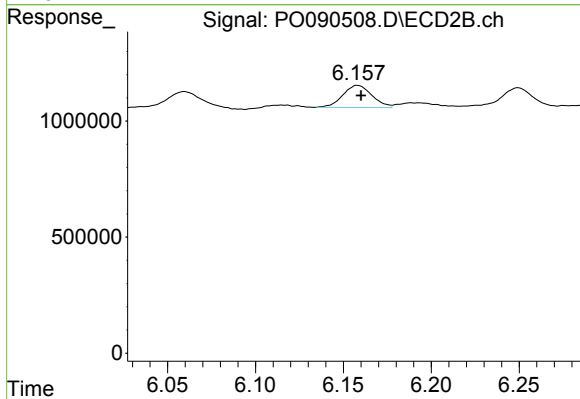

#29 AR-1254-4

R.T.: 6.157 min
Delta R.T.: -0.003 min
Response: 1103897
Conc: 22.23 ng/ml m

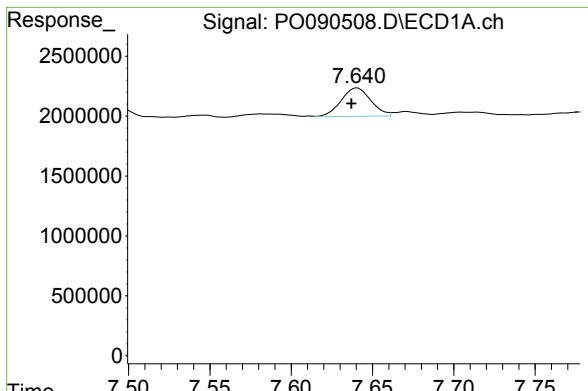


#30 AR-1254-5

R.T.: 7.640 min
Delta R.T.: 0.003 min
Response: 3062886
Conc: 21.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2022-40A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2022
Supervised By :Ankita Jodhani 11/14/2022

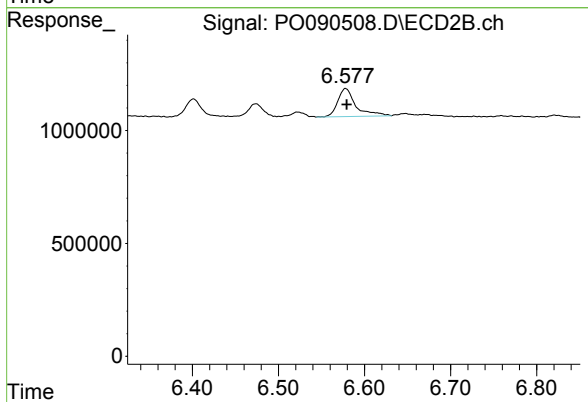

#30 AR-1254-5

R.T.: 6.578 min
Delta R.T.: -0.001 min
Response: 1828432
Conc: 24.42 ng/ml