

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111219\
 Data File : P0063655.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2019 13:56
 Operator : SM/AJ
 Sample : K5762-01RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HP-640RE

Manual Integrations
 APPROVED

Ankita
 11/13/2019 10:18:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 15:48:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 04:54:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.325	3.565	1285662	696849	38.853m	33.050m
2)	SA Decachlor...	9.947	8.549	266284	179857	4.853m	6.068 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111219\
Data File : PO063655.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2019 13:56
Operator : SM/AJ
Sample : K5762-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HP-640RE


Manual Integrations
APPROVED

Ankita
11/13/2019 10:18:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 15:48:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

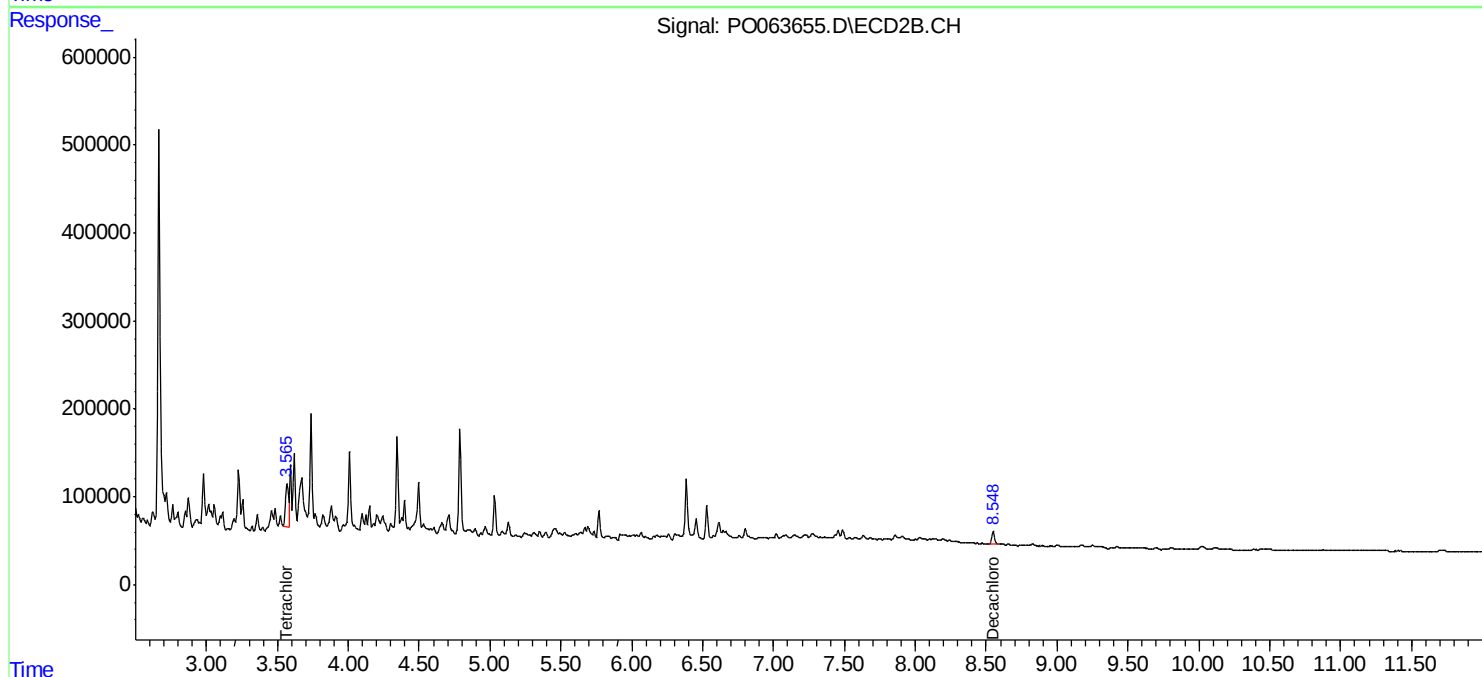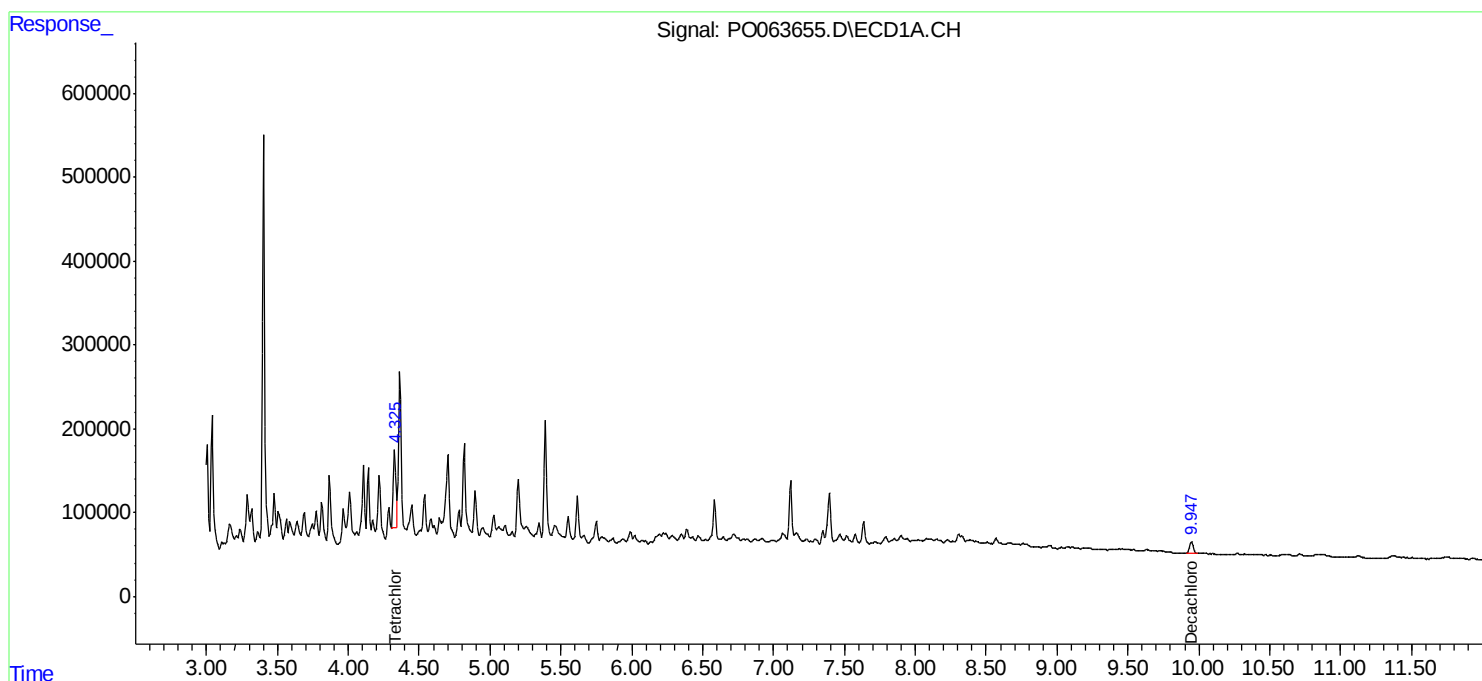

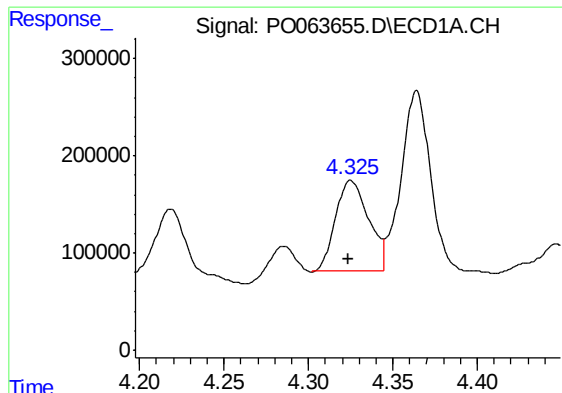


#1 Tetrachloro-m-xylene

R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 1285662
Conc: 38.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HP-640RE


Manual Integrations
APPROVED

Ankita
11/13/2019 10:18:36 AM

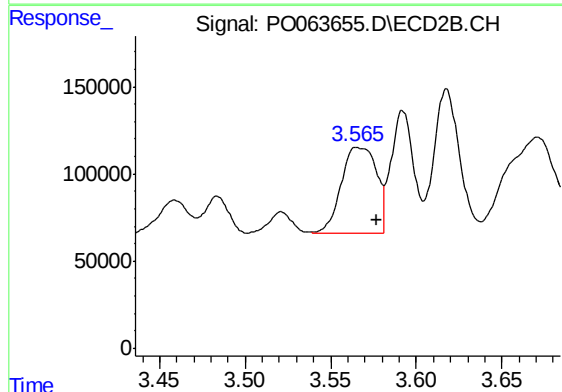


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.013 min
Response: 696849
Conc: 33.05 ng/ml m

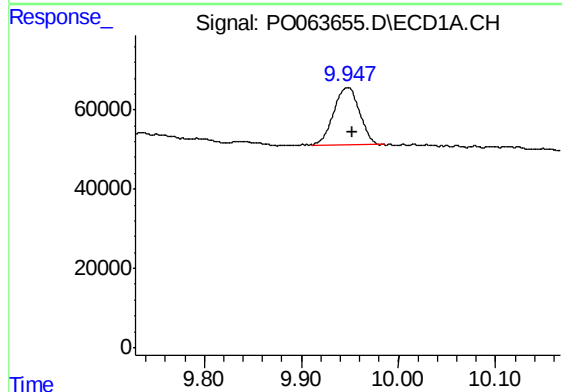

#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.005 min
Response: 266284
Conc: 4.85 ng/ml m

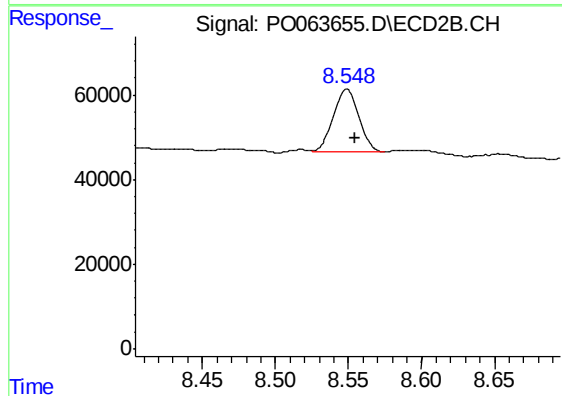

#2 Decachlorobiphenyl

R.T.: 8.549 min
Delta R.T.: -0.005 min
Response: 179857
Conc: 6.07 ng/ml