

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111219\
 Data File : P0063660.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2019 15:21
 Operator : SM/AJ
 Sample : K5670-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-111119

Manual Integrations
 APPROVED

Ankita
 11/13/2019 10:18:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 15:50:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 04:54:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.320	3.574	1098566	812963	33.199	38.557
2)	SA Decachlor...	9.946	8.549	941589	584896	17.160m	19.732

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111219\
Data File : PO063660.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2019 15:21
Operator : SM/AJ
Sample : K5670-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-11119


Manual Integrations
APPROVED

Ankita
11/13/2019 10:18:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 15:50:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110719.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 04:54:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

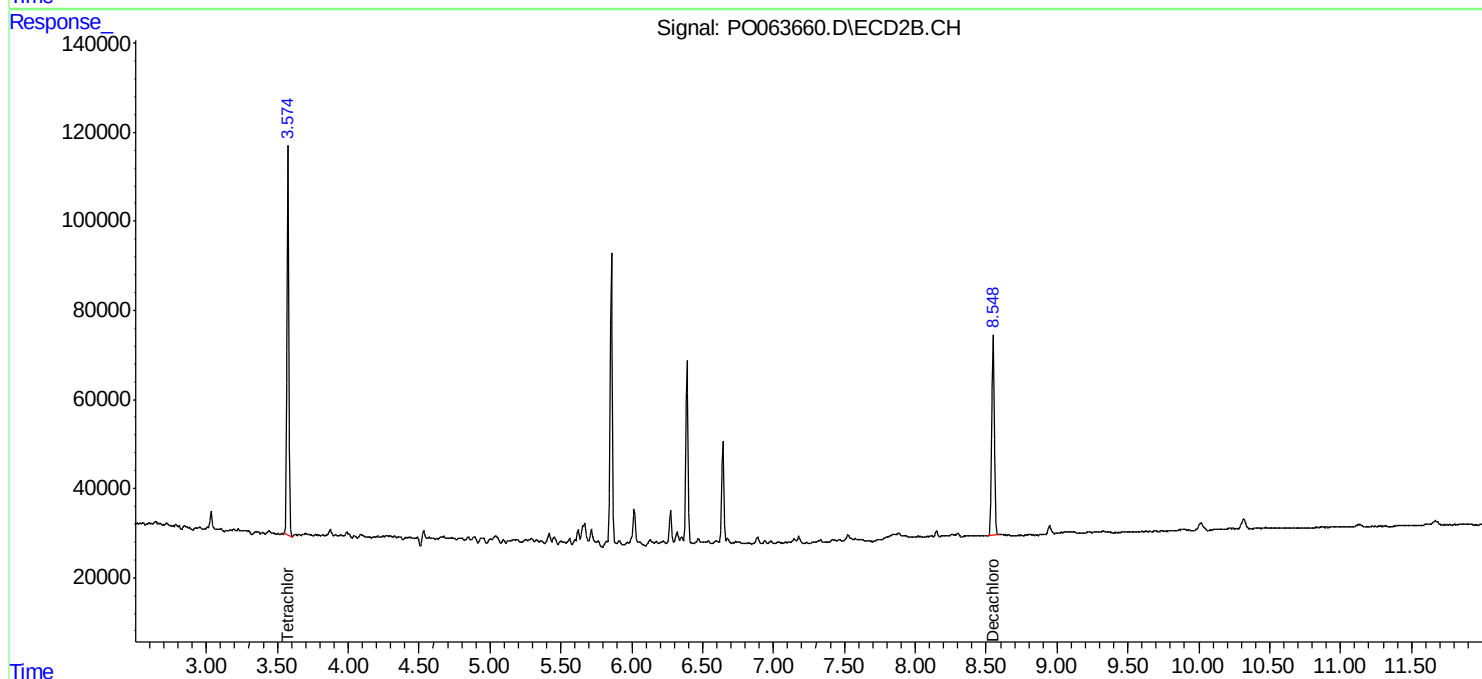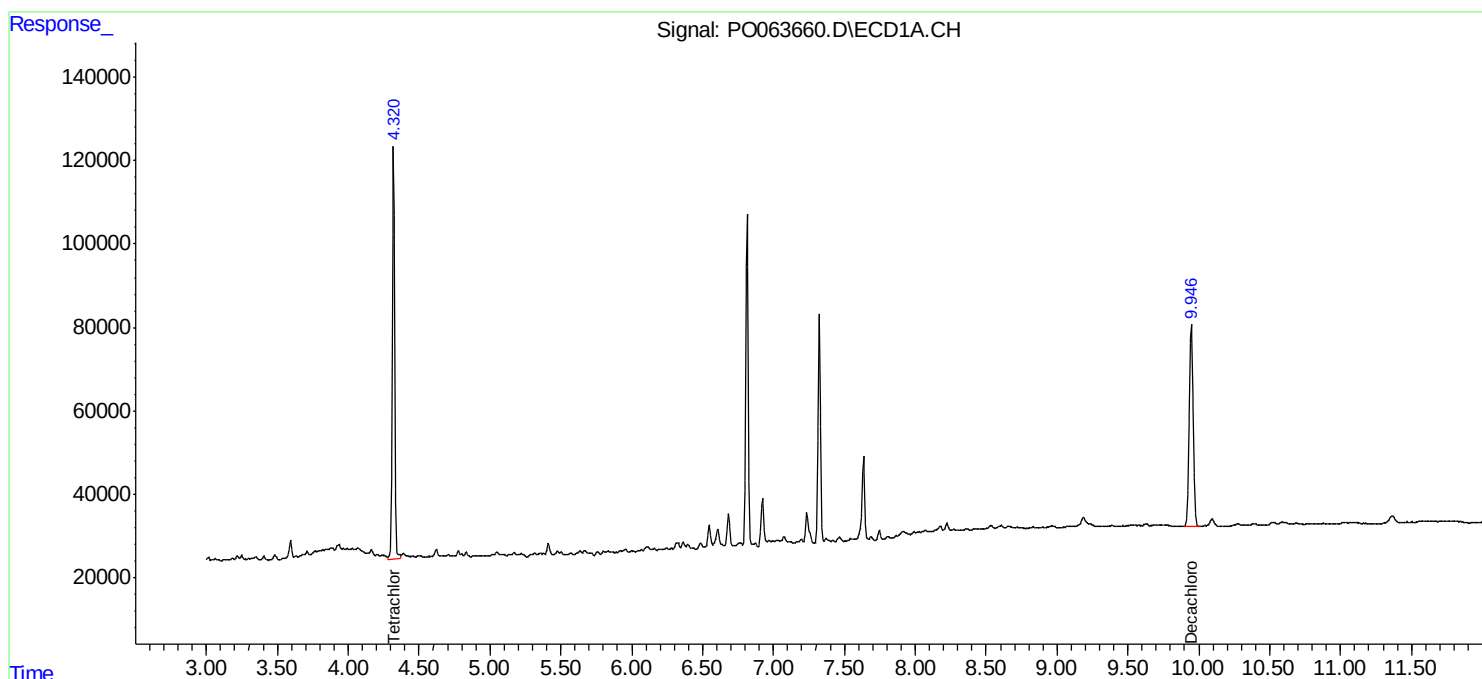

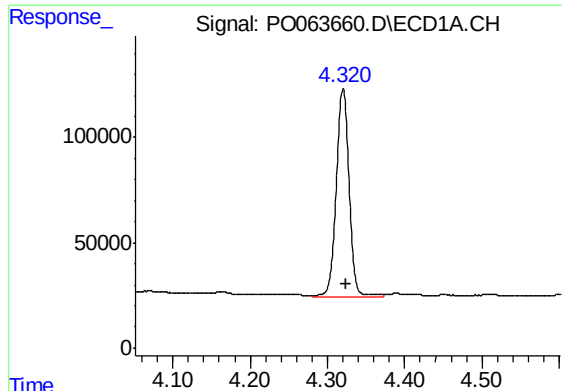


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: -0.004 min
Response: 1098566
Conc: 33.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-111119


Manual Integrations
APPROVED

Ankita
11/13/2019 10:18:57 AM

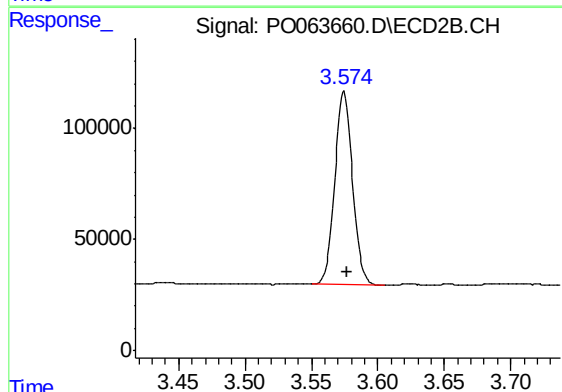


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: -0.003 min
Response: 812963
Conc: 38.56 ng/ml

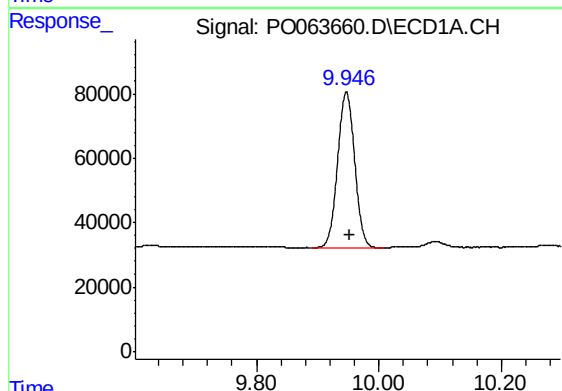

#2 Decachlorobiphenyl

R.T.: 9.946 min
Delta R.T.: -0.006 min
Response: 941589
Conc: 17.16 ng/ml m

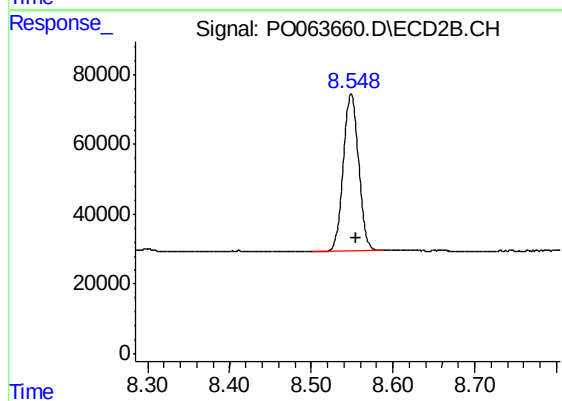

#2 Decachlorobiphenyl

R.T.: 8.549 min
Delta R.T.: -0.005 min
Response: 584896
Conc: 19.73 ng/ml