

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111220\
 Data File : P0073232.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2020 12:44
 Operator : DD\AJ
 Sample : L4573-04RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OB-722-XRE

Manual Integrations
 APPROVED

Ankita
 11/13/2020 8:09:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 17:46:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 10 11:30:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.947	4.017	2016167	1278064	38.042	35.766m
2) SA Decachlor...	10.977	9.293	1452263	1019556	35.093	30.560

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
Data File : PO073232.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2020 12:44
Operator : DD\AJ
Sample : L4573-04RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OB-722-XRE


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 17:46:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 10 11:30:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

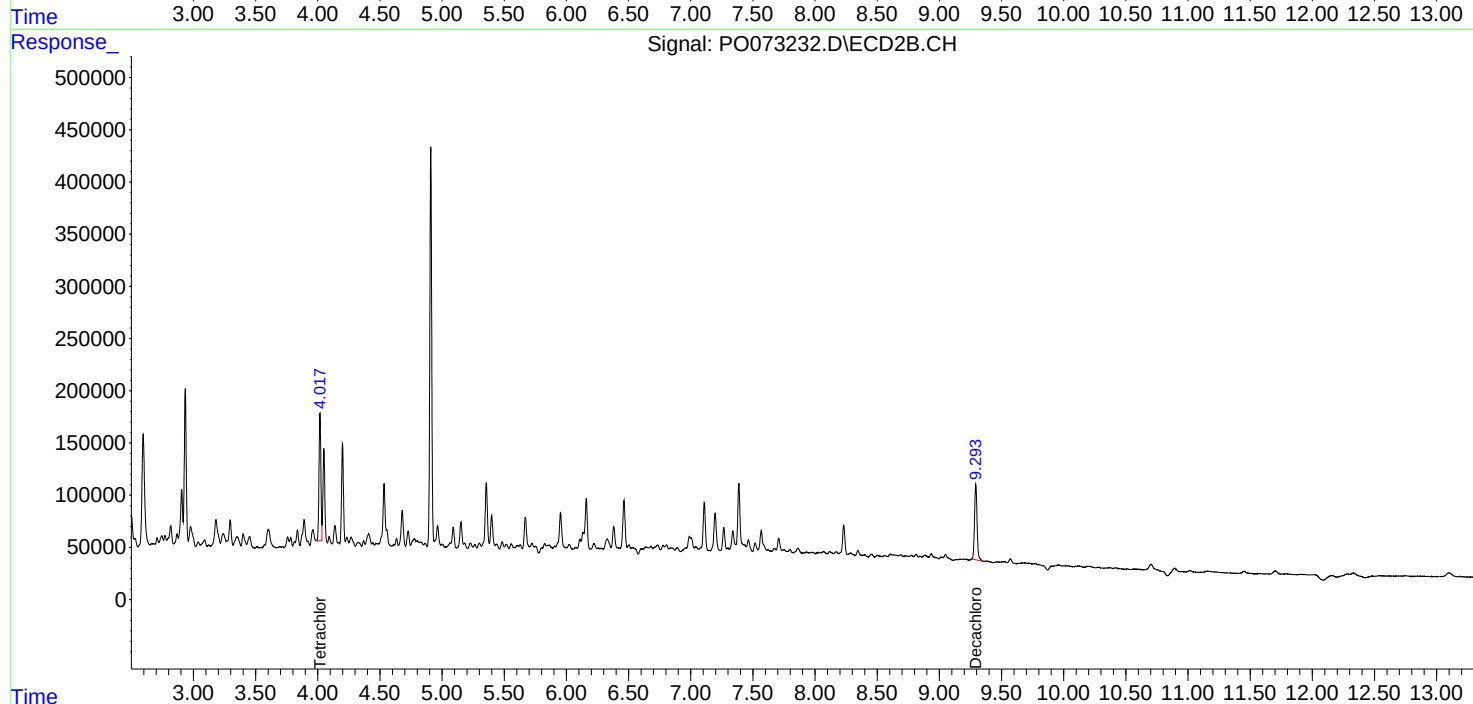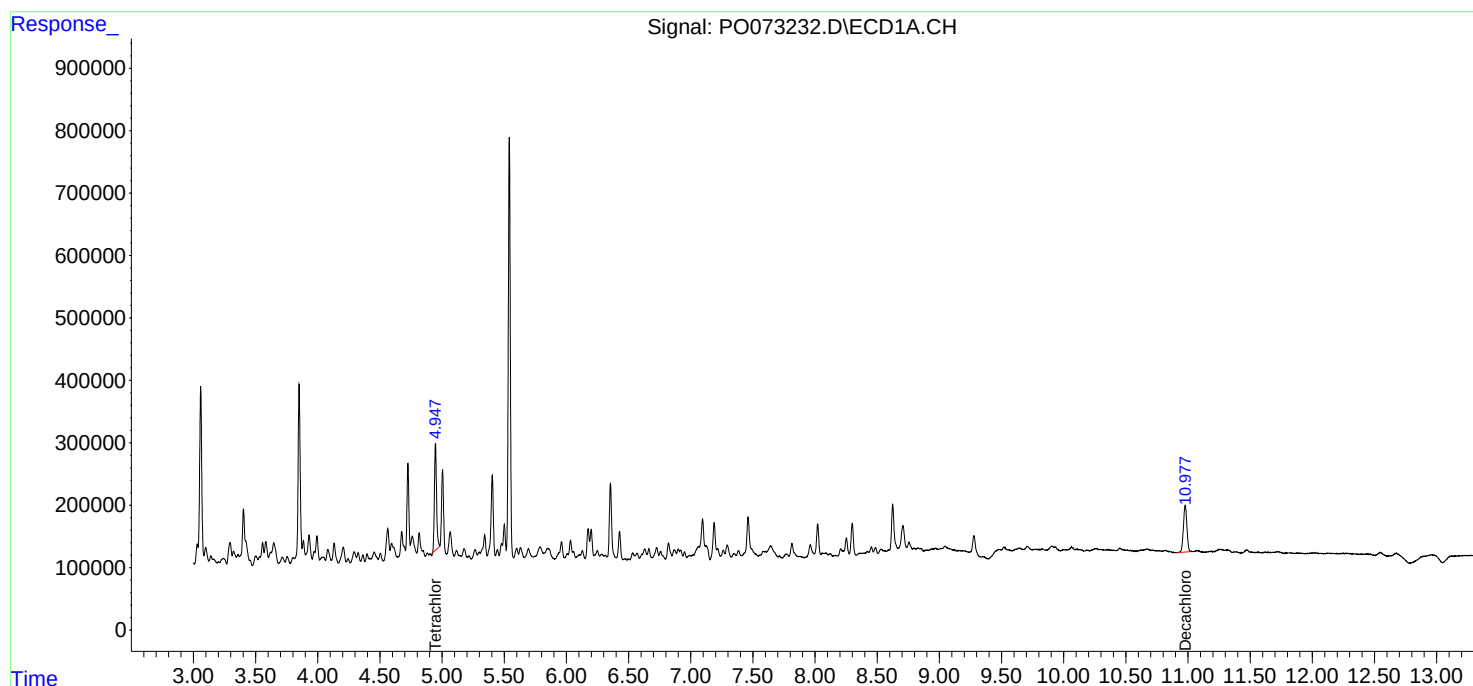

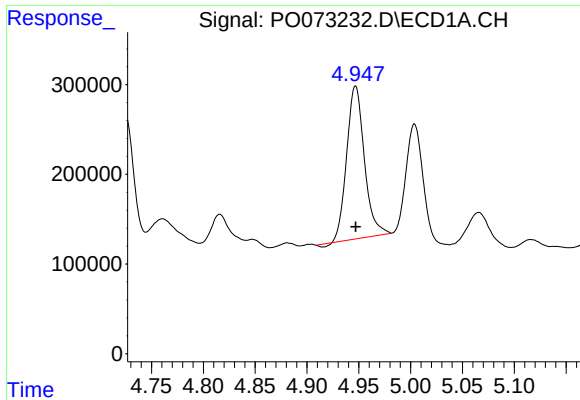


#1 Tetrachloro-m-xylene

R.T.: 4.947 min
Delta R.T.: 0.000 min
Response: 2016167
Conc: 38.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
OB-722-XRE


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:42 AM

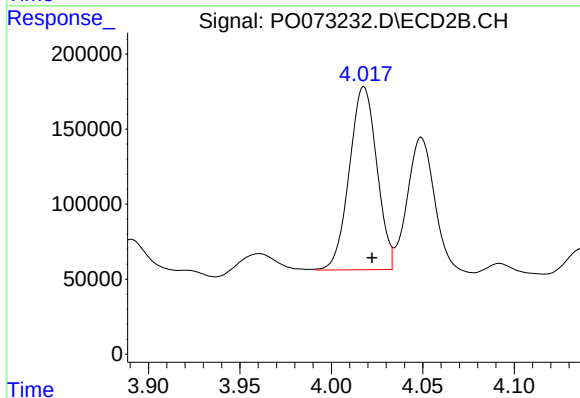


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: -0.005 min
Response: 1278064
Conc: 35.77 ng/ml m

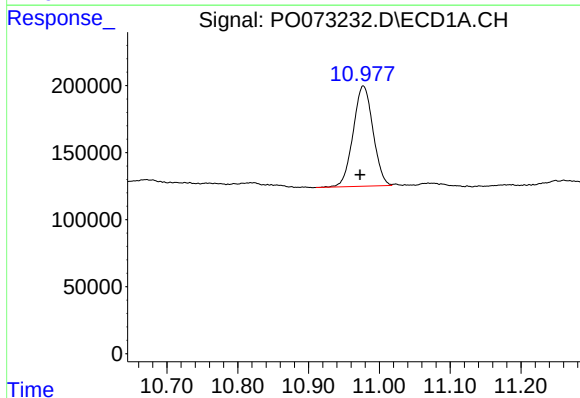

#2 Decachlorobiphenyl

R.T.: 10.977 min
Delta R.T.: 0.005 min
Response: 1452263
Conc: 35.09 ng/ml

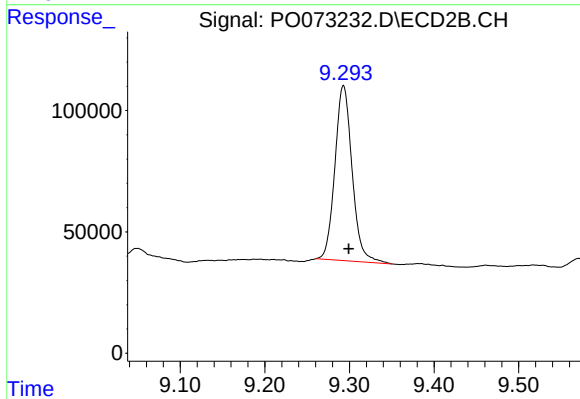

#2 Decachlorobiphenyl

R.T.: 9.293 min
Delta R.T.: -0.006 min
Response: 1019556
Conc: 30.56 ng/ml