

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
 Data File : PO073236.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2020 13:53
 Operator : DD\AJ
 Sample : L4683-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-WATER-001-002-003

Manual Integrations
 APPROVED

Ankita
 11/13/2020 8:09:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 17:47:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 10 11:30:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.957	4.039f	1357371	836703	25.611m	23.415m
2) SA Decachlor...	10.976	9.294	1223989	851223	29.577	25.515

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
Data File : PO073236.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2020 13:53
Operator : DD\AJ
Sample : L4683-06
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER-001-002-003


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 17:47:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 10 11:30:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

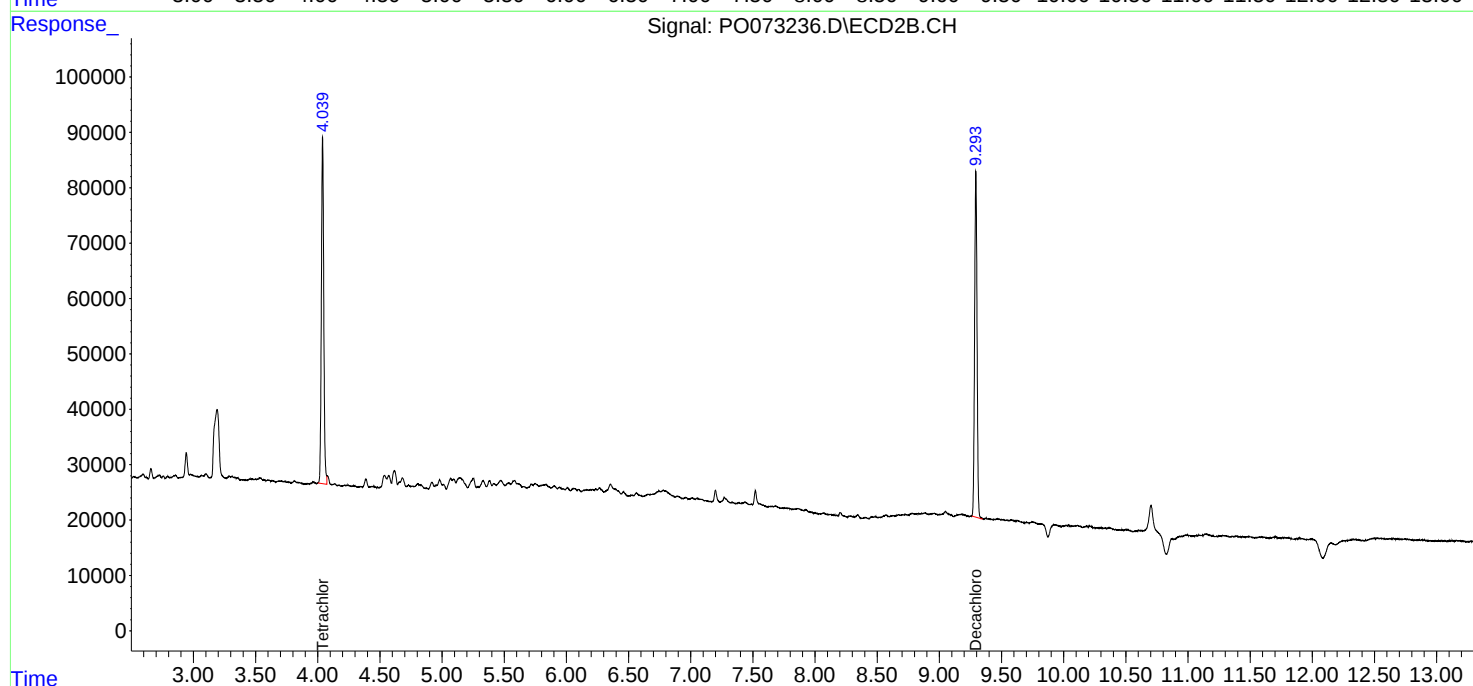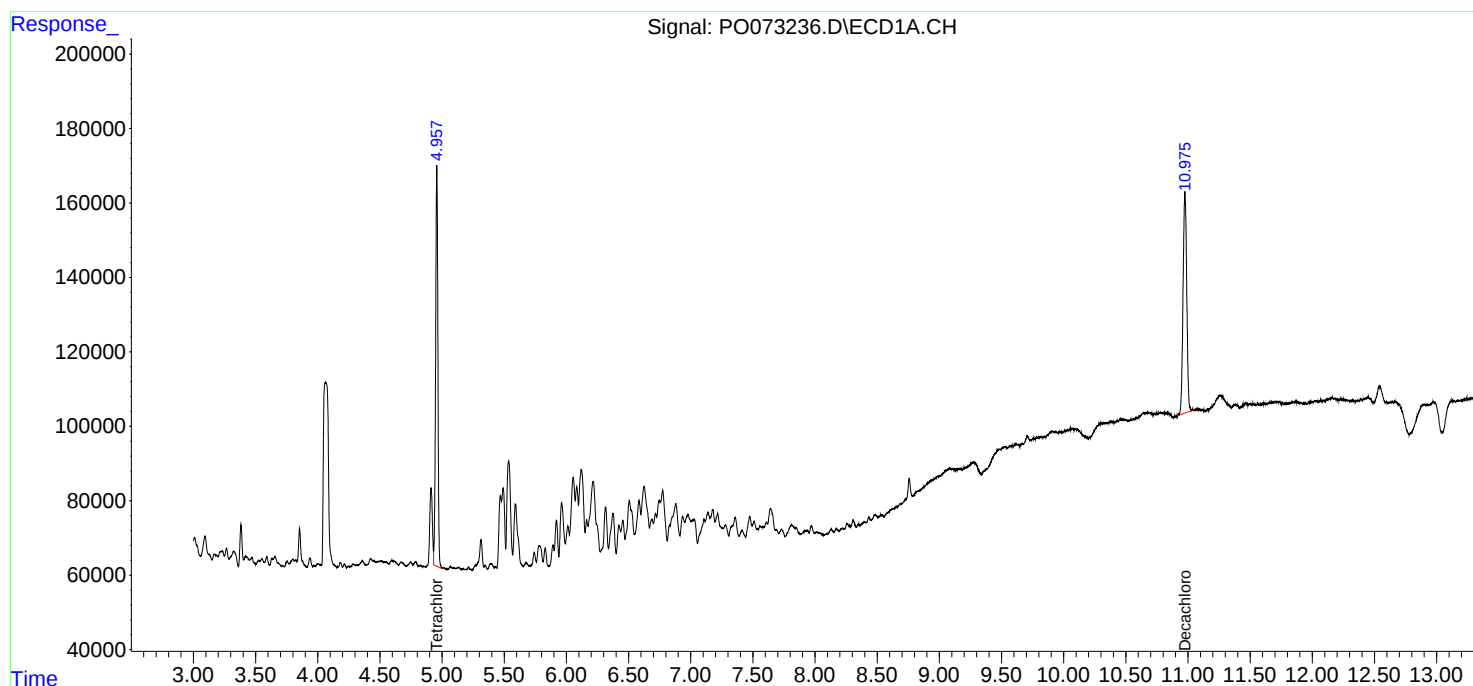

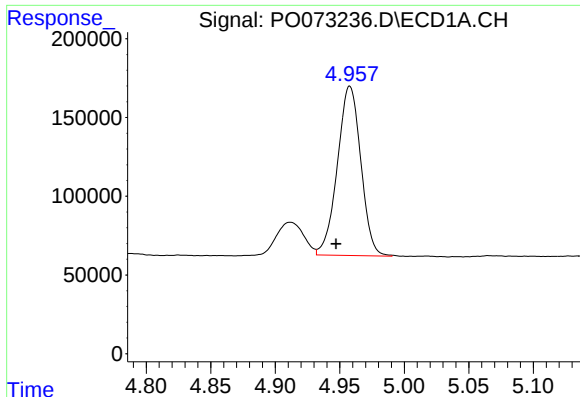


#1 Tetrachloro-m-xylene

R.T.: 4.957 min
Delta R.T.: 0.010 min
Response: 1357371
Conc: 25.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OILY-WATER-001-002-003


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:47 AM

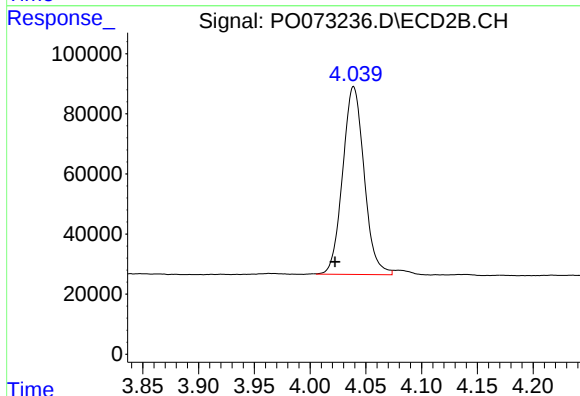


#1 Tetrachloro-m-xylene

R.T.: 4.039 min
Delta R.T.: 0.016 min
Response: 836703
Conc: 23.41 ng/ml m

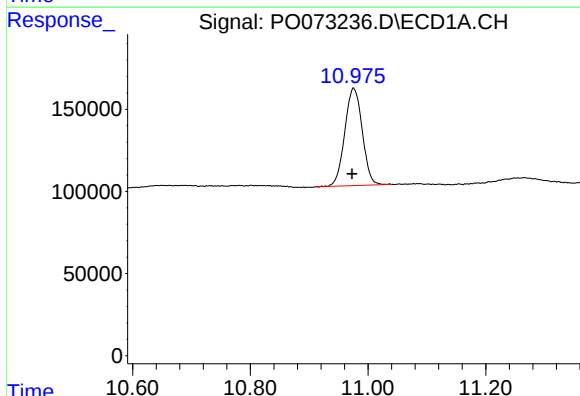

#2 Decachlorobiphenyl

R.T.: 10.976 min
Delta R.T.: 0.003 min
Response: 1223989
Conc: 29.58 ng/ml

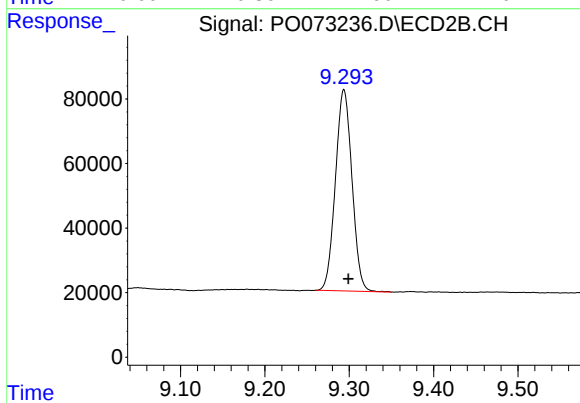

#2 Decachlorobiphenyl

R.T.: 9.294 min
Delta R.T.: -0.005 min
Response: 851223
Conc: 25.51 ng/ml