

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
 Data File : PO073244.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2020 19:14
 Operator : DD\AJ
 Sample : L4587-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-02-111120

Manual Integrations
 APPROVED

Ankita
 11/13/2020 8:09:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:53:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 10 11:30:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.946	4.017	1521220	928997	28.703m	25.997
2) SA Decachlor...	10.974	9.291	1166260	781306	28.182	23.419

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
Data File : PO073244.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2020 19:14
Operator : DD\AJ
Sample : L4587-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HR-02-111120


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:53:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 10 11:30:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

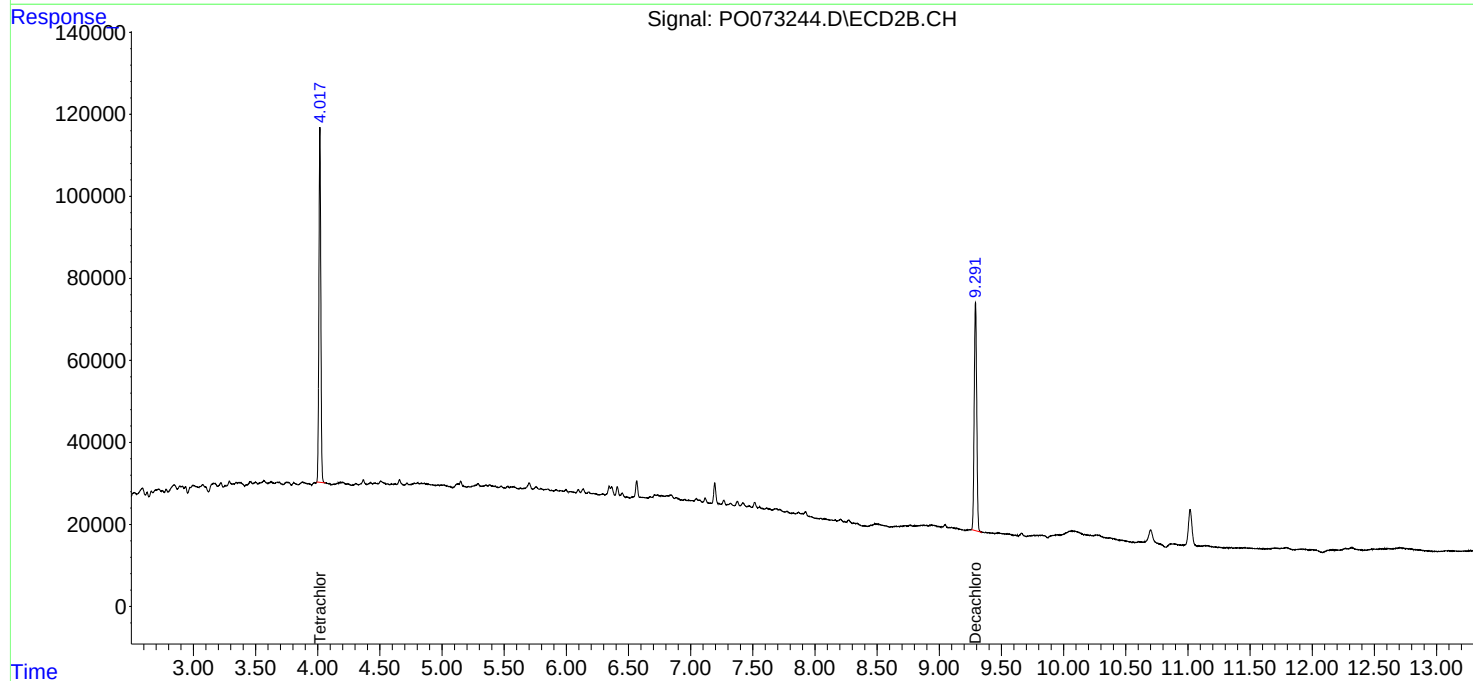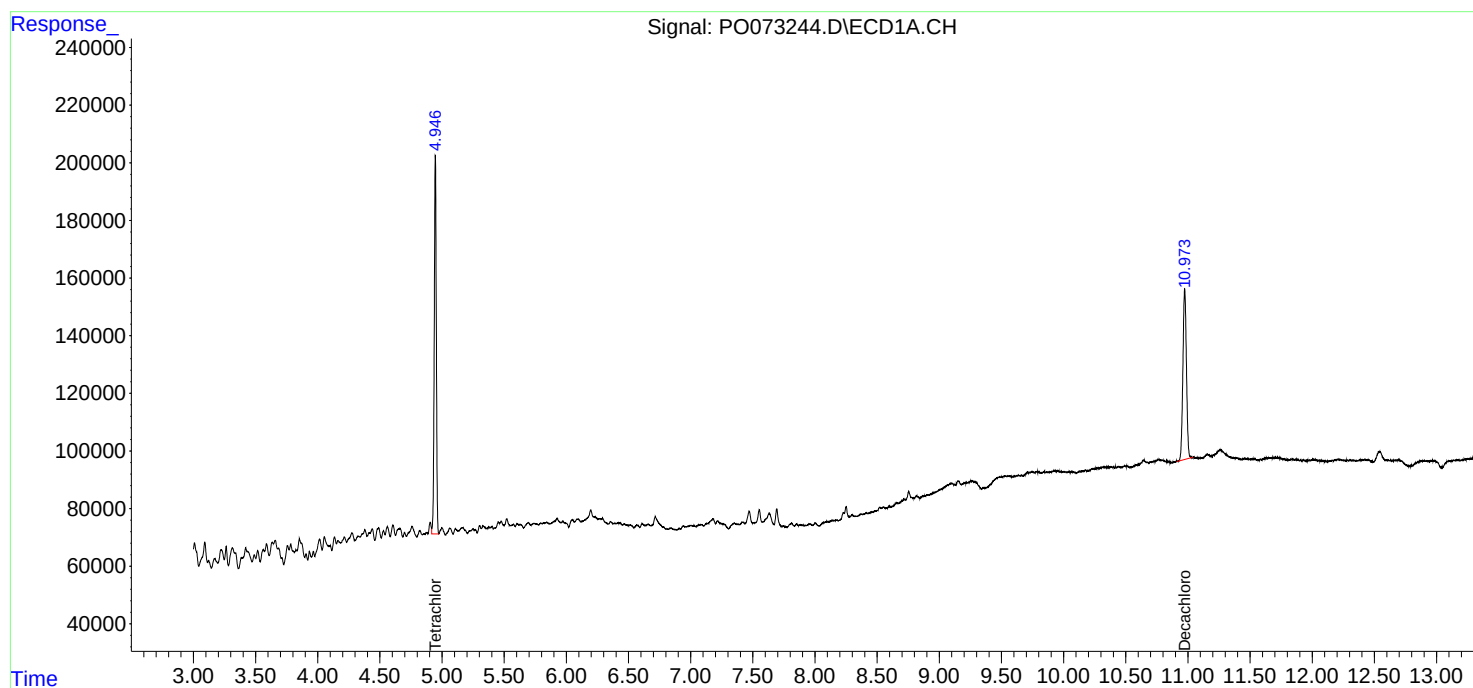

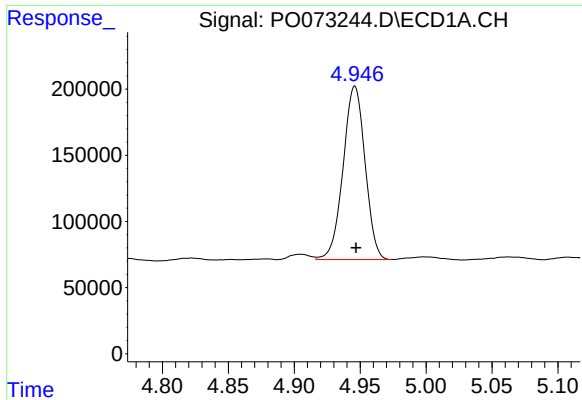


#1 Tetrachloro-m-xylene

R.T.: 4.946 min
Delta R.T.: -0.001 min
Response: 1521220
Conc: 28.70 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HR-02-111120


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:51 AM

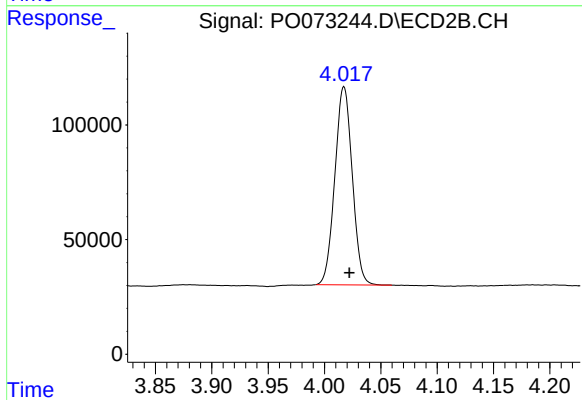


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: -0.005 min
Response: 928997
Conc: 26.00 ng/ml

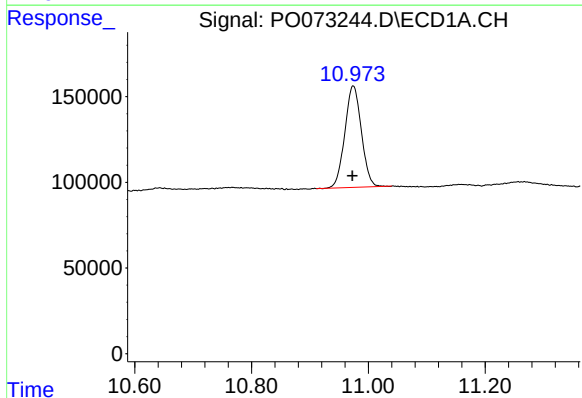

#2 Decachlorobiphenyl

R.T.: 10.974 min
Delta R.T.: 0.001 min
Response: 1166260
Conc: 28.18 ng/ml

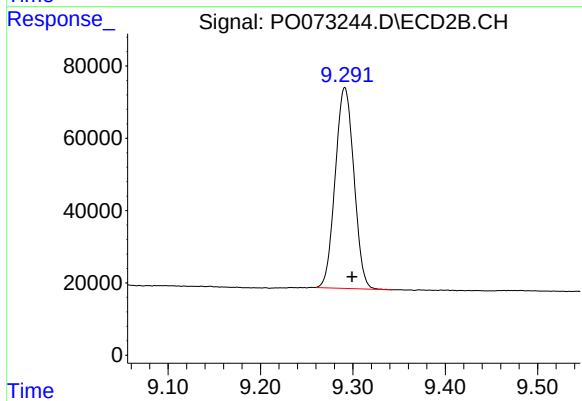

#2 Decachlorobiphenyl

R.T.: 9.291 min
Delta R.T.: -0.008 min
Response: 781306
Conc: 23.42 ng/ml