

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111220\
 Data File : P0073245.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2020 19:31
 Operator : DD\AJ
 Sample : L4595-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-03-111120

Manual Integrations
 APPROVED

Ankita
 11/13/2020 8:09:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:53:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 10 11:30:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.946	4.018	1494895	922586	28.206m	25.818
2) SA Decachlor...	10.977	9.291	1117561	773474	27.005	23.184

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
Data File : PO073245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2020 19:31
Operator : DD\AJ
Sample : L4595-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-03-111120


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:53:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 10 11:30:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

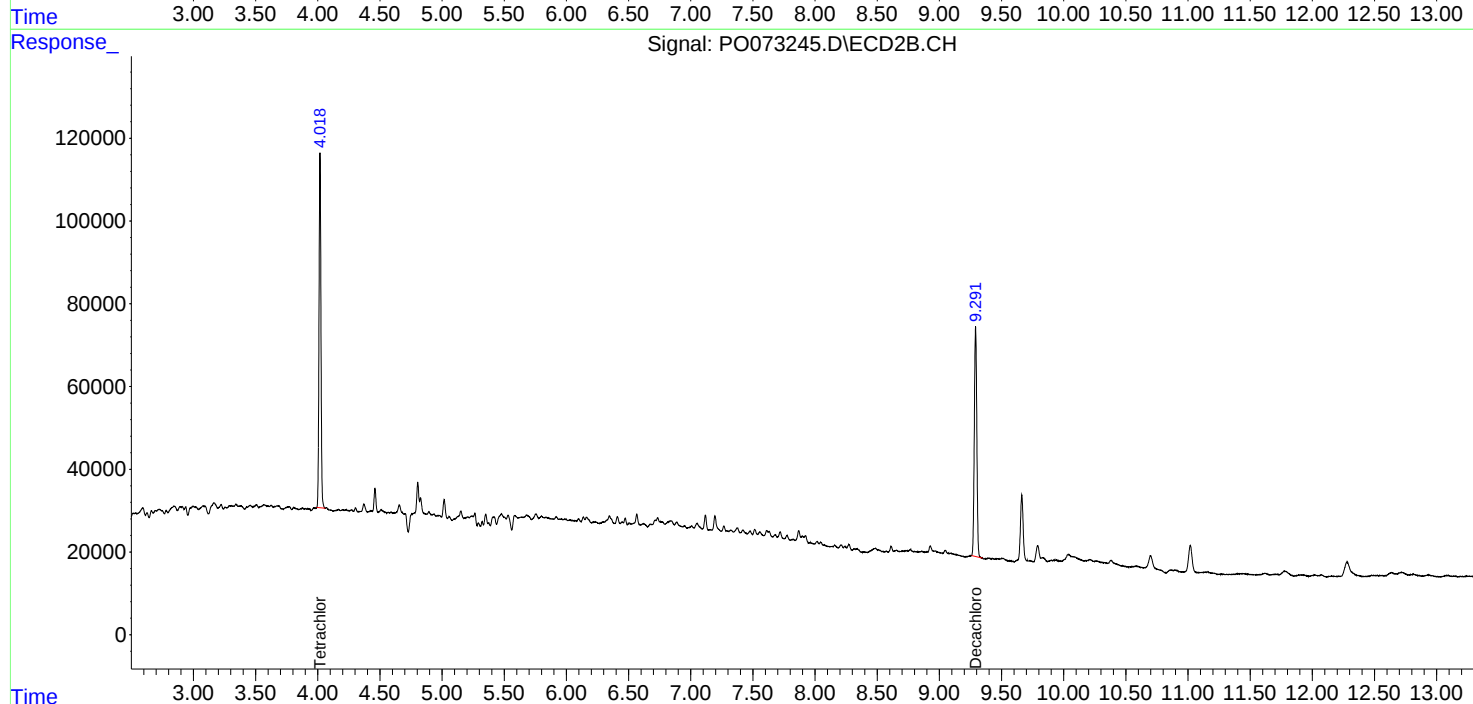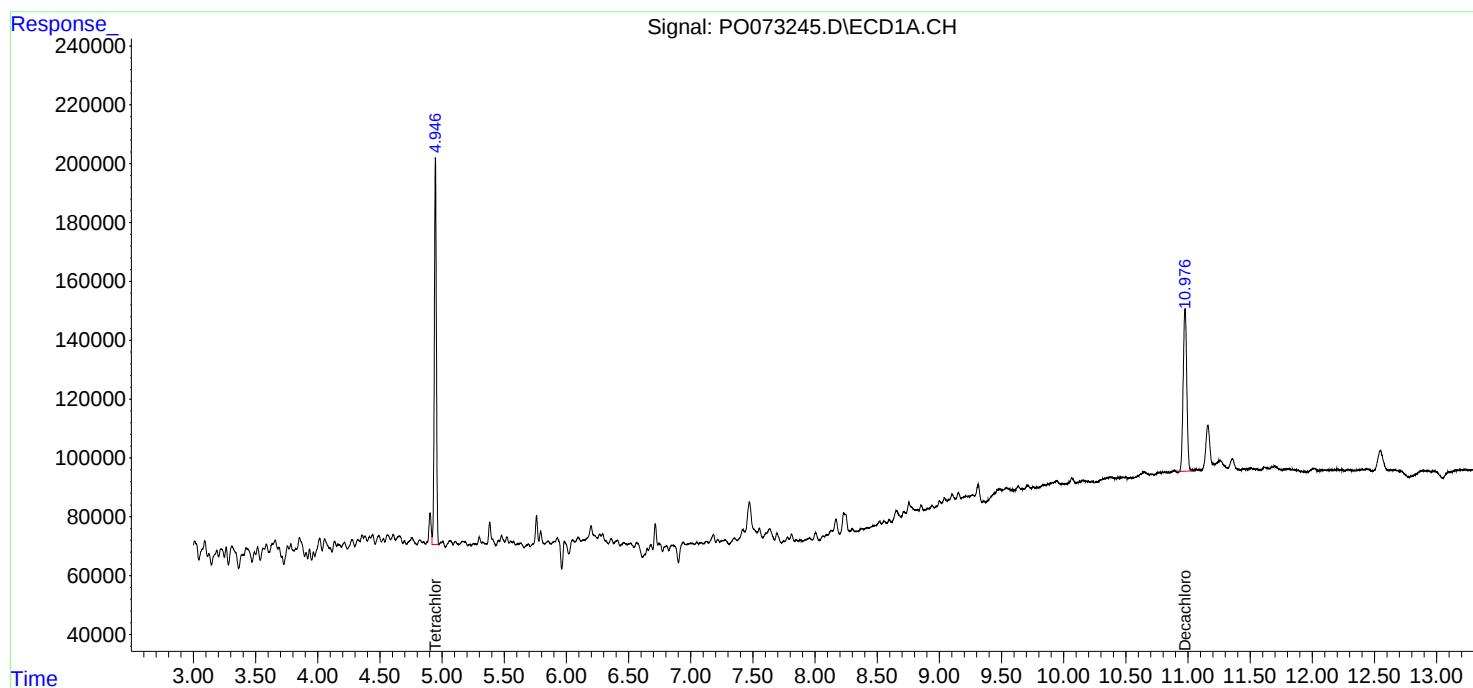

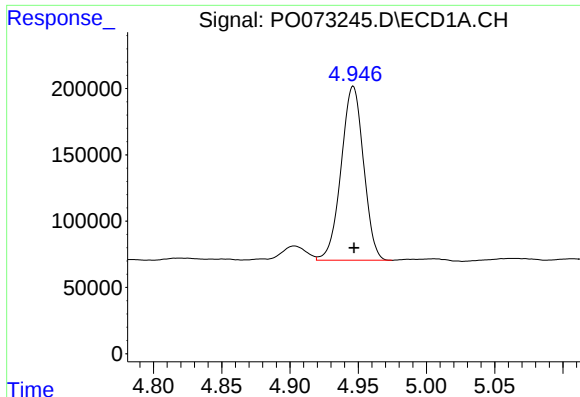


#1 Tetrachloro-m-xylene

R.T.: 4.946 min
Delta R.T.: -0.001 min
Response: 1494895
Conc: 28.21 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SU-03-111120


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:52 AM

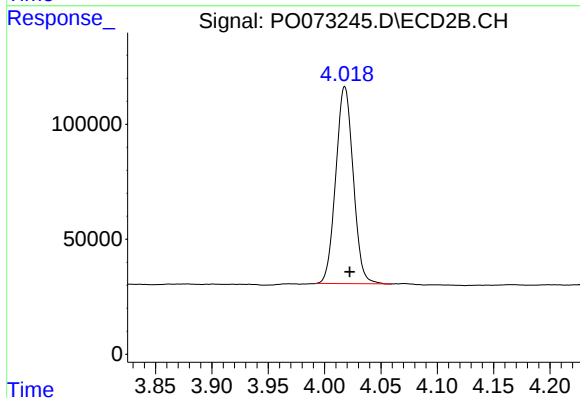


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: -0.004 min
Response: 922586
Conc: 25.82 ng/ml

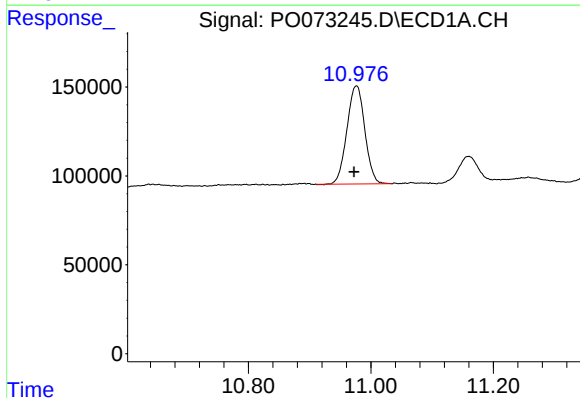

#2 Decachlorobiphenyl

R.T.: 10.977 min
Delta R.T.: 0.004 min
Response: 1117561
Conc: 27.01 ng/ml

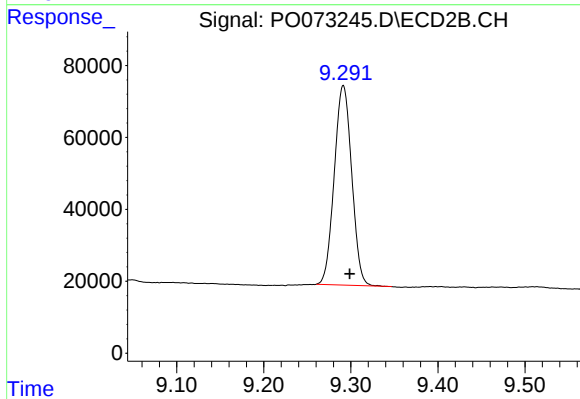

#2 Decachlorobiphenyl

R.T.: 9.291 min
Delta R.T.: -0.008 min
Response: 773474
Conc: 23.18 ng/ml