

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
 Data File : PO073246.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2020 19:49
 Operator : DD\AJ
 Sample : L4706-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-30706-30707-40854

Manual Integrations
 APPROVED

Ankita
 11/13/2020 8:09:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 00:53:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 10 11:30:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.954	4.032	1204042	744408	22.718m	20.832m
2) SA Decachlor...	11.008f	9.323f	947673	663431	22.900m	19.886

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111220\
Data File : PO073246.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2020 19:49
Operator : DD\AJ
Sample : L4706-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-30706-30707-40854


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 00:53:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 10 11:30:16 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

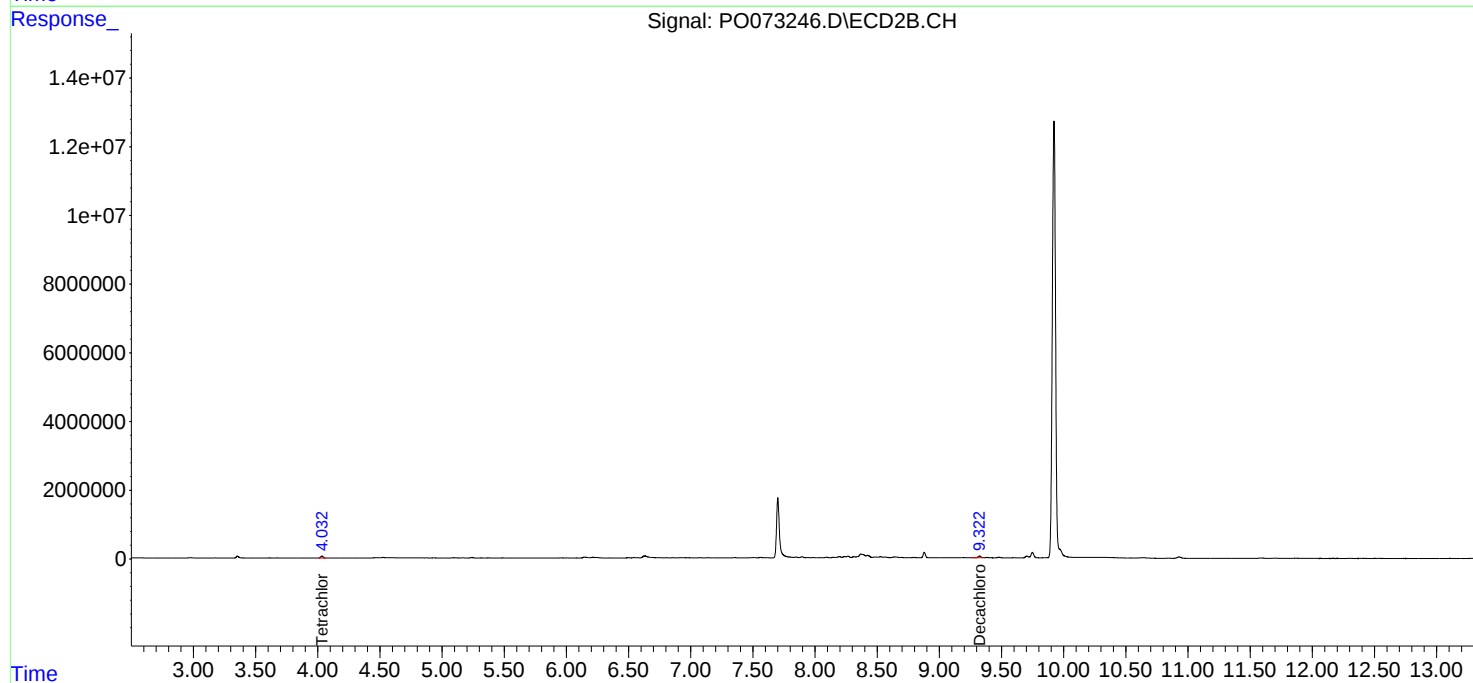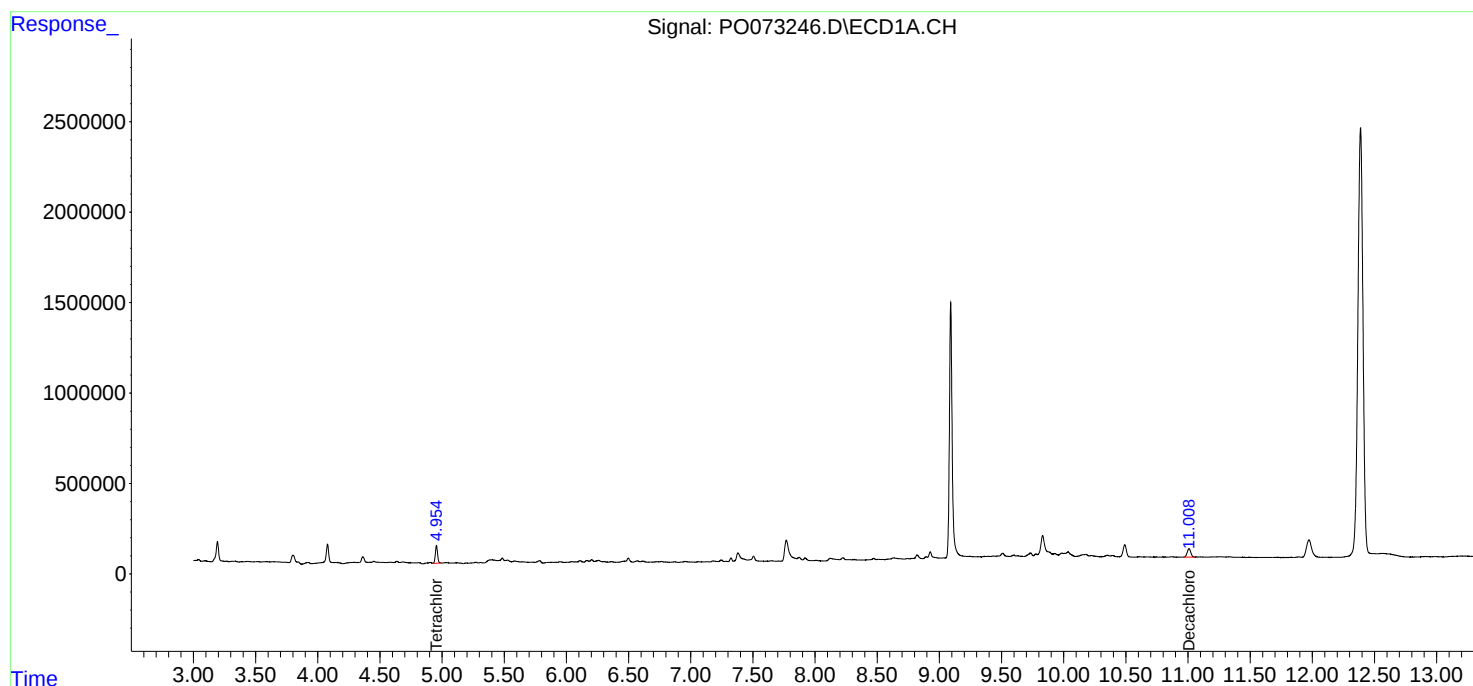

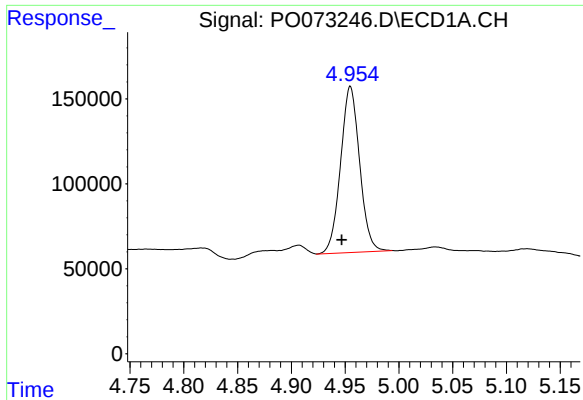


#1 Tetrachloro-m-xylene

R.T.: 4.954 min
Delta R.T.: 0.007 min
Response: 1204042
Conc: 22.72 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-30706-30707-40854


Manual Integrations
APPROVED

Ankita
11/13/2020 8:09:54 AM

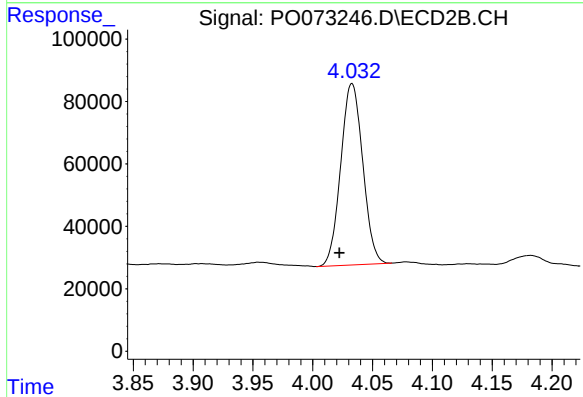


#1 Tetrachloro-m-xylene

R.T.: 4.032 min
Delta R.T.: 0.010 min
Response: 744408
Conc: 20.83 ng/ml m

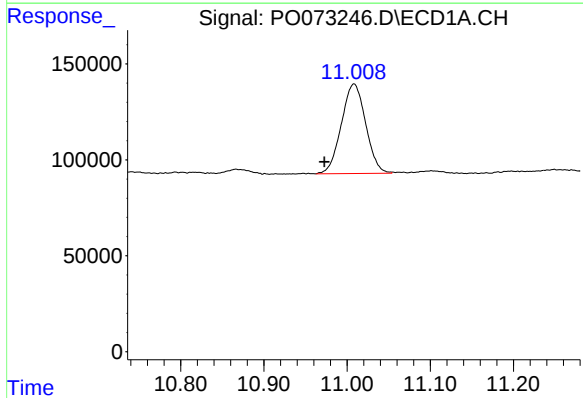

#2 Decachlorobiphenyl

R.T.: 11.008 min
Delta R.T.: 0.035 min
Response: 947673
Conc: 22.90 ng/ml m

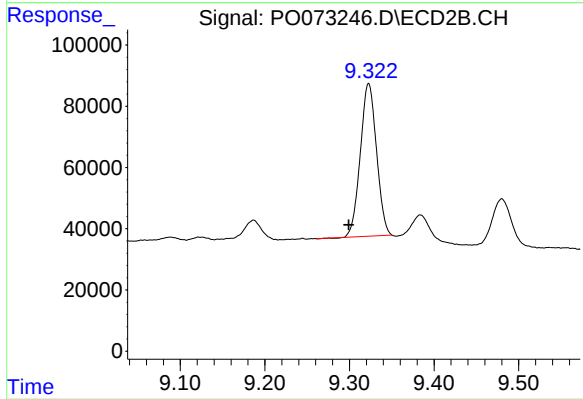

#2 Decachlorobiphenyl

R.T.: 9.323 min
Delta R.T.: 0.024 min
Response: 663431
Conc: 19.89 ng/ml