

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111318\
 Data File : P0051493.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Nov 2018 19:17
 Operator : SM/SJ
 Sample : J5904-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 110818-SIDI-F-D-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 03:54:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 13 14:44:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.310	3.300	50168395	16065969	15.709	14.590
2) SA Decachlor...	9.954	8.057	33988583	16444632	17.709	19.838

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111318\
Data File : P0051493.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2018 19:17
Operator : SM/SJ
Sample : J5904-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
110818-SIDI-F-D-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:54:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 13 14:44:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

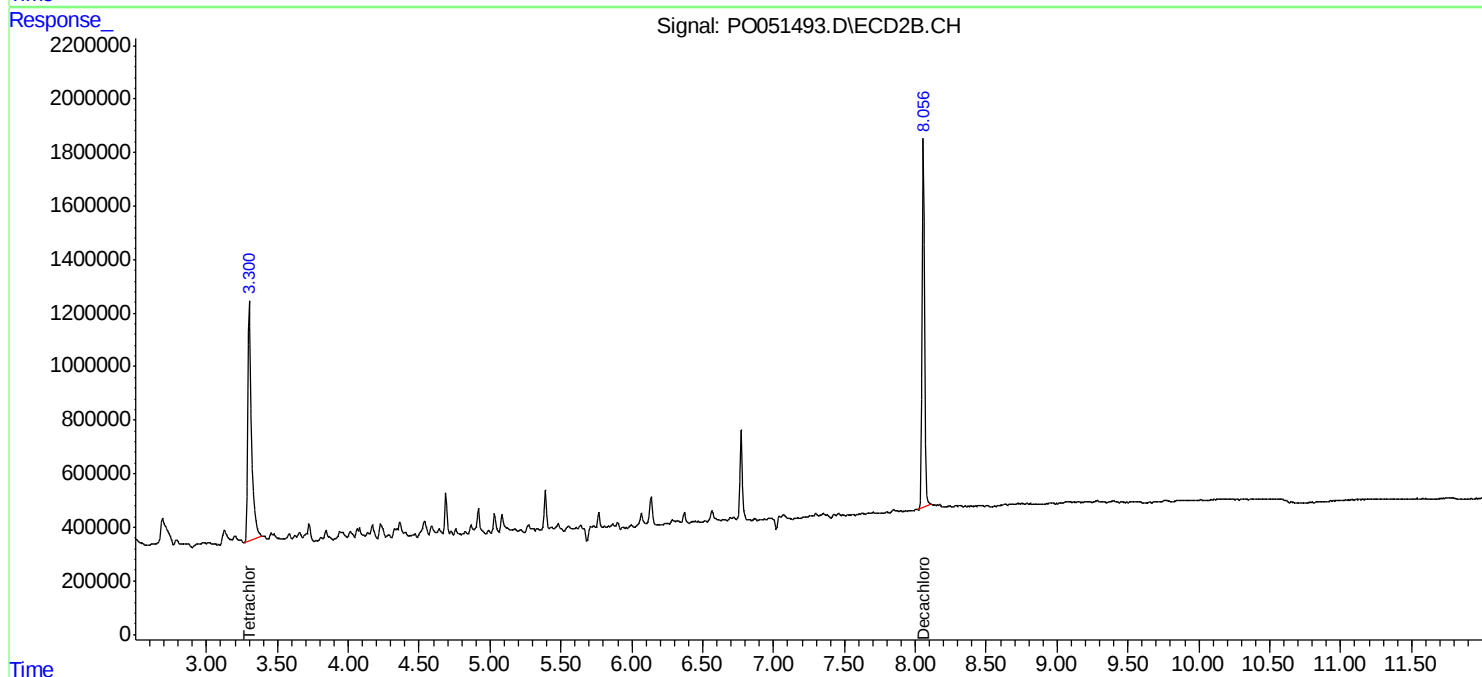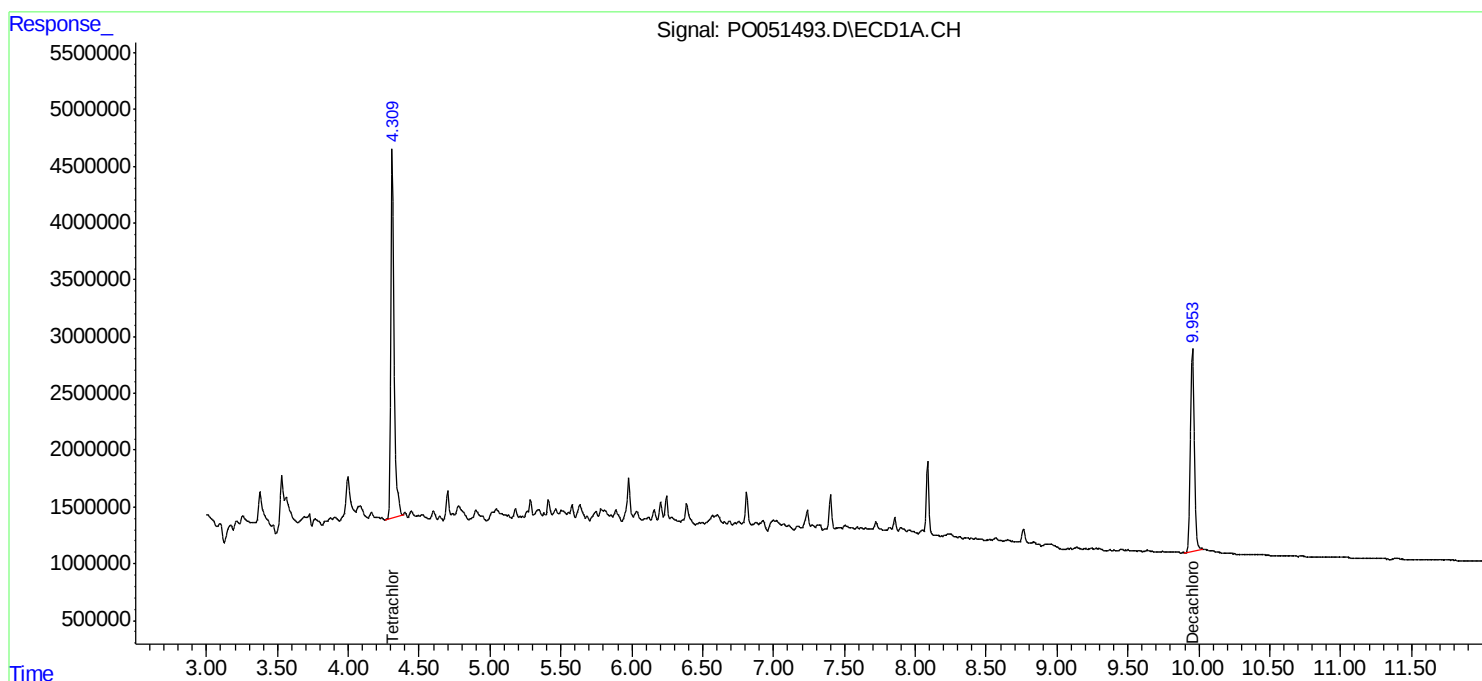


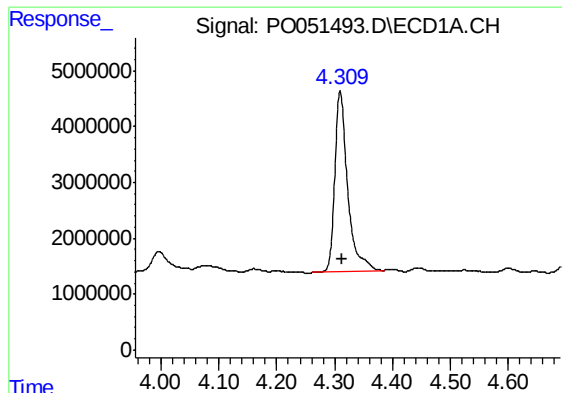

#1 Tetrachloro-m-xylene


R.T.: 4.310 min
Delta R.T.: -0.003 min
Response: 50168395
Conc: 15.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
110818-SIDI-F-D-B

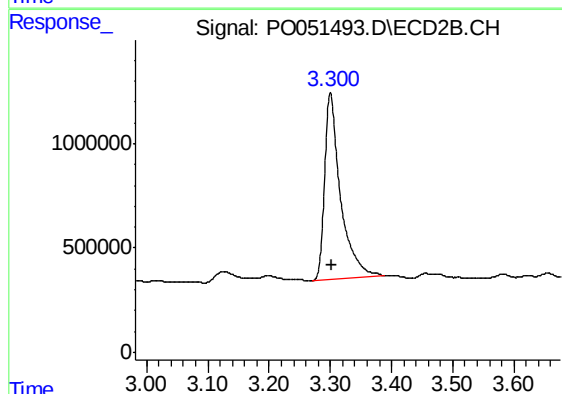


#1 Tetrachloro-m-xylene

R.T.: 3.300 min
Delta R.T.: -0.002 min
Response: 16065969
Conc: 14.59 ng/ml

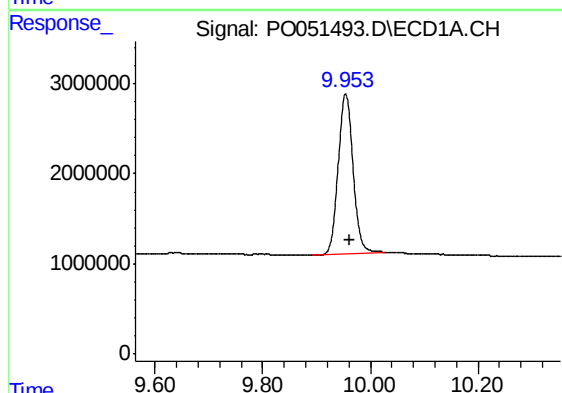

#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.008 min
Response: 33988583
Conc: 17.71 ng/ml

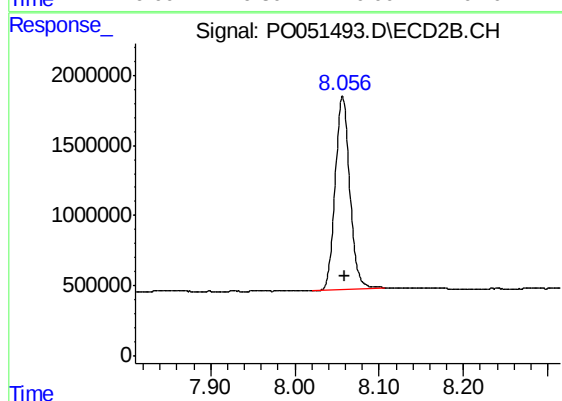

#2 Decachlorobiphenyl

R.T.: 8.057 min
Delta R.T.: -0.003 min
Response: 16444632
Conc: 19.84 ng/ml