

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111318\
Data File : P0051494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2018 19:34
Operator : SM/SJ
Sample : J5904-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
110818-SIDI-F-D-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:54:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 13 14:44:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.310	3.301	50805534	16409974	15.909	14.902
2)	SA Decachlor...	9.953	8.056	34672267	16941447	18.065	20.437

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111318\
Data File : PO051494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2018 19:34
Operator : SM/SJ
Sample : J5904-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
110818-SIDI-F-D-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:54:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 13 14:44:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

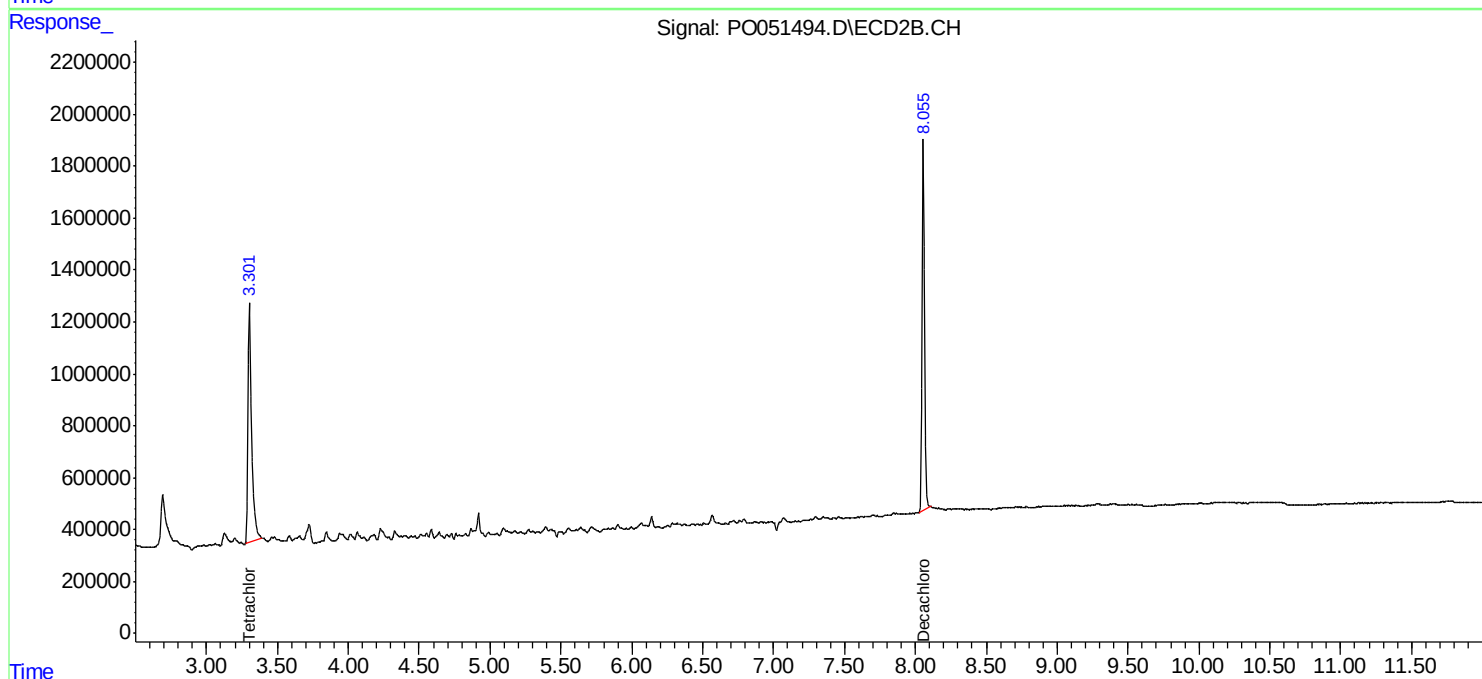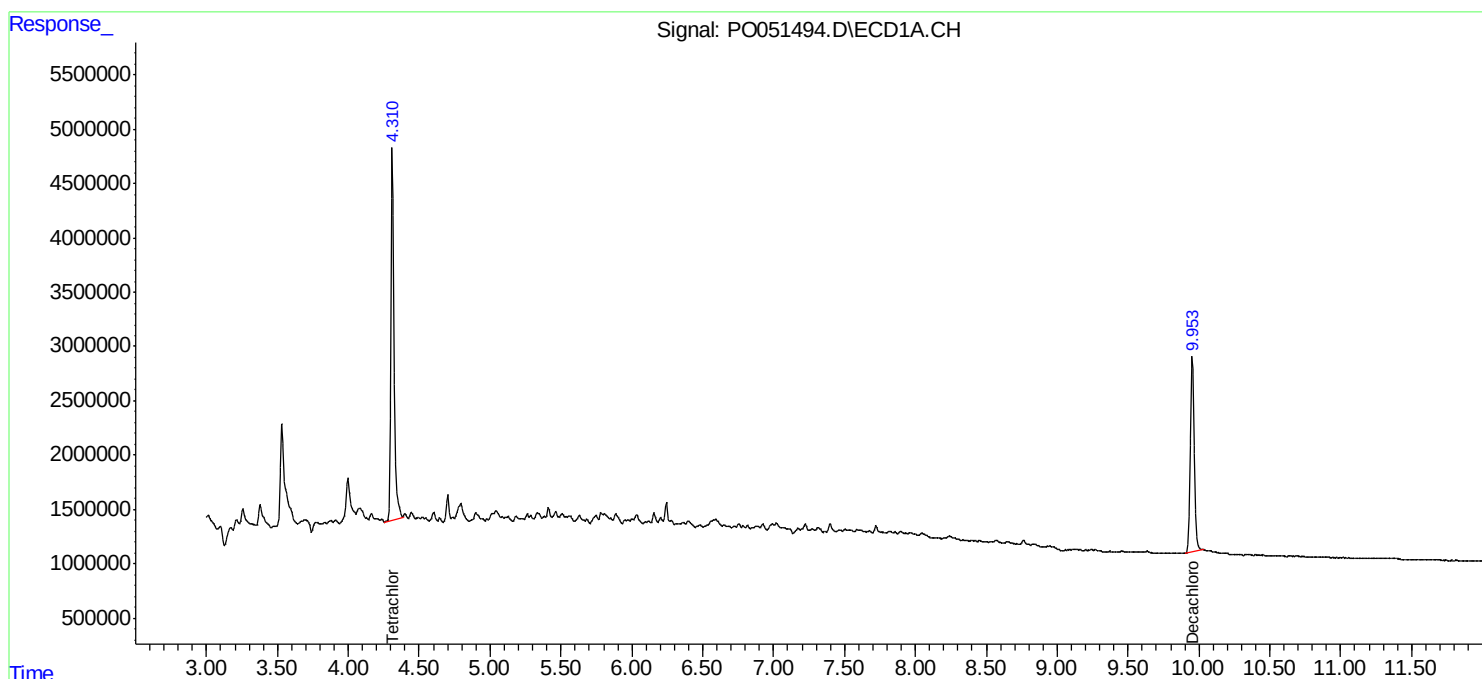


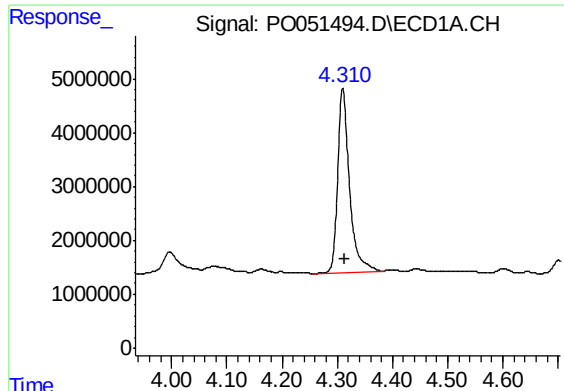

#1 Tetrachloro-m-xylene


R.T.: 4.310 min
Delta R.T.: -0.003 min
Response: 50805534
Conc: 15.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
110818-SIDI-F-D-M

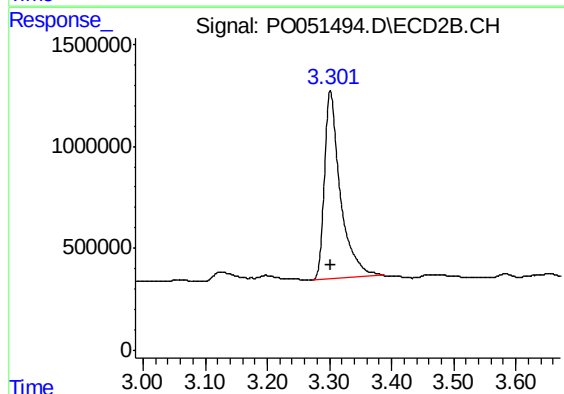


#1 Tetrachloro-m-xylene

R.T.: 3.301 min
Delta R.T.: 0.000 min
Response: 16409974
Conc: 14.90 ng/ml

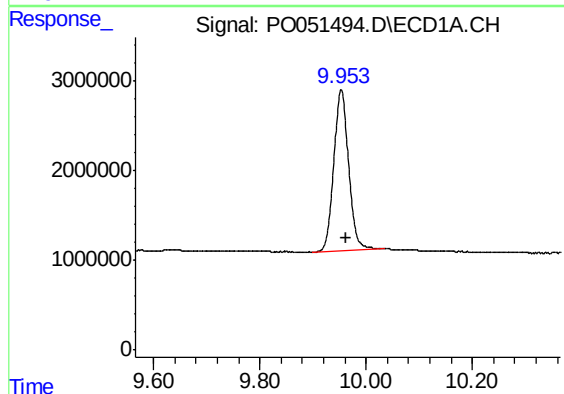

#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: -0.008 min
Response: 34672267
Conc: 18.07 ng/ml

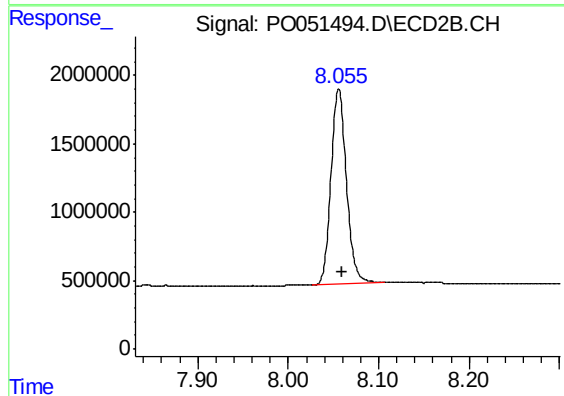

#2 Decachlorobiphenyl

R.T.: 8.056 min
Delta R.T.: -0.003 min
Response: 16941447
Conc: 20.44 ng/ml