

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111318\
 Data File : P0051497.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Nov 2018 20:25
 Operator : SM/SJ
 Sample : J5904-13
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 110818-SIDI-F-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 03:55:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 13 14:44:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.310	3.301	49006889	16028671	15.345	14.556
2) SA Decachlor...	9.954	8.056	33762655	16657566	17.591	20.095

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111318\
Data File : PO051497.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2018 20:25
Operator : SM/SJ
Sample : J5904-13
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
110818-SIDI-F-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:55:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 13 14:44:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

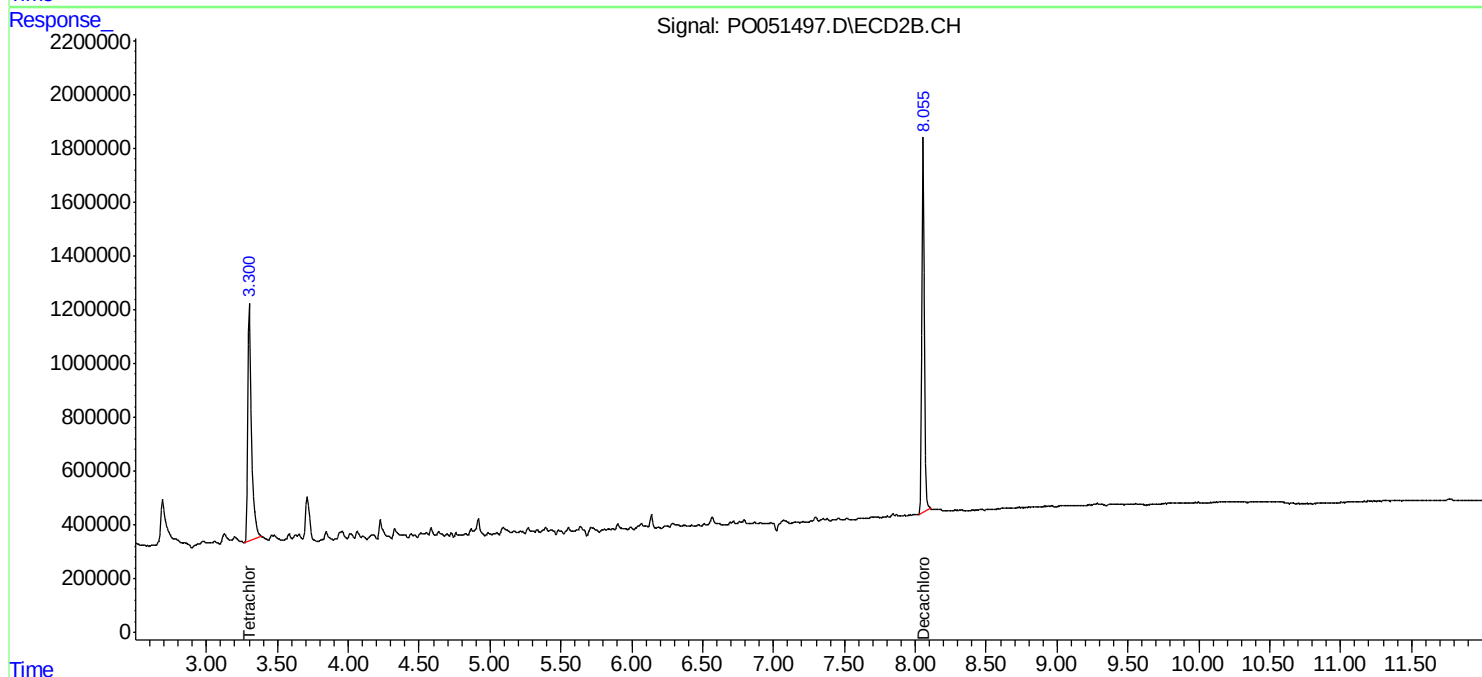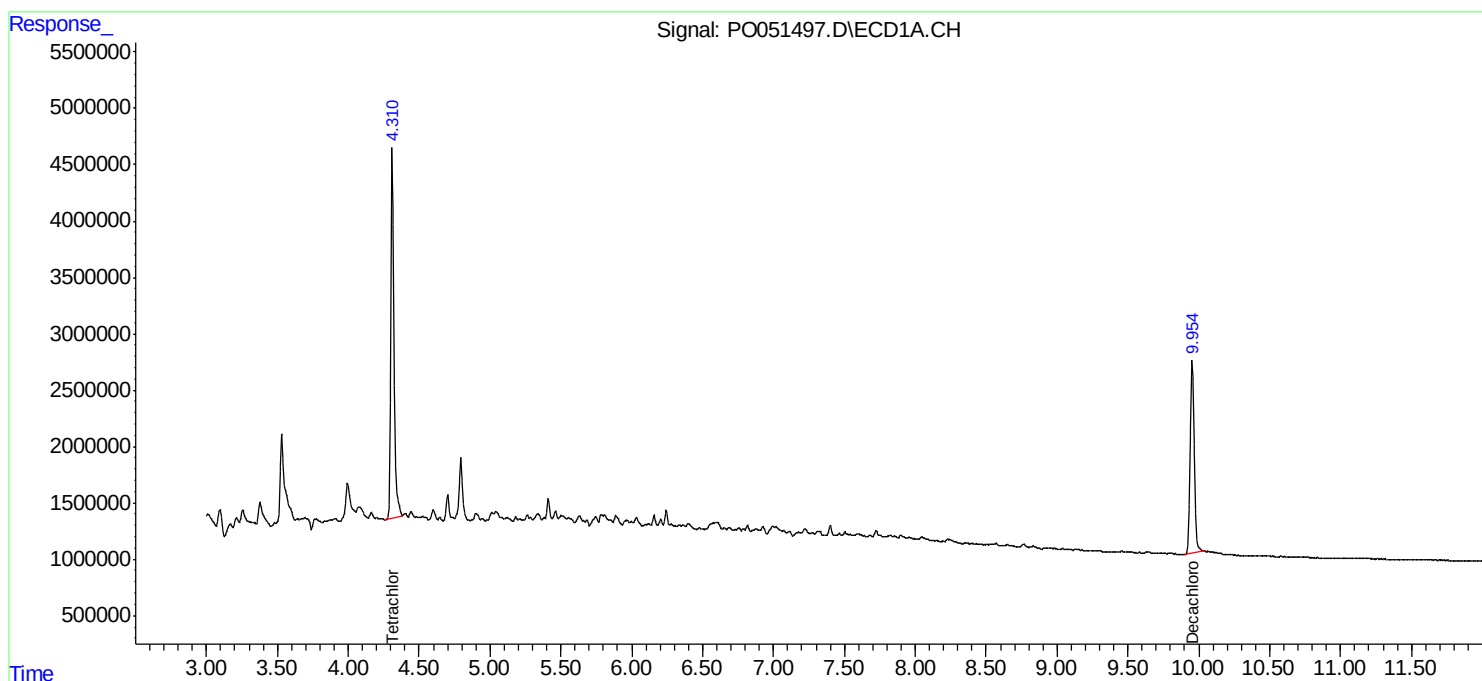


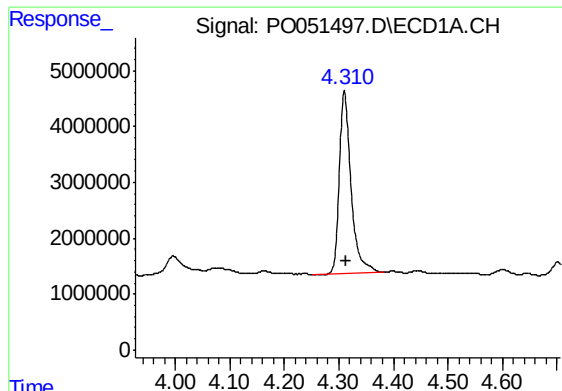

#1 Tetrachloro-m-xylene


R.T.: 4.310 min
Delta R.T.: -0.003 min
Response: 49006889
Conc: 15.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
110818-SIDI-F-D-S

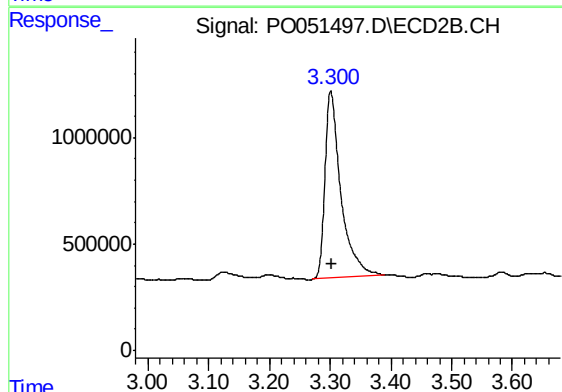


#1 Tetrachloro-m-xylene

R.T.: 3.301 min
Delta R.T.: -0.001 min
Response: 16028671
Conc: 14.56 ng/ml

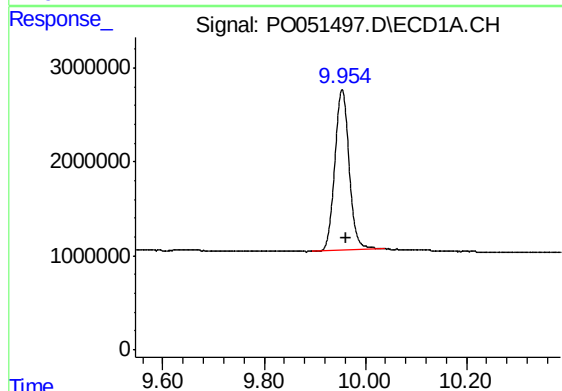

#2 Decachlorobiphenyl

R.T.: 9.954 min
Delta R.T.: -0.008 min
Response: 33762655
Conc: 17.59 ng/ml

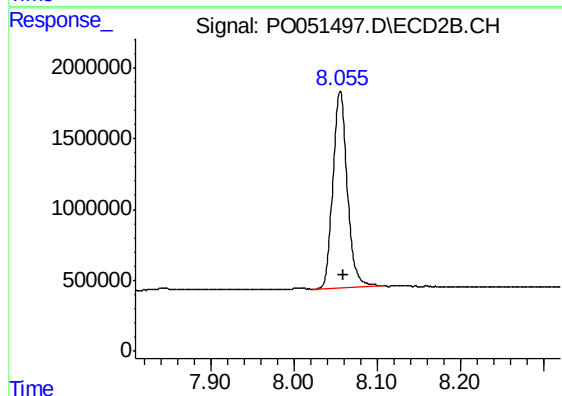

#2 Decachlorobiphenyl

R.T.: 8.056 min
Delta R.T.: -0.003 min
Response: 16657566
Conc: 20.09 ng/ml