

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111321\
 Data File : PO082829.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2021 23:05
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 01:11:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.963	3.960	1723621	639620	19.330	19.712
2)	SA Decachlor...	11.062	9.273	1281973	623970	22.136	22.007
Target Compounds							
8)	L2 AR-1221-1	5.205	0.000	51035	0	52.178	N.D. #
9)	L2 AR-1221-2	5.319	0.000	23340	0	33.889	N.D. #
10)	L2 AR-1221-3	0.000	4.405	0	25608	N.D.	25.893 #
11)	L3 AR-1232-1	0.000	4.405	0	25608	N.D.	31.614 #
24)	L5 AR-1248-4	7.221f	0.000	41117	0	15.651	N.D. #
26)	L6 AR-1254-1	7.221	0.000	41117	0	14.710	N.D. #
28)	L6 AR-1254-3	7.846f	0.000	29106	0	6.841	N.D. #
32)	L7 AR-1260-2	8.290f	0.000	9459	0	2.575	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111321\
Data File : PO082829.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2021 23:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 01:11:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

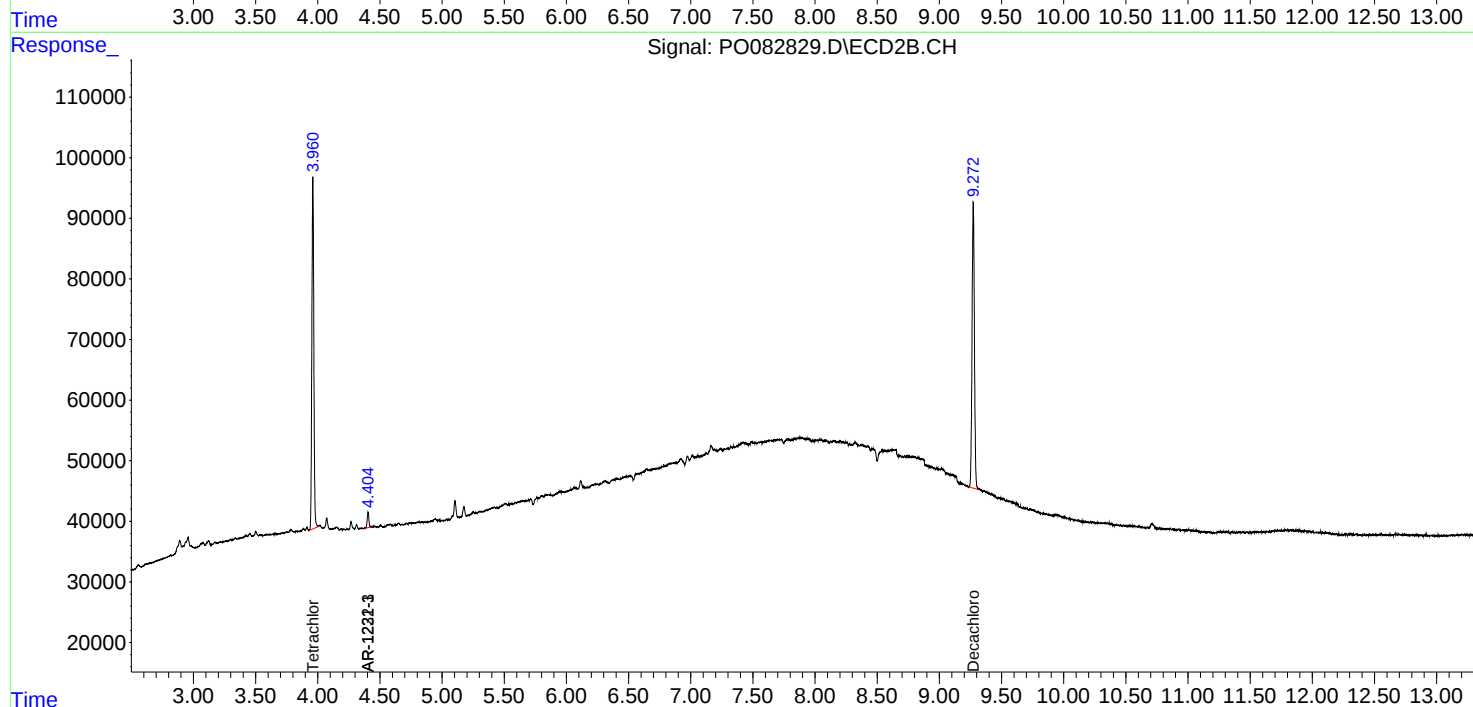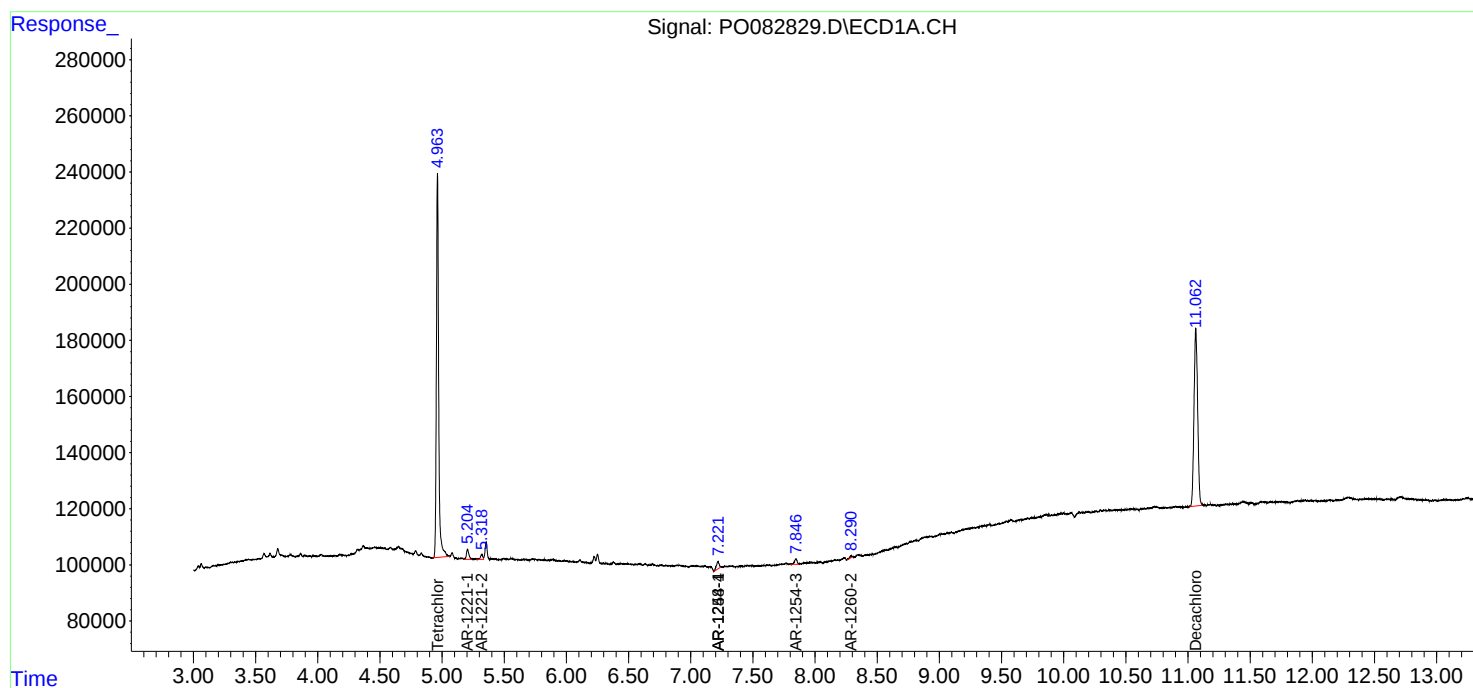


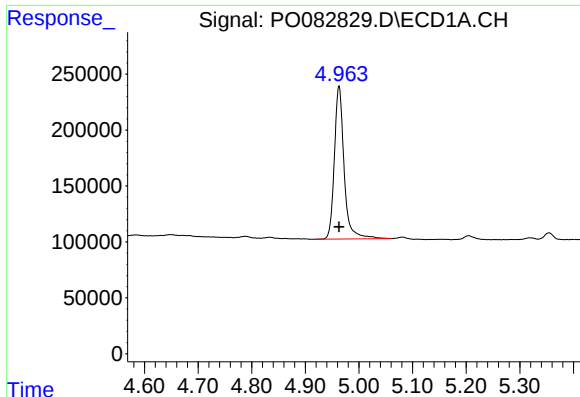

#1 Tetrachloro-m-xylene


R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 1723621
Conc: 19.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

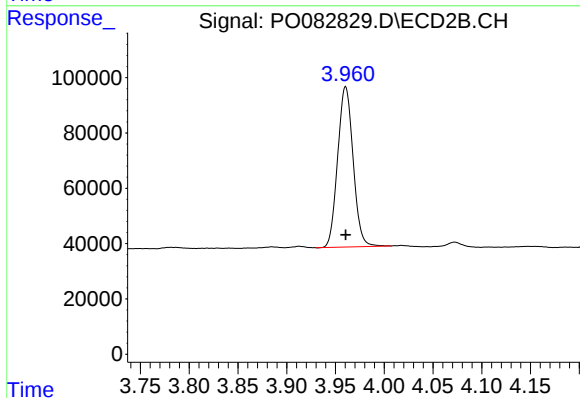


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 639620
Conc: 19.71 ng/ml

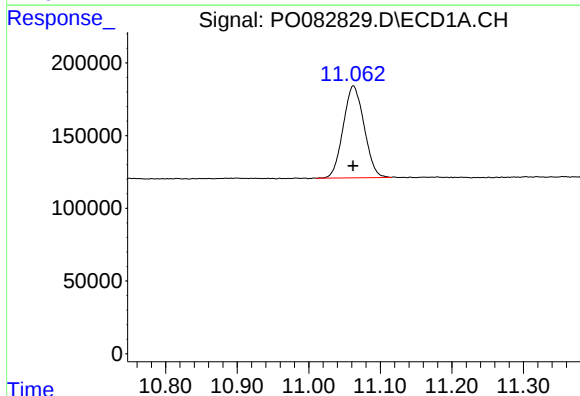


#2 Decachlorobiphenyl

R.T.: 11.062 min
Delta R.T.: 0.000 min
Response: 1281973
Conc: 22.14 ng/ml

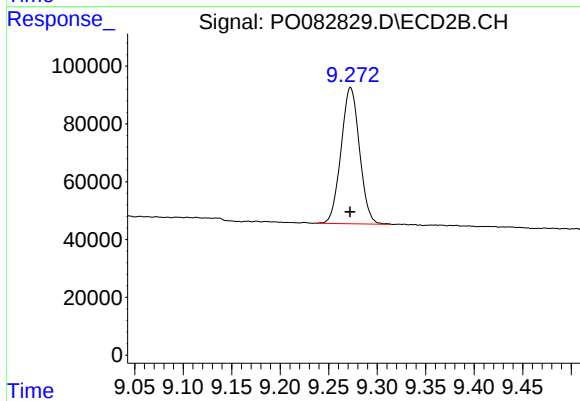

#2 Decachlorobiphenyl


R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 623970
Conc: 22.01 ng/ml

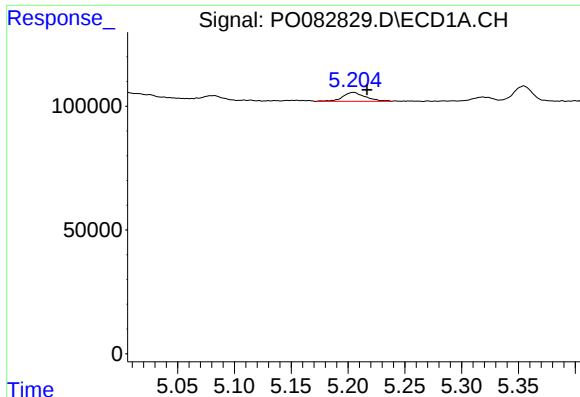

#8 AR-1221-1


R.T.: 5.205 min
Delta R.T.: -0.012 min
Response: 51035
Conc: 52.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

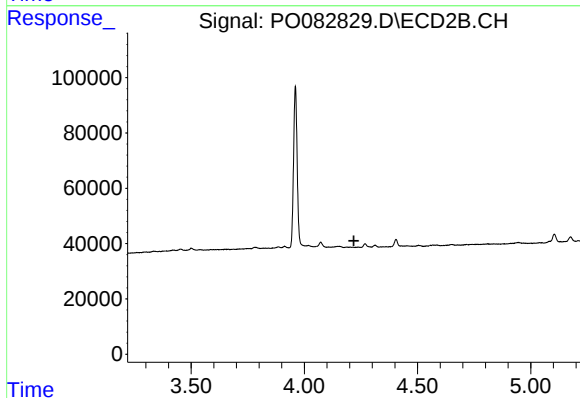


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.219 min
Response: 0
Conc: N.D.

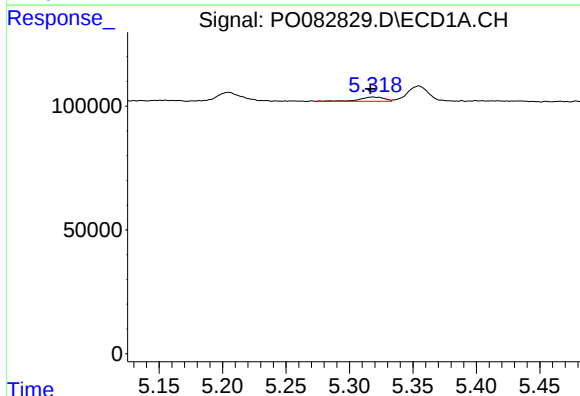


#9 AR-1221-2

R.T.: 5.319 min
Delta R.T.: 0.002 min
Response: 23340
Conc: 33.89 ng/ml

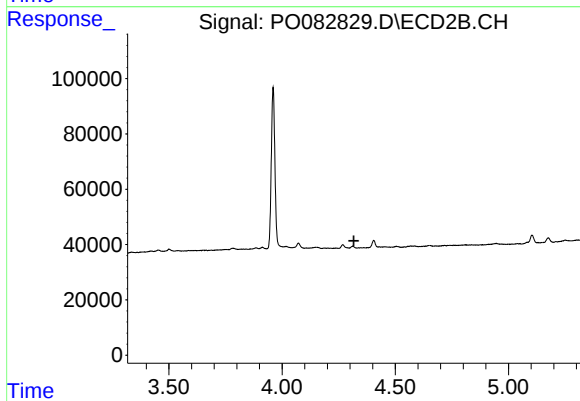

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.317 min
Response: 0
Conc: N.D.

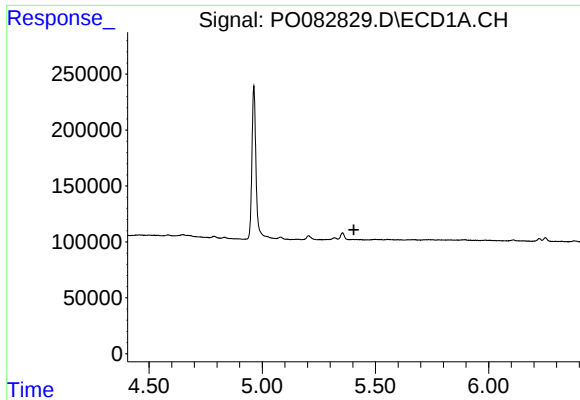

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

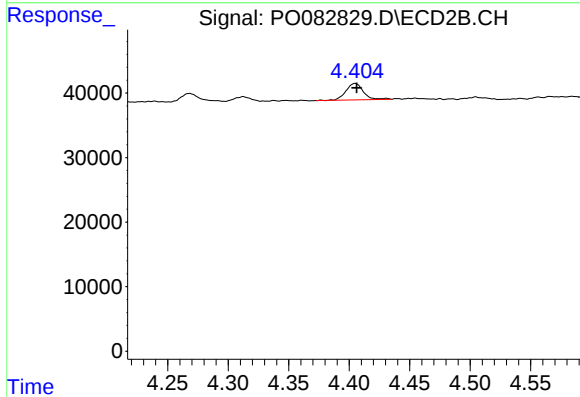


#10 AR-1221-3

R.T.: 4.405 min
Delta R.T.: -0.001 min
Response: 25608
Conc: 25.89 ng/ml

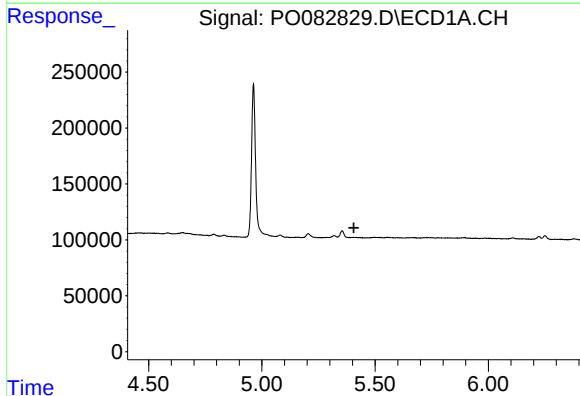


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

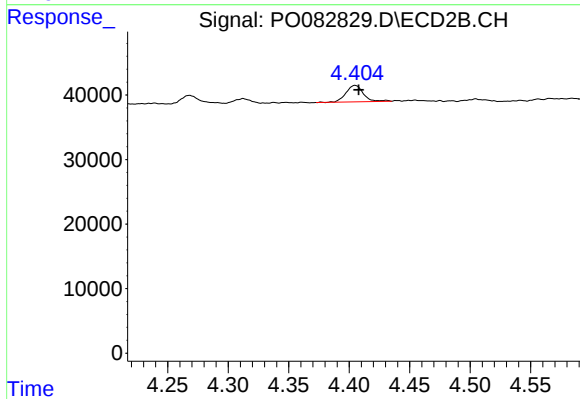

#11 AR-1232-1


R.T.: 4.405 min
Delta R.T.: -0.003 min
Response: 25608
Conc: 31.61 ng/ml

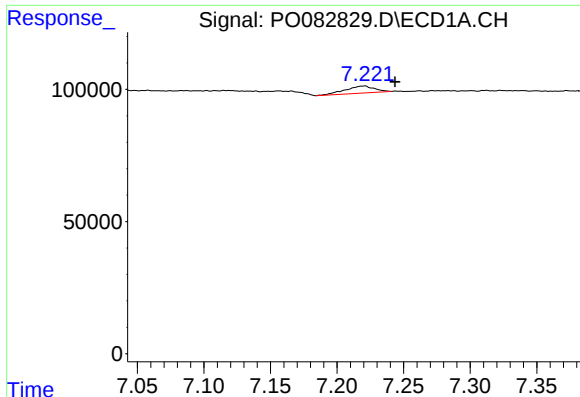

#24 AR-1248-4


R.T.: 7.221 min
Delta R.T.: -0.022 min
Response: 41117
Conc: 15.65 ng/ml

Instrument :
ECD_O
ClientSampleId :

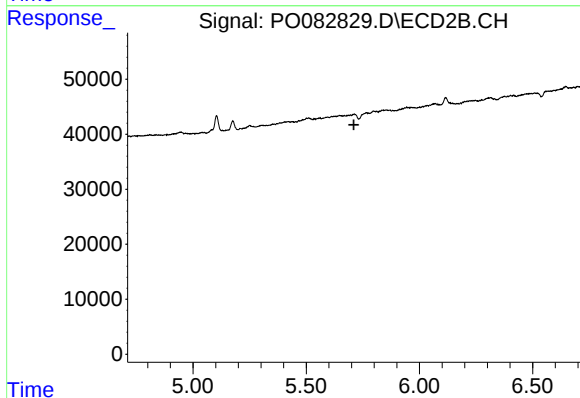


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.711 min
Response: 0
Conc: N.D.

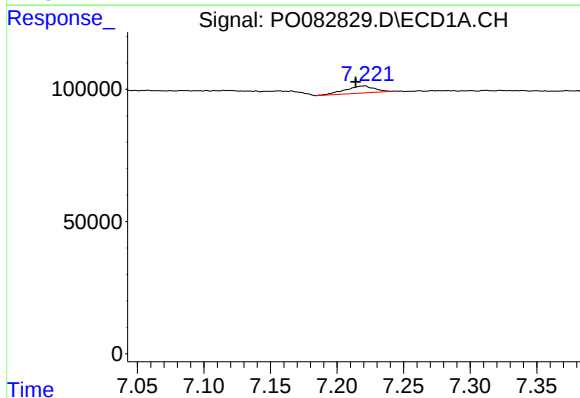


#26 AR-1254-1

R.T.: 7.221 min
Delta R.T.: 0.007 min
Response: 41117
Conc: 14.71 ng/ml

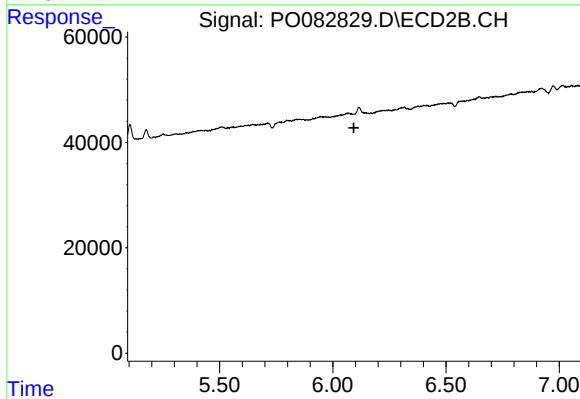

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

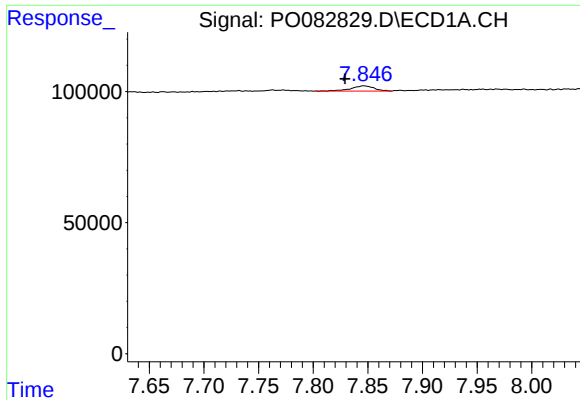

#28 AR-1254-3


R.T.: 7.846 min
Delta R.T.: 0.017 min
Response: 29106
Conc: 6.84 ng/ml

Instrument :
ECD_O
ClientSampleId :

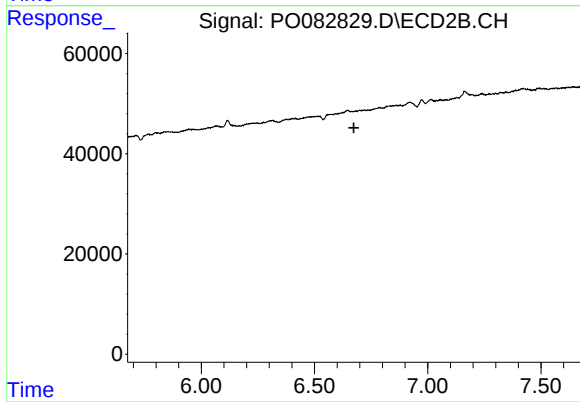


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.674 min
Response: 0
Conc: N.D.

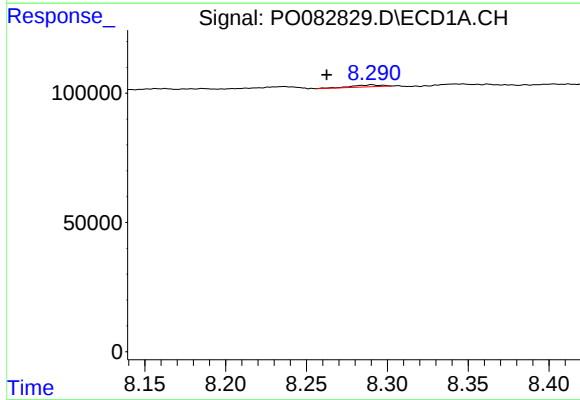

#32 AR-1260-2

R.T.: 8.290 min
Delta R.T.: 0.028 min
Response: 9459
Conc: 2.58 ng/ml

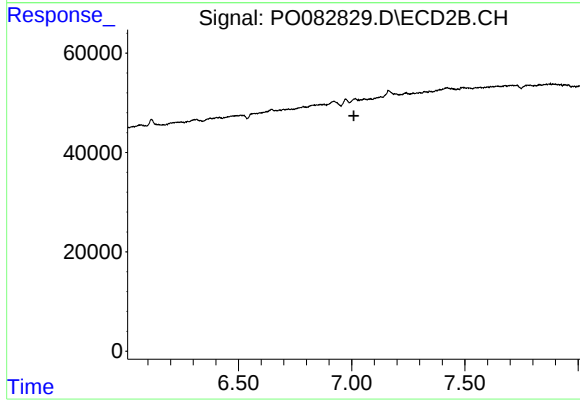

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.010 min
Response: 0
Conc: N.D.