

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111321\
 Data File : PO082818.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Nov 2021 19:38
 Operator : AJ\MA
 Sample : M4656-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-COMP

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/15/2021
 Supervised By :mohammad ahmed 11/15/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 01:08:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.961	1058474	545653	11.870m	16.816 #
2) SA Decachlor...	11.064	9.272	485281	244819	8.379	8.635

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO111321\
Data File : PO082818.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2021 19:38
Operator : AJ\MA
Sample : M4656-06
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_0
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/15/2021
Supervised By :mohammad ahmed 11/15/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 01:08:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

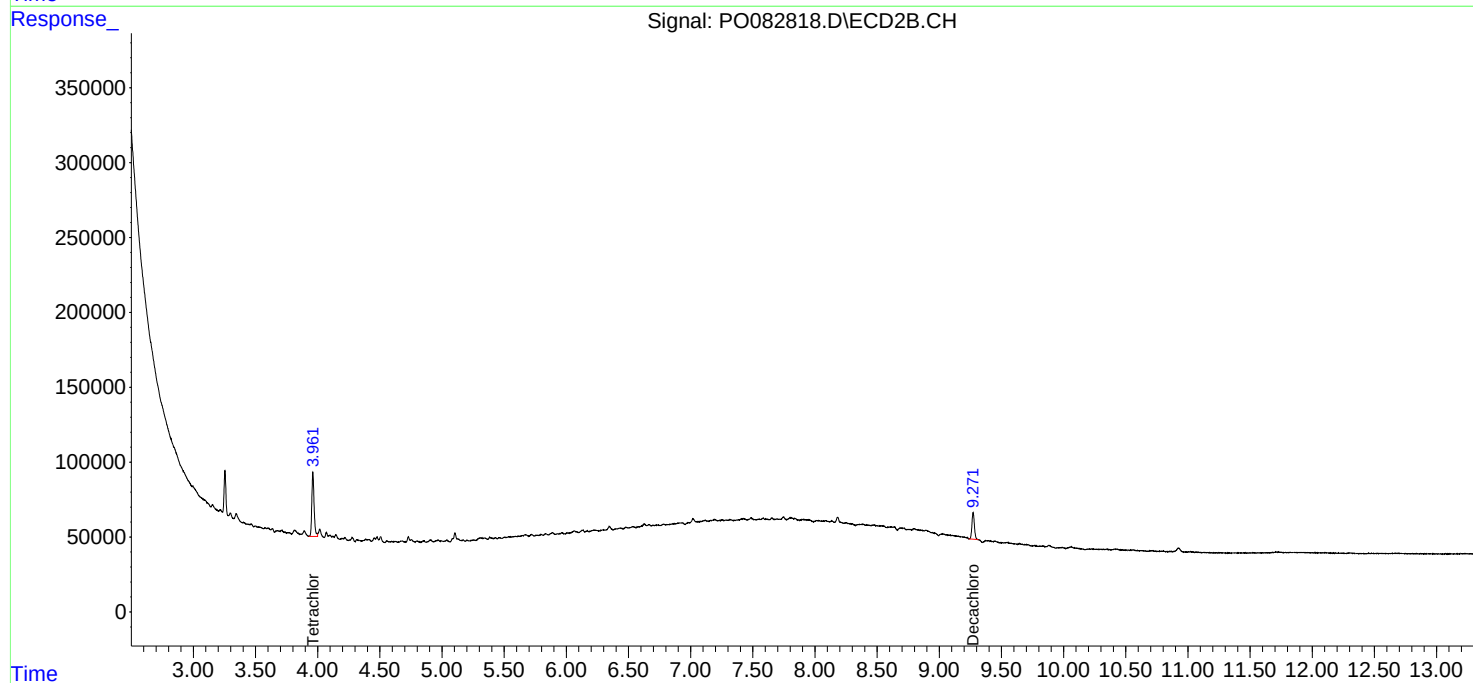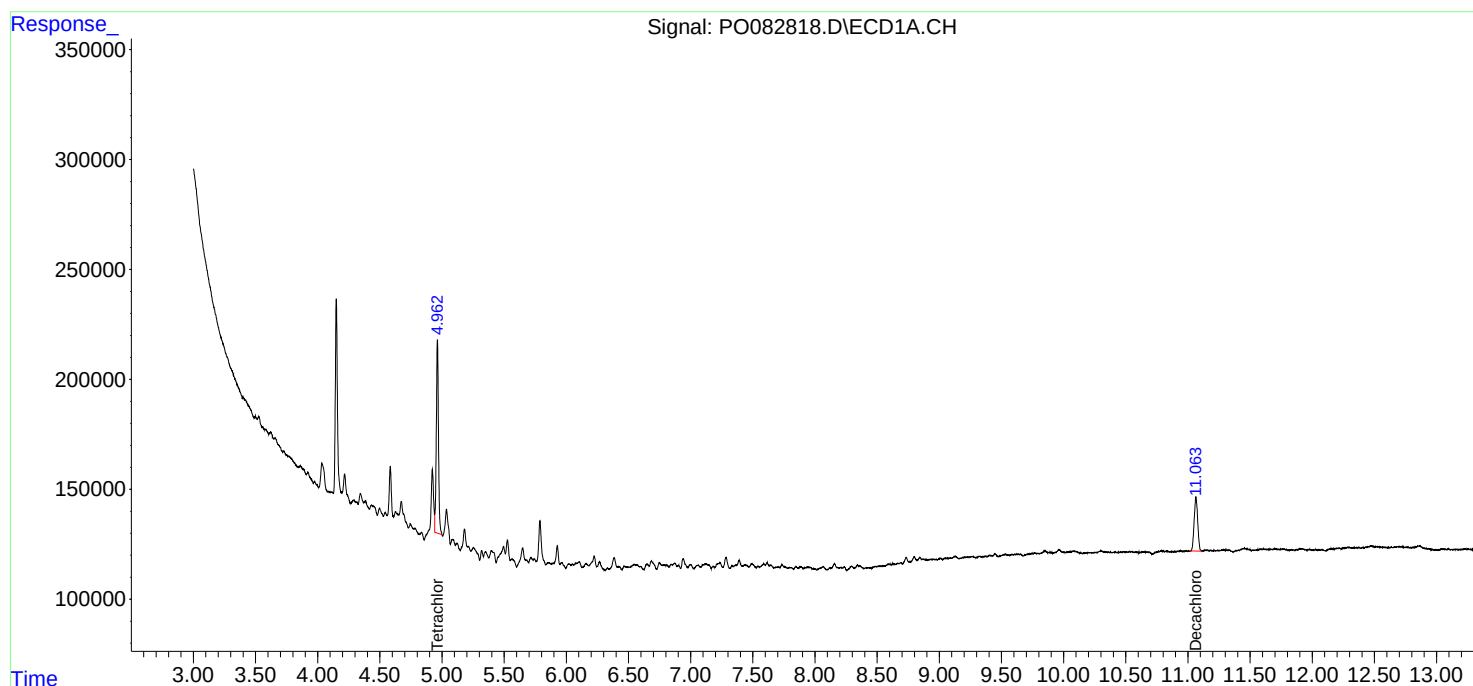

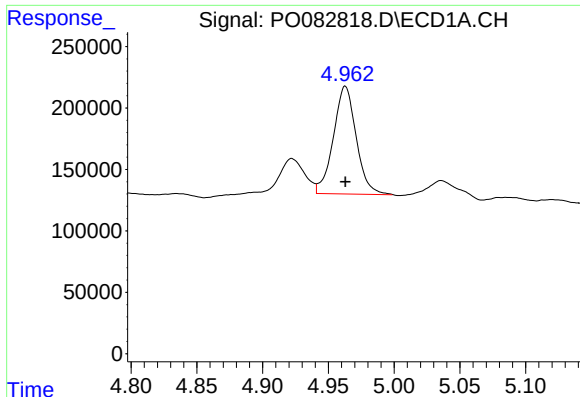


#1 Tetrachloro-m-xylene

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 1058474
Conc: 11.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/15/2021
Supervised By :mohammad ahmed 11/15/2021

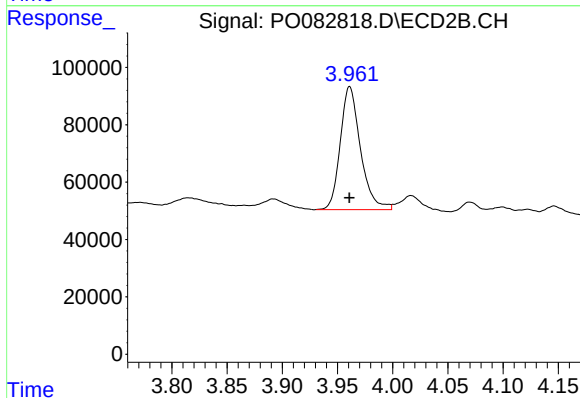


#1 Tetrachloro-m-xylene

R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 545653
Conc: 16.82 ng/ml

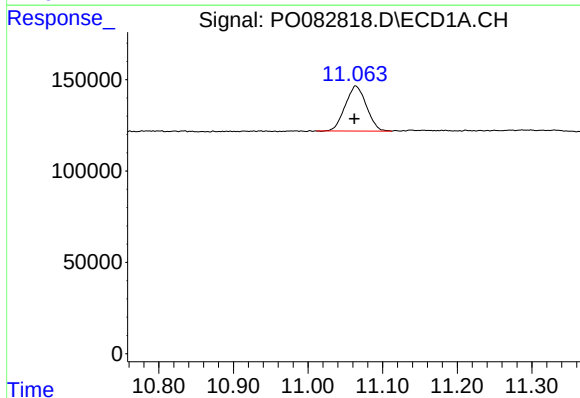

#2 Decachlorobiphenyl

R.T.: 11.064 min
Delta R.T.: 0.002 min
Response: 485281
Conc: 8.38 ng/ml

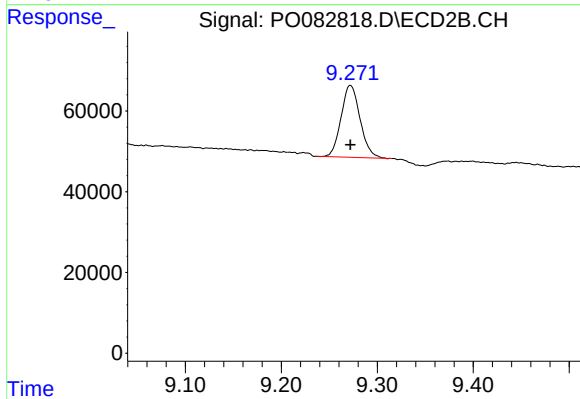

#2 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 244819
Conc: 8.63 ng/ml