

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111321\
Data File : PO082829.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2021 23:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 01:11:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.963	3.960	1723621	639620	19.330	19.712
2) SA Decachlor...	11.062	9.273	1281973	623970	22.136	22.007

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111321\
Data File : PO082829.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Nov 2021 23:05
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 01:11:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

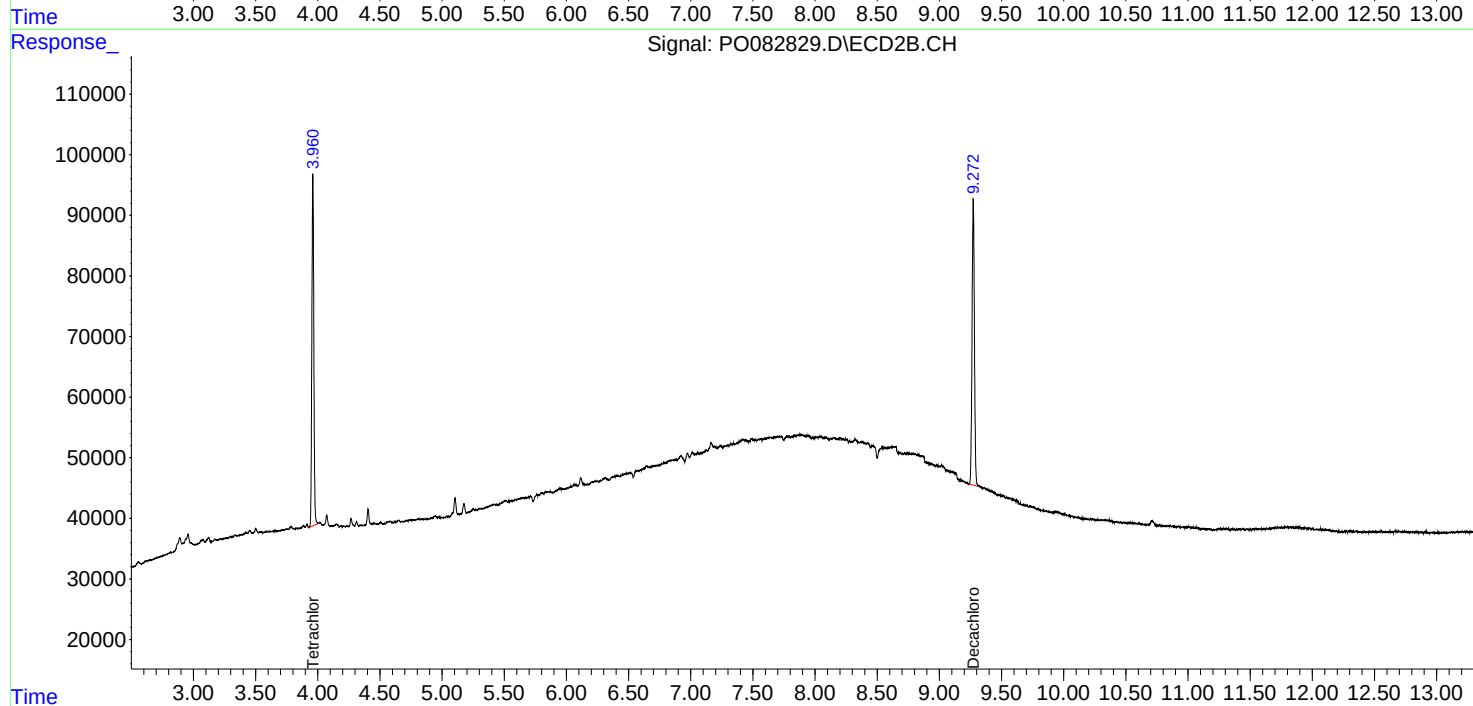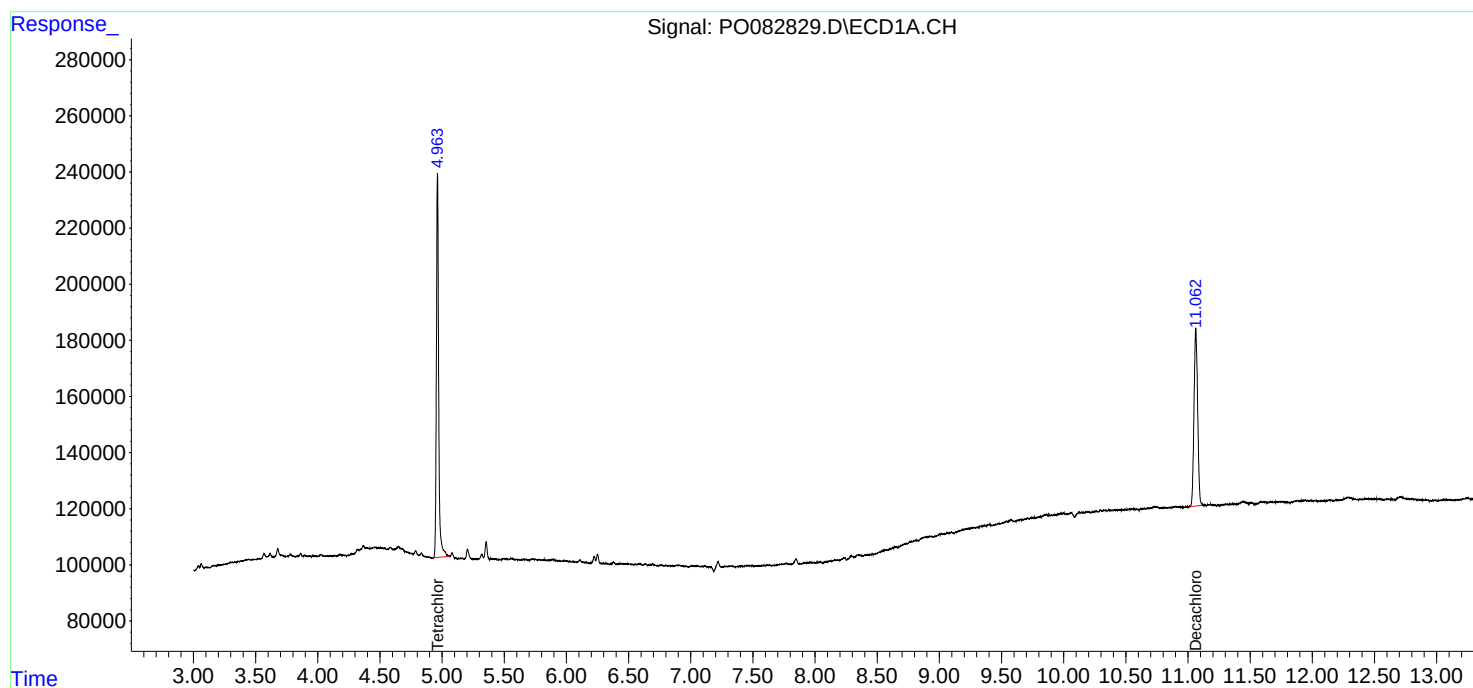


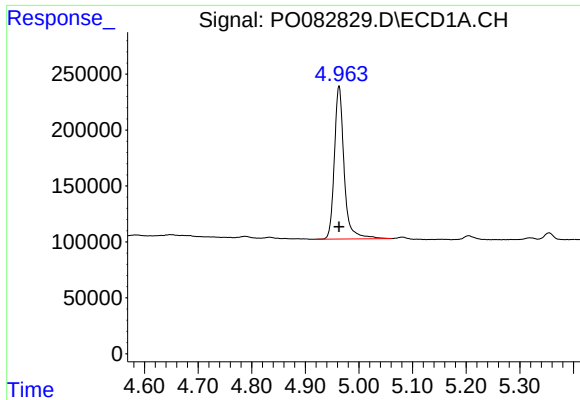

#1 Tetrachloro-m-xylene


R.T.: 4.963 min
Delta R.T.: 0.000 min
Response: 1723621
Conc: 19.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

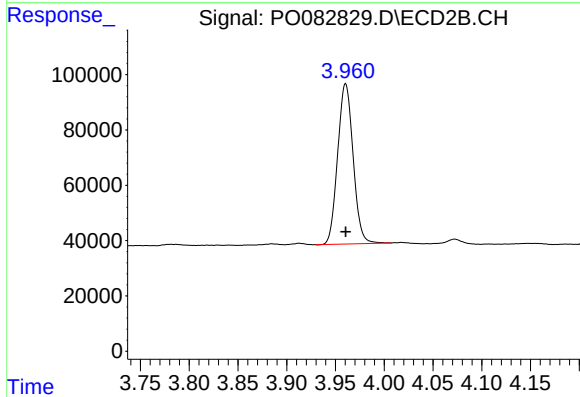


#1 Tetrachloro-m-xylene

R.T.: 3.960 min
Delta R.T.: 0.000 min
Response: 639620
Conc: 19.71 ng/ml

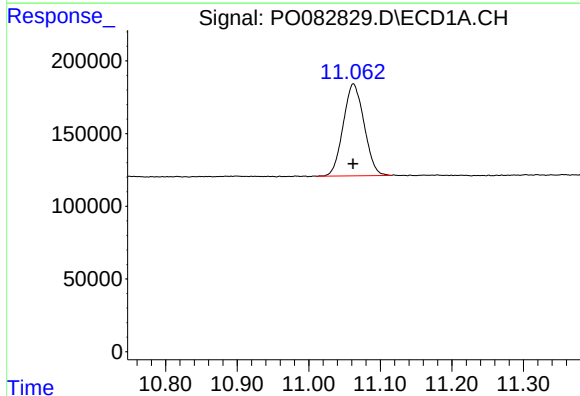

#2 Decachlorobiphenyl

R.T.: 11.062 min
Delta R.T.: 0.000 min
Response: 1281973
Conc: 22.14 ng/ml

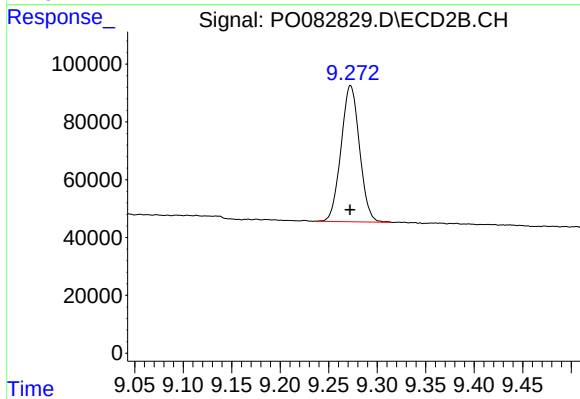

#2 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 623970
Conc: 22.01 ng/ml