

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO111321\  
 Data File : PO082853.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 13 Nov 2021 6:34  
 Operator : AJ\MA  
 Sample : M4655-14 10X  
 Misc :  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 MOO-2021-18-B

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 13 08:31:02 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO111221.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Nov 12 10:10:59 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml |
|-----------------------------|--------|-------|--------|--------|-------|-------|
| -----                       |        |       |        |        |       |       |
| System Monitoring Compounds |        |       |        |        |       |       |
| 1) SA Tetrachlo...          | 4.963  | 3.959 | 114975 | 47231  | 1.289 | 1.456 |
| 2) SA Decachlor...          | 11.067 | 9.273 | 110344 | 42037  | 1.905 | 1.483 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO111321\  
Data File : P0082853.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 13 Nov 2021 6:34  
Operator : AJ\MA  
Sample : M4655-14 10X  
Misc :  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
MOO-2021-18-B

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 13 08:31:02 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO111221.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Nov 12 10:10:59 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

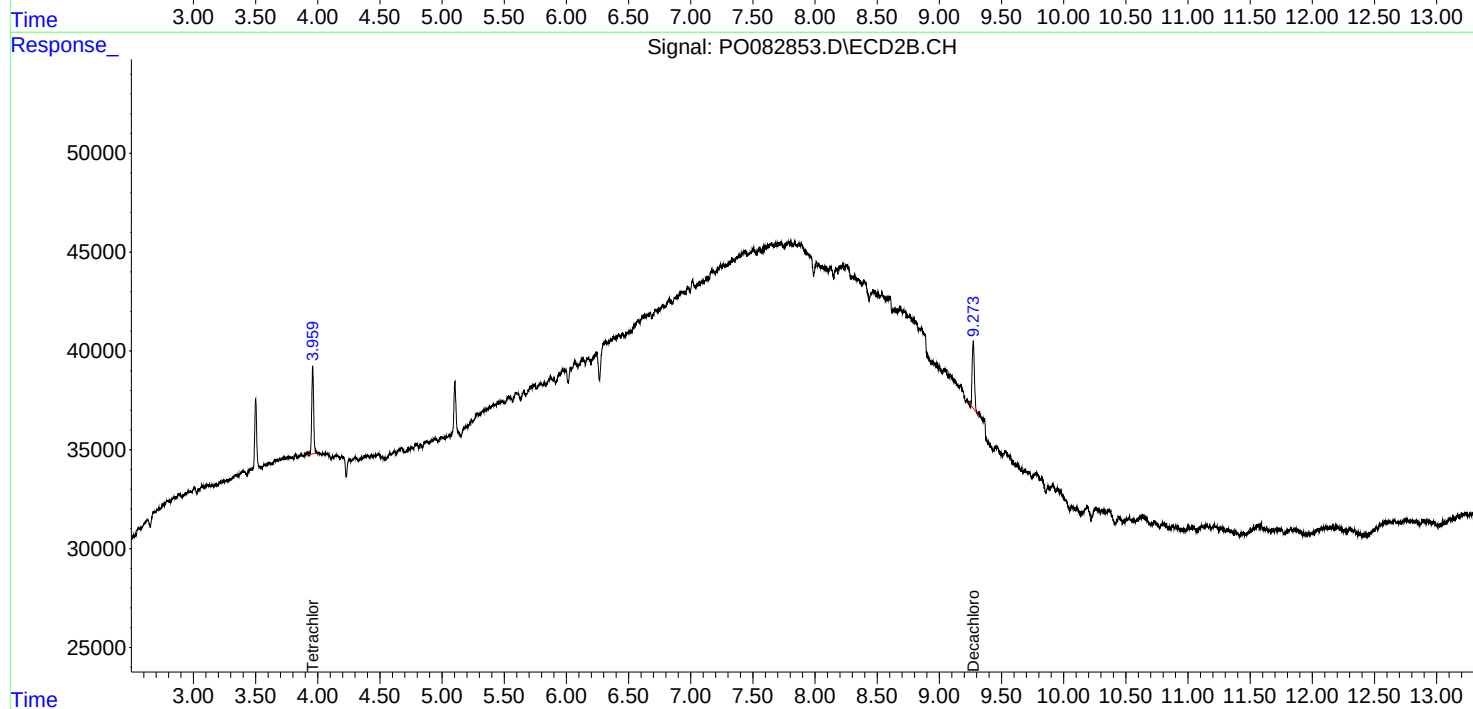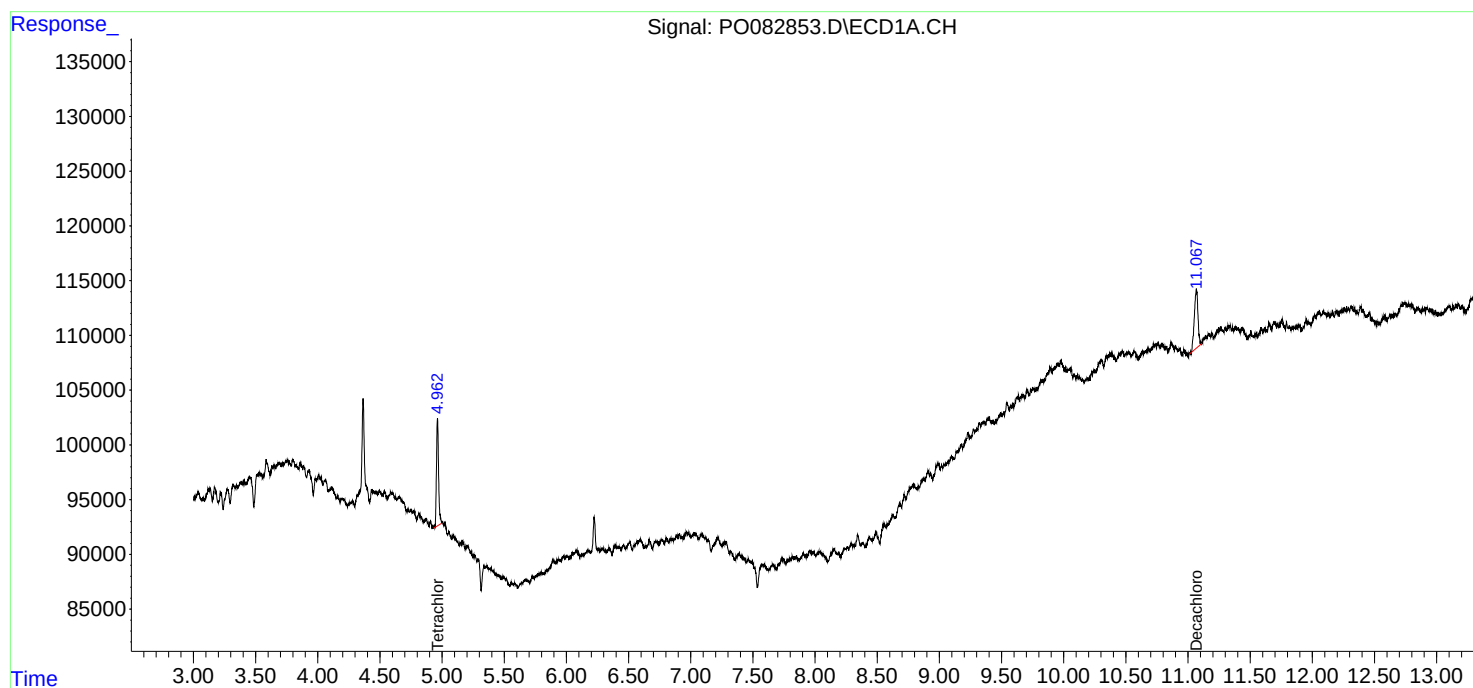


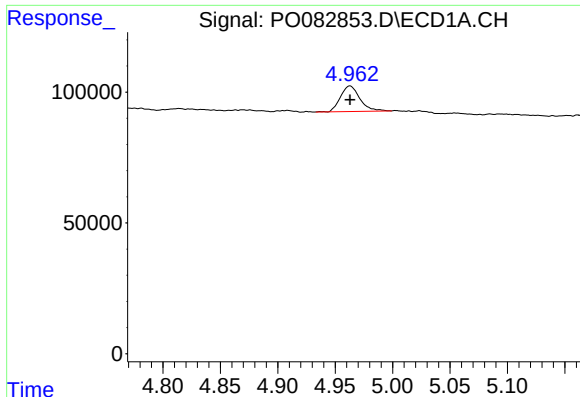

#1 Tetrachloro-m-xylene


R.T.: 4.963 min  
Delta R.T.: 0.000 min  
Response: 114975  
Conc: 1.29 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
MOO-2021-18-B

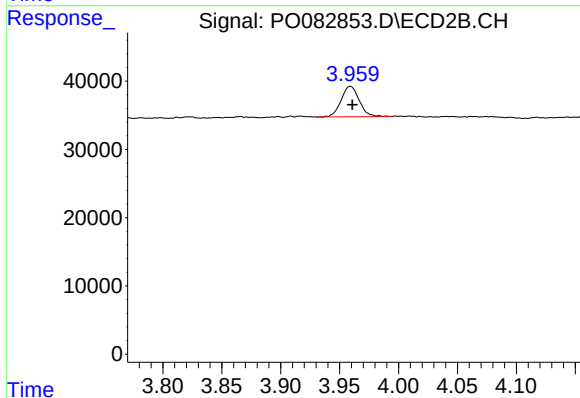


#1 Tetrachloro-m-xylene

R.T.: 3.959 min  
Delta R.T.: -0.002 min  
Response: 47231  
Conc: 1.46 ng/ml

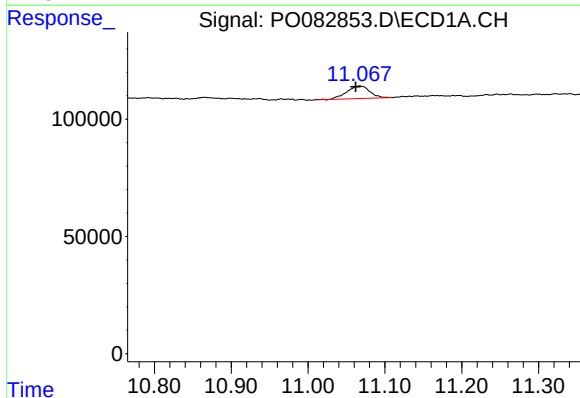

#2 Decachlorobiphenyl

R.T.: 11.067 min  
Delta R.T.: 0.005 min  
Response: 110344  
Conc: 1.91 ng/ml

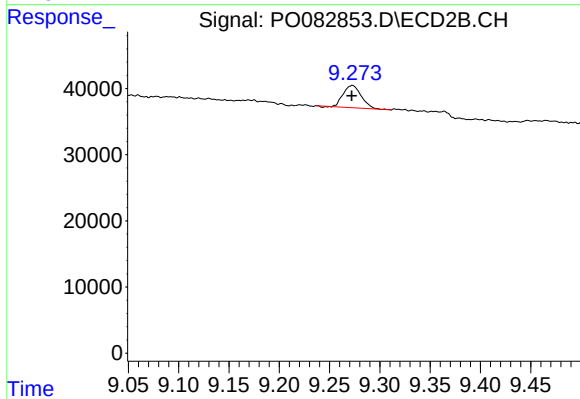

#2 Decachlorobiphenyl

R.T.: 9.273 min  
Delta R.T.: 0.000 min  
Response: 42037  
Conc: 1.48 ng/ml