

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111321\
 Data File : P0082860.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Nov 2021 9:09
 Operator : AJ\MA
 Sample : M4655-16 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-2021-19-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:30:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 12 10:10:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.962	3.959	154271	59222	1.730	1.825
2) SA Decachlor...	11.064	9.272	116593	42272	2.013	1.491 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111321\
Data File : P0082860.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2021 9:09
Operator : AJ\MA
Sample : M4655-16 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MOO-2021-19-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:30:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 12 10:10:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

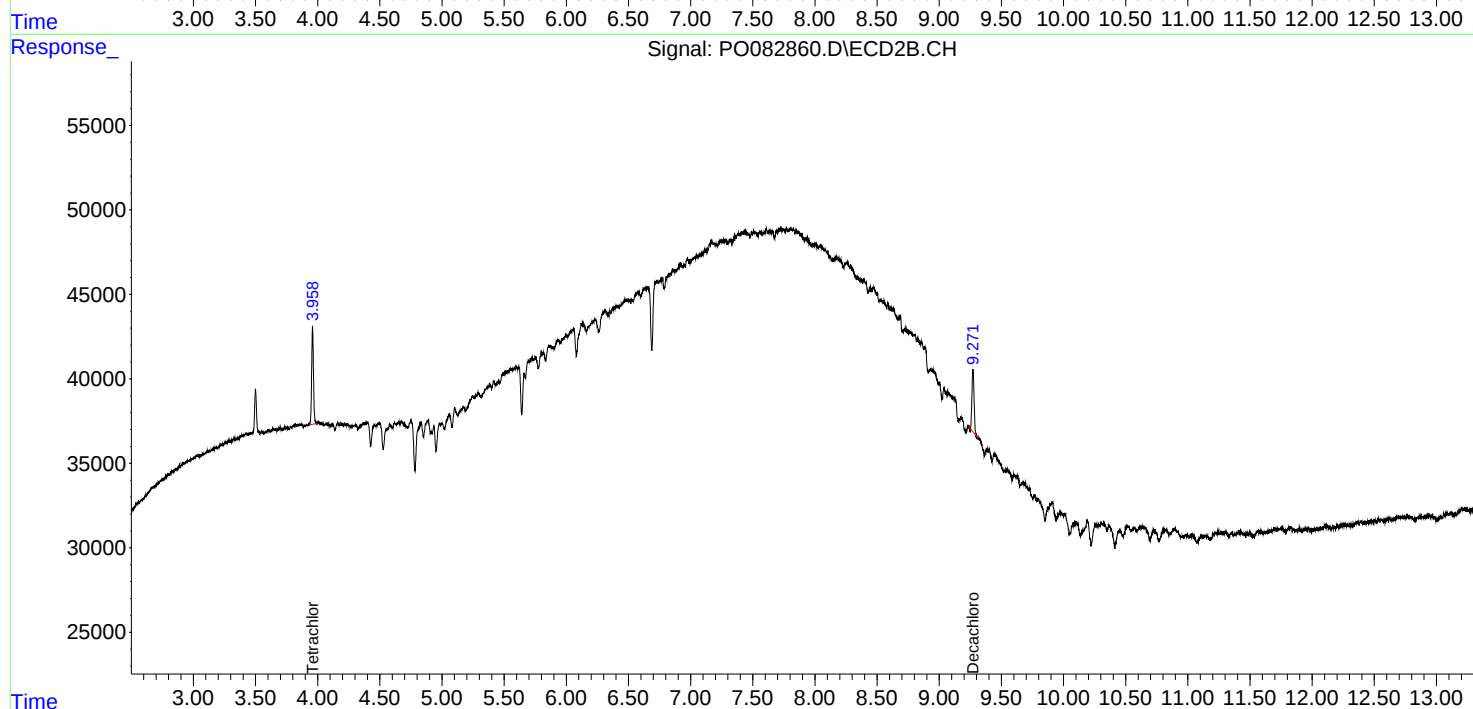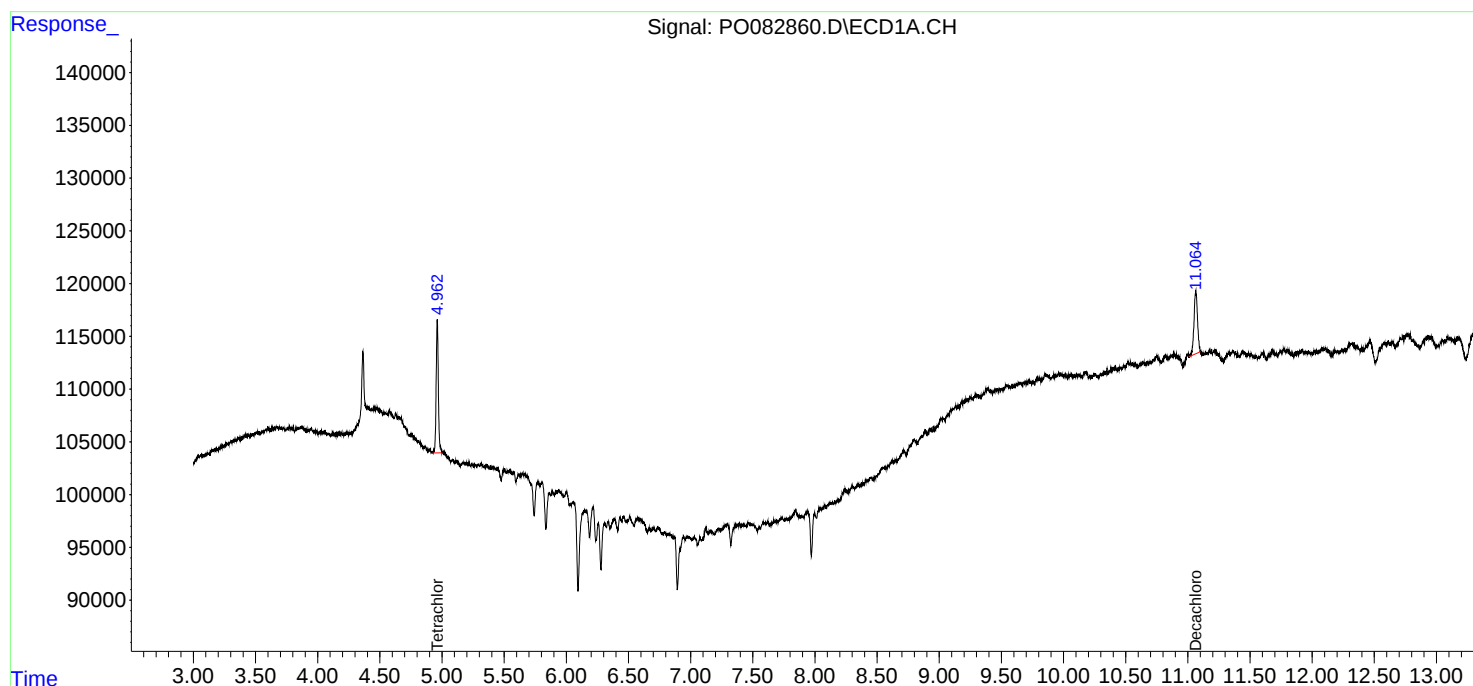


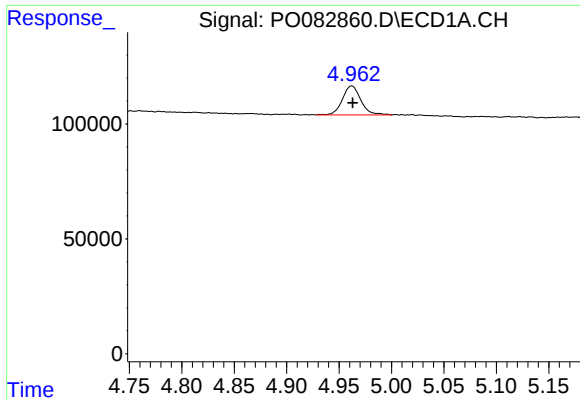

#1 Tetrachloro-m-xylene


R.T.: 4.962 min
Delta R.T.: -0.001 min
Response: 154271
Conc: 1.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-2021-19-B

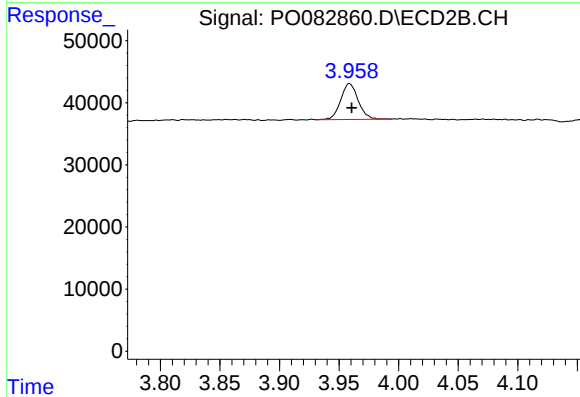


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: -0.002 min
Response: 59222
Conc: 1.83 ng/ml

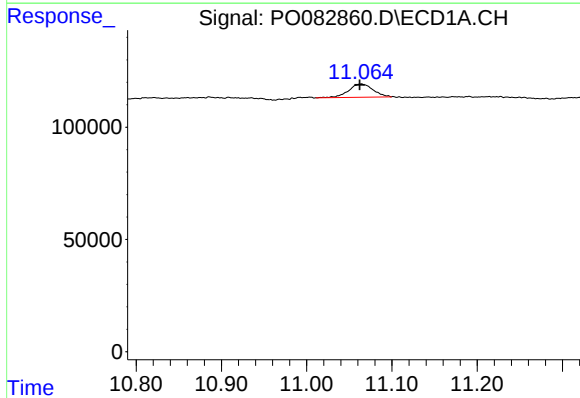

#2 Decachlorobiphenyl

R.T.: 11.064 min
Delta R.T.: 0.002 min
Response: 116593
Conc: 2.01 ng/ml

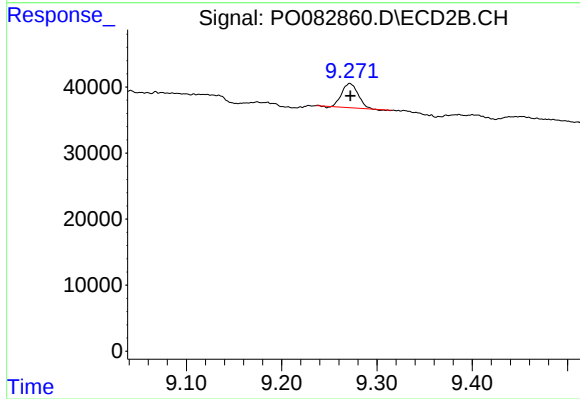

#2 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.000 min
Response: 42272
Conc: 1.49 ng/ml