

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111324\
 Data File : P0107946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 20:11
 Operator : YP/AJ
 Sample : P4813-04 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 419

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :Ankita Jodhani 11/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 23:47:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 12 01:21:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.370	3.638	20546268	7439279	2.289m	2.215m
2) SA Decachlor...	10.082	8.633	4790559	4458969	1.616m	1.411

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111324\
Data File : PO107946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 20:11
Operator : YP/AJ
Sample : P4813-04 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
419


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :Ankita Jodhani 11/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 23:47:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 12 01:21:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

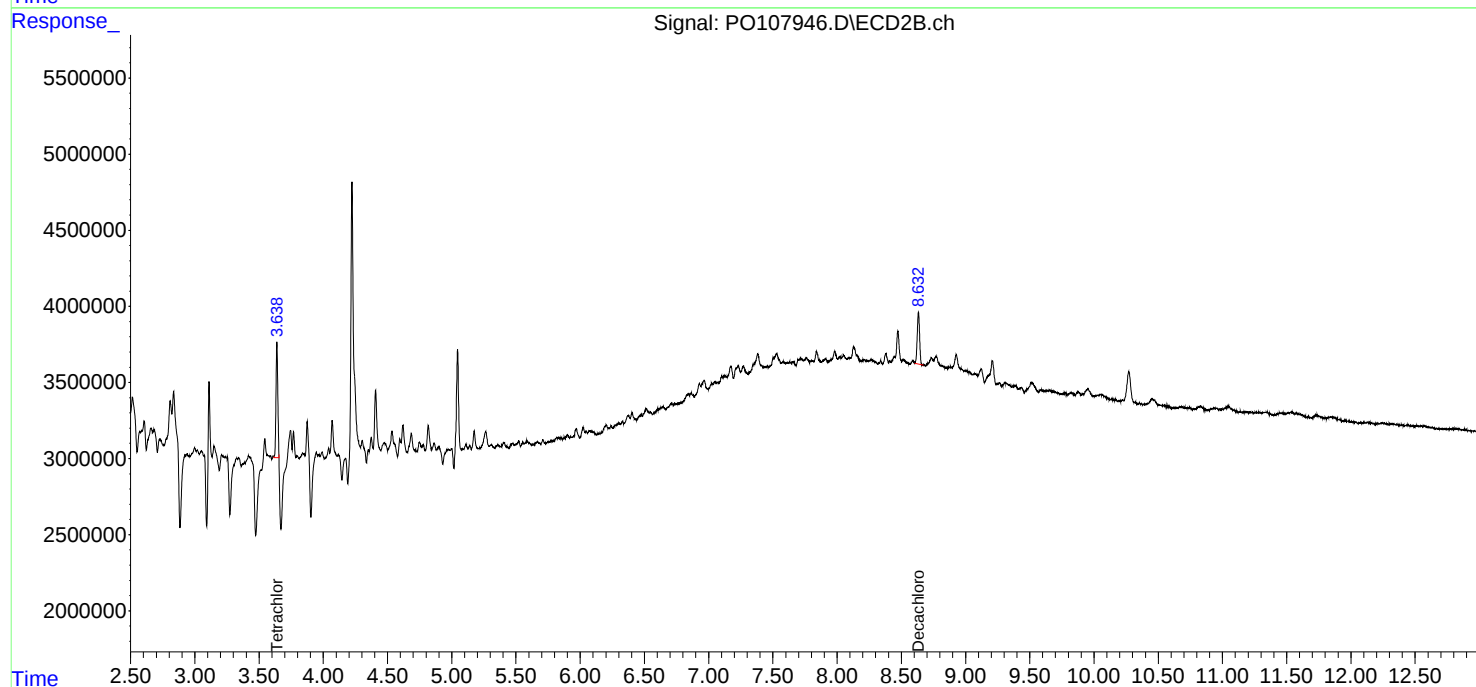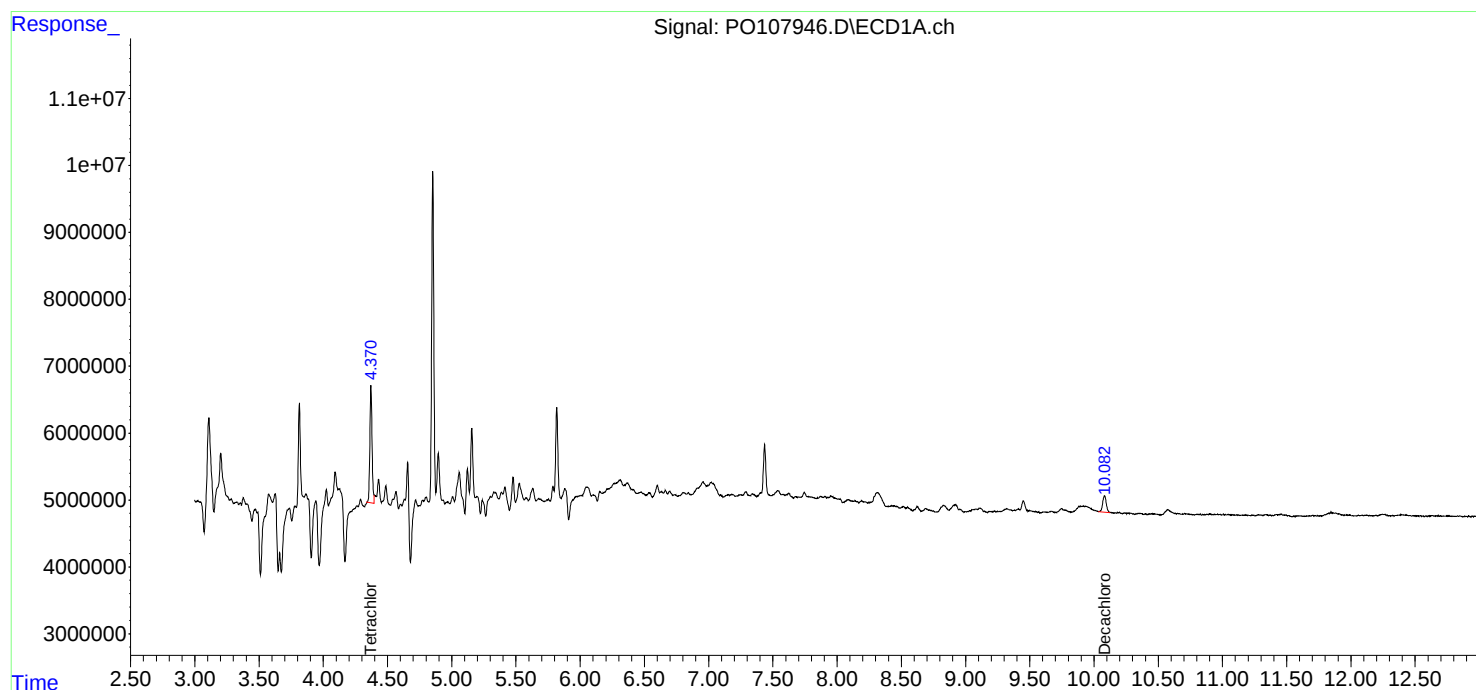

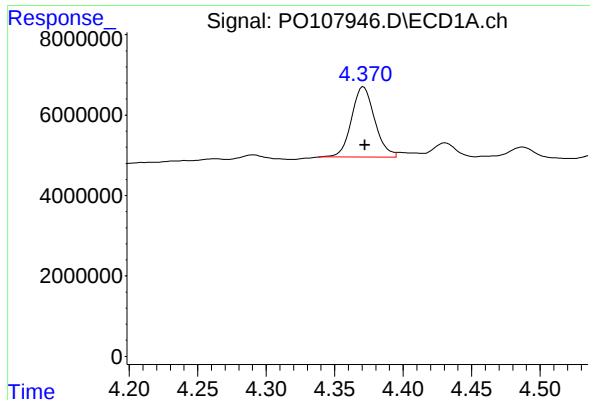


#1 Tetrachloro-m-xylene

R.T.: 4.370 min
Delta R.T.: -0.002 min
Response: 20546268
Conc: 2.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
419


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :Ankita Jodhani 11/14/2024

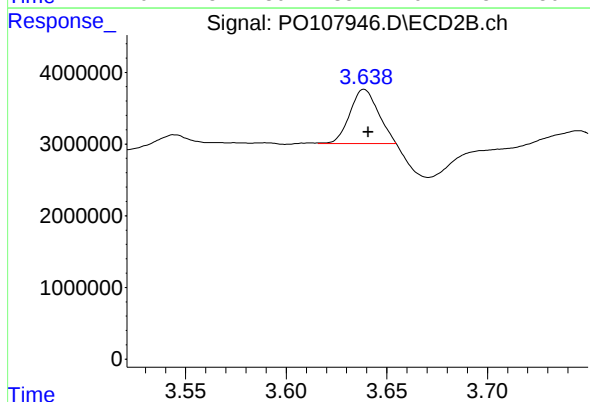


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 7439279
Conc: 2.21 ng/ml

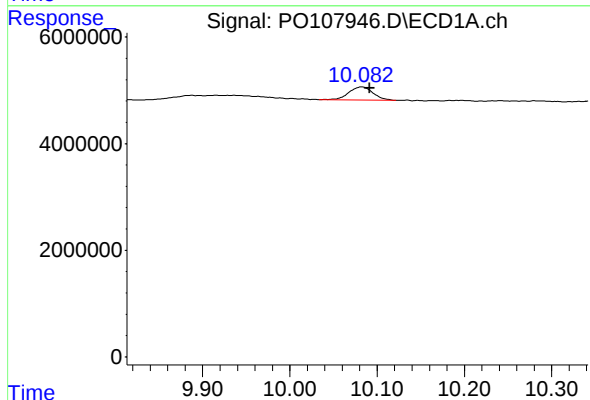

#2 Decachlorobiphenyl

R.T.: 10.082 min
Delta R.T.: -0.010 min
Response: 4790559
Conc: 1.62 ng/ml

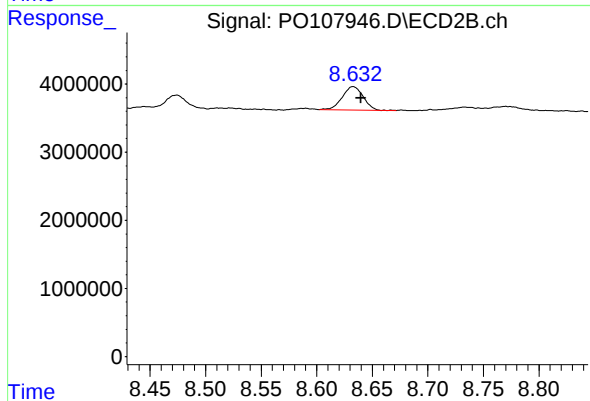

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.007 min
Response: 4458969
Conc: 1.41 ng/ml