

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111324\
 Data File : P0107951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 22:02
 Operator : YP/AJ
 Sample : P4819-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1594

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2024
 Supervised By :Ankita Jodhani 11/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 23:50:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111124.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 12 01:21:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.369	3.639	175.6E6	76370926	19.557m	22.739
2) SA Decachlor...	10.079	8.633	53302465	58968108	17.981	18.666

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111324\
Data File : PO107951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 22:02
Operator : YP/AJ
Sample : P4819-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1594


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :Ankita Jodhani 11/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 23:50:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111124.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 12 01:21:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

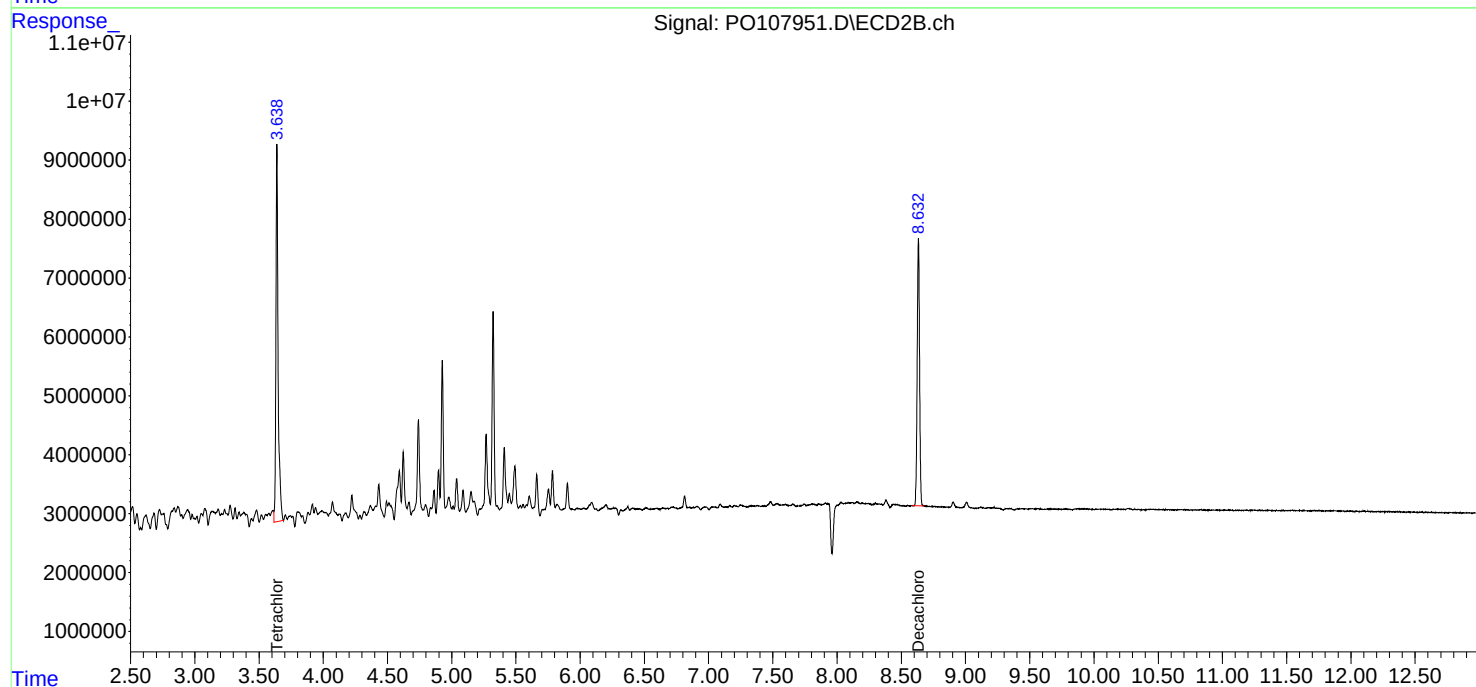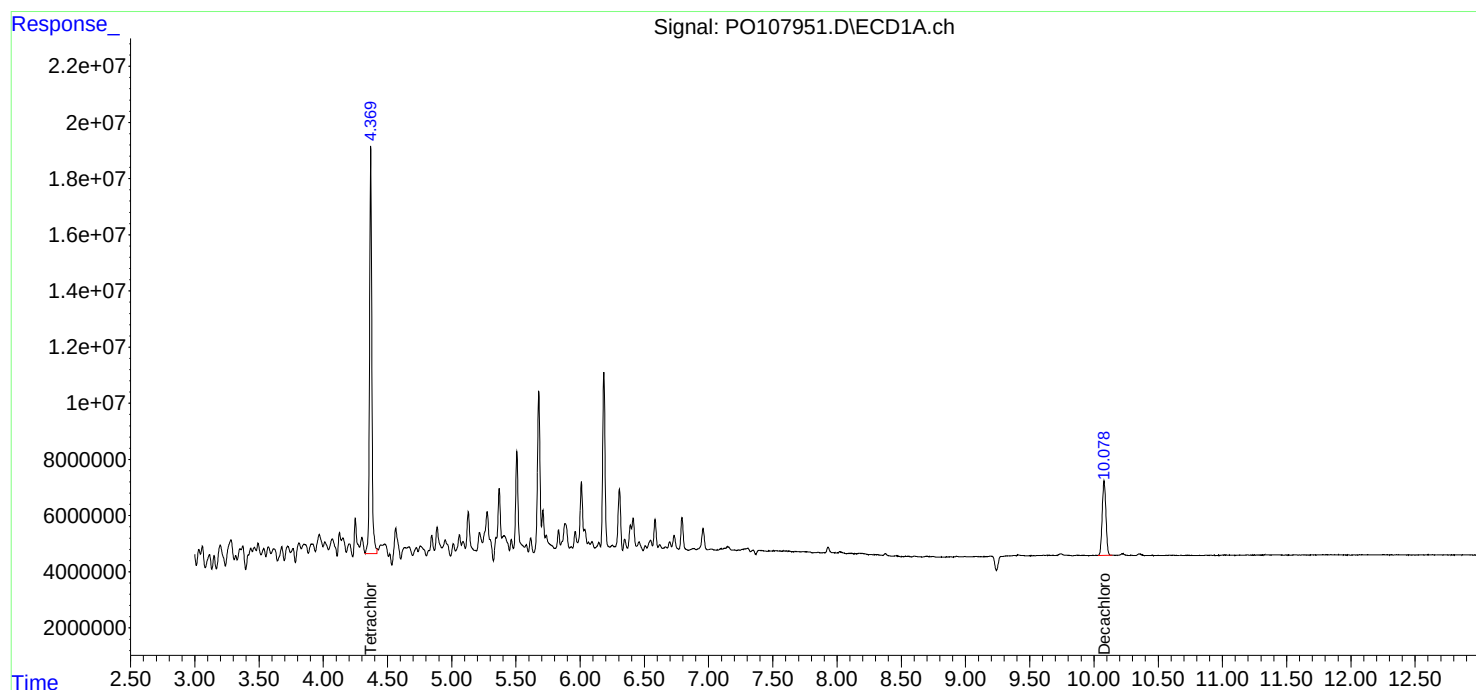

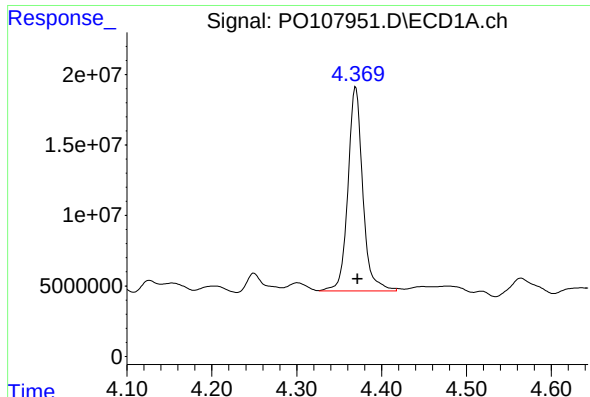


#1 Tetrachloro-m-xylene

R.T.: 4.369 min
Delta R.T.: -0.003 min
Response: 175553938
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
1594


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2024
Supervised By :Ankita Jodhani 11/14/2024

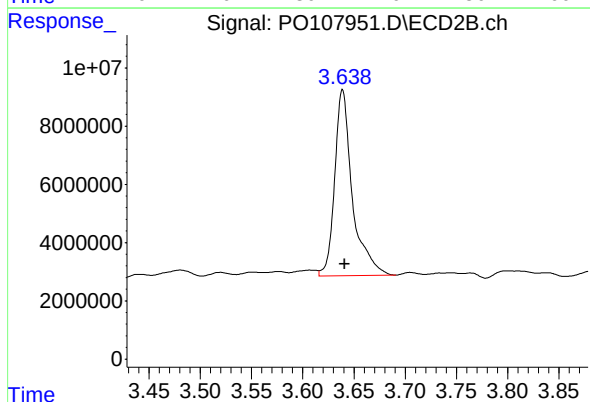


#1 Tetrachloro-m-xylene

R.T.: 3.639 min
Delta R.T.: -0.002 min
Response: 76370926
Conc: 22.74 ng/ml

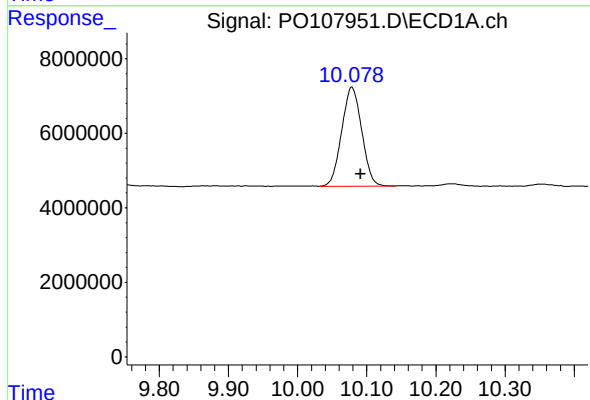

#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: -0.013 min
Response: 53302465
Conc: 17.98 ng/ml

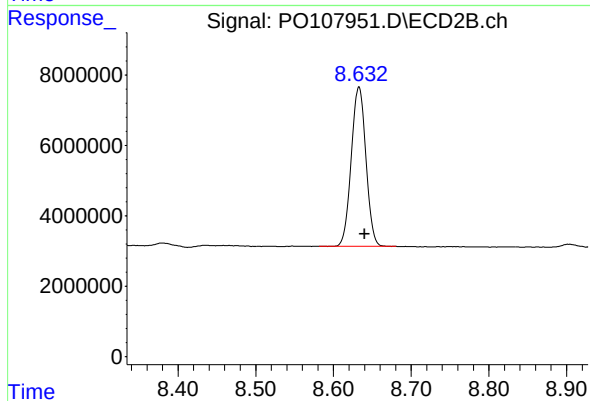

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.007 min
Response: 58968108
Conc: 18.67 ng/ml