

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111325\
 Data File : PO115088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2025 18:36
 Operator : YP/AJ
 Sample : Q3624-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-11122025

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/14/2025
 Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 01:15:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 05 06:00:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.647	149.4E6	102.2E6	21.225m	22.870
2) SA Decachlor...	9.928	8.638	285.3E6	223.2E6	64.533	57.185

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111325\
Data File : PO115088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2025 18:36
Operator : YP/AJ
Sample : Q3624-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-11122025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/14/2025
Supervised By :Sohil Jodhani 11/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 01:15:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110425.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 05 06:00:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

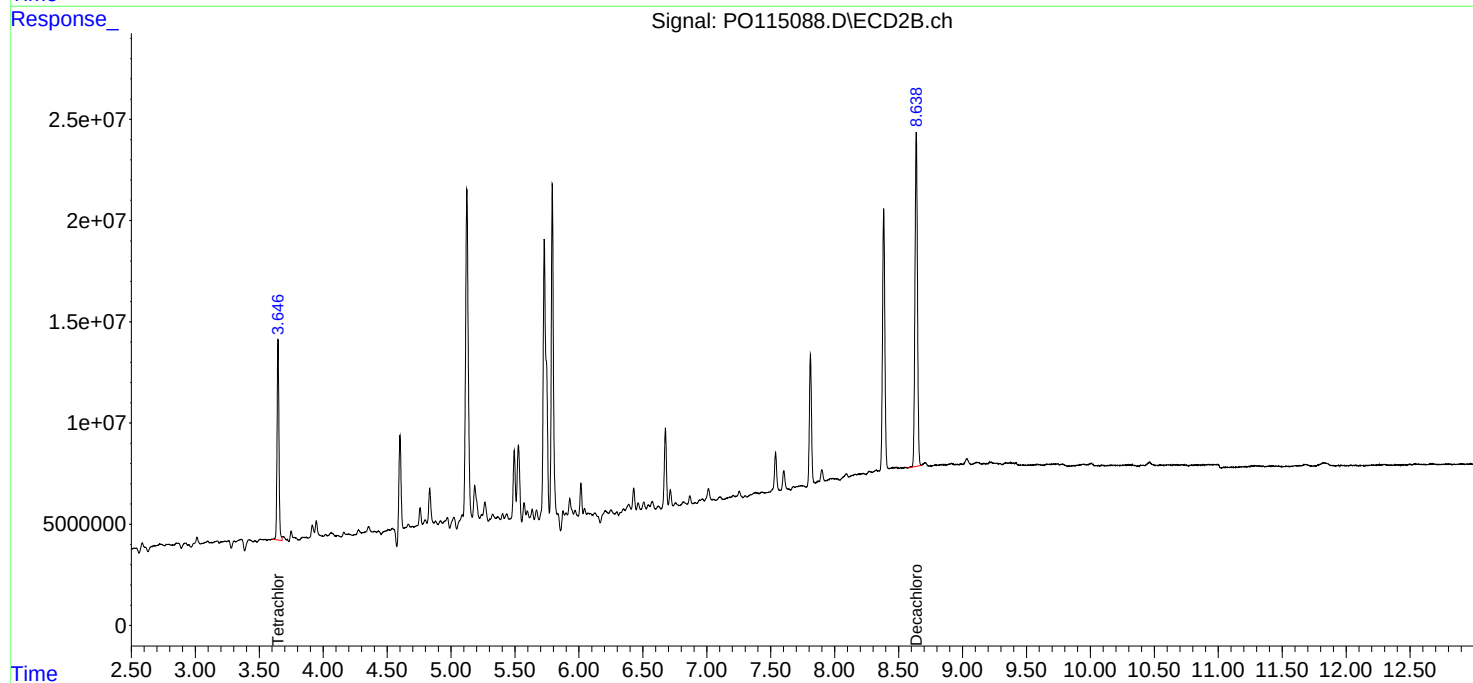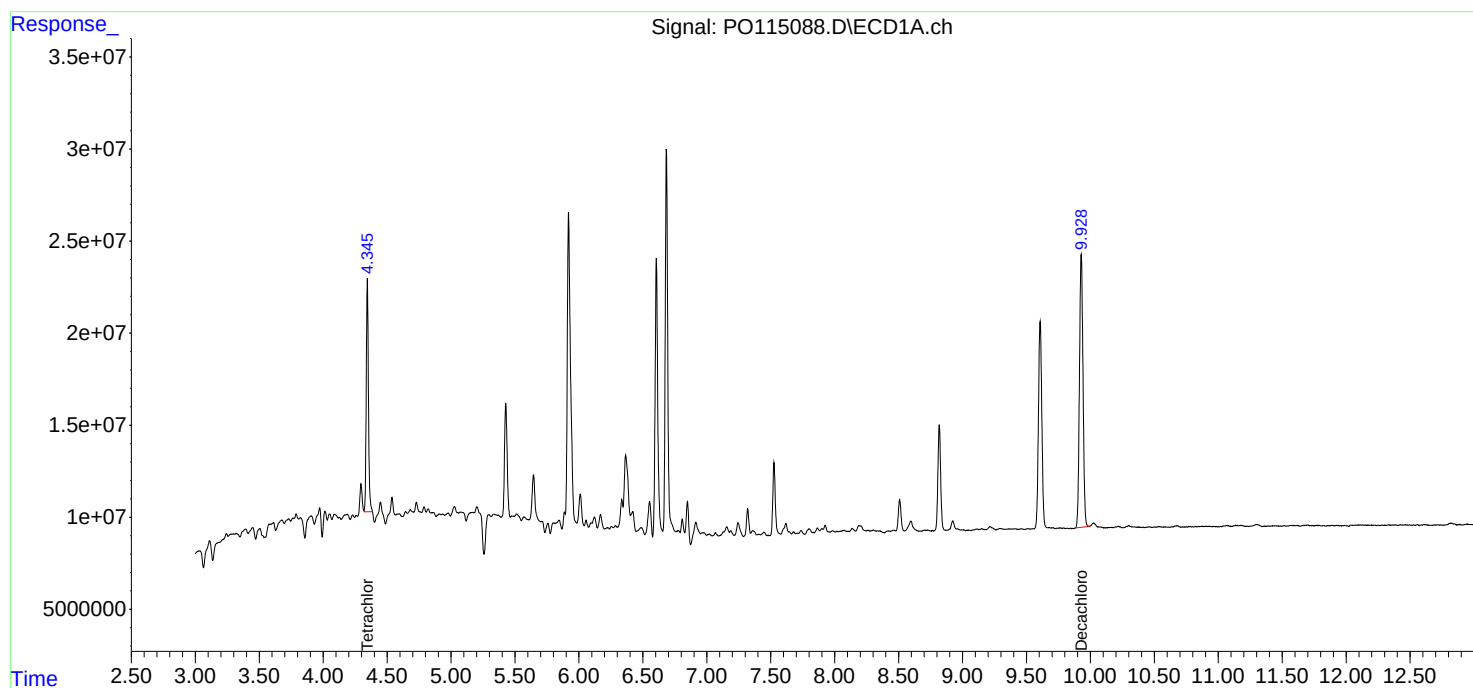

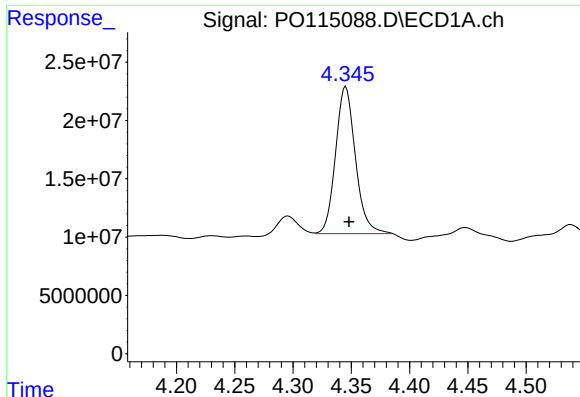


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: -0.003 min
Response: 149385468
Conc: 21.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-02-11122025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/14/2025
Supervised By :Sohil Jodhani 11/14/2025

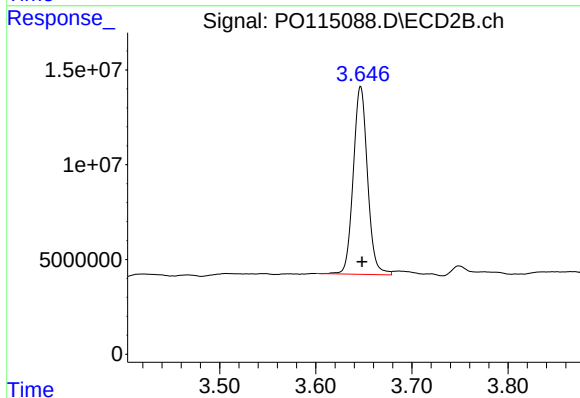


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: -0.002 min
Response: 102154352
Conc: 22.87 ng/ml

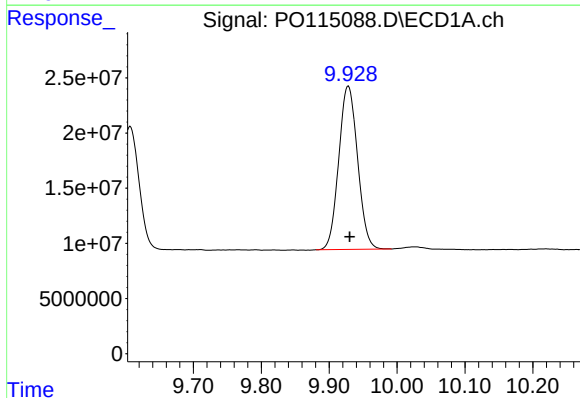

#2 Decachlorobiphenyl

R.T.: 9.928 min
Delta R.T.: -0.002 min
Response: 285252296
Conc: 64.53 ng/ml

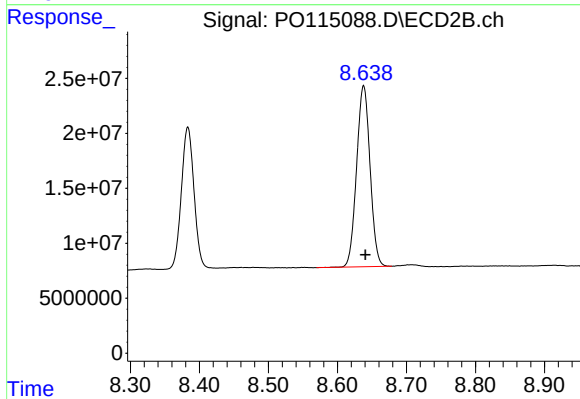

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: -0.003 min
Response: 223238614
Conc: 57.18 ng/ml