

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111418\
Data File : P0051542.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Nov 2018 18:03
Operator : SM/SJ
Sample : J5921-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-TANK2-N48963

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 23:52:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 14 08:52:41 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.311	3.307	51069559	18163721	15.991	16.495
2) SA Decachlor...	9.950	8.053	24332204	10884922	12.678	13.131

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111418\
Data File : PO051542.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Nov 2018 18:03
Operator : SM/SJ
Sample : J5921-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SP-TANK2-N48963

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 23:52:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111318.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 14 08:52:41 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

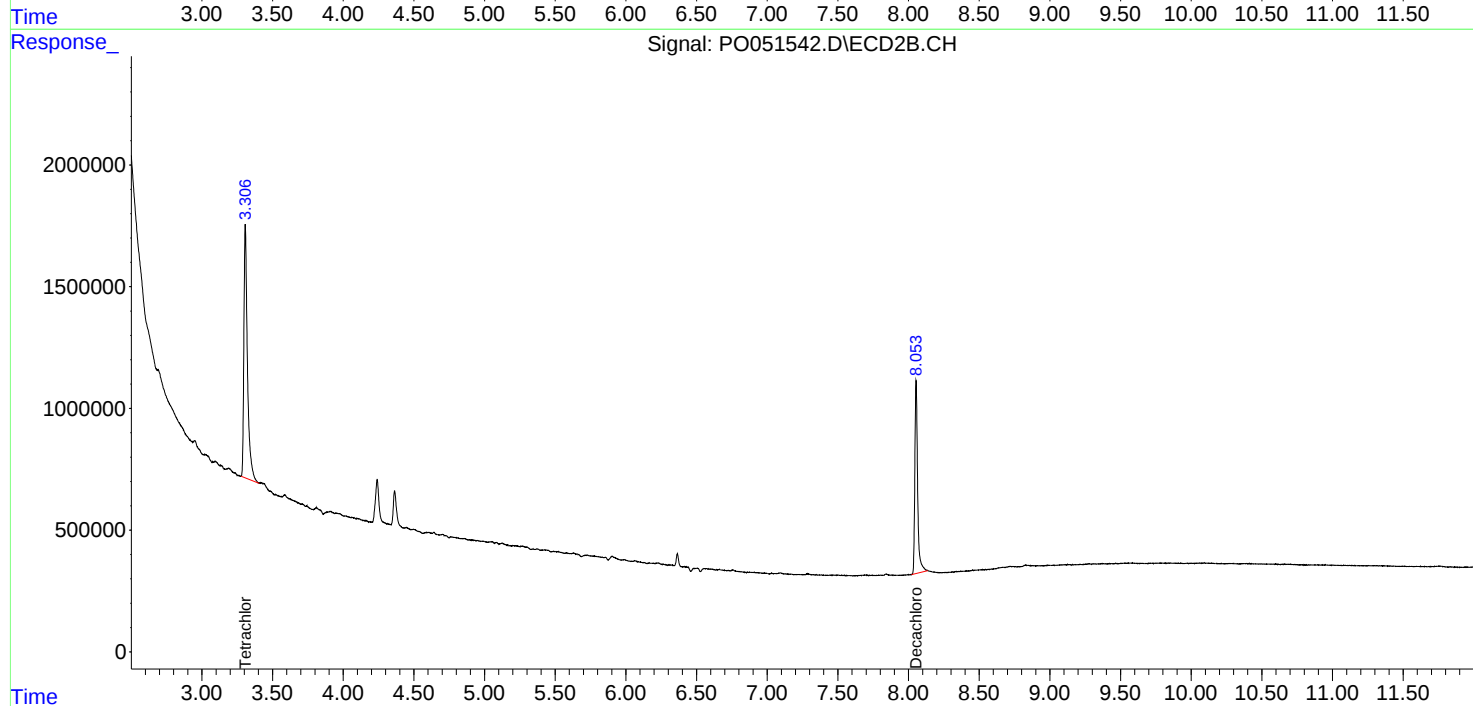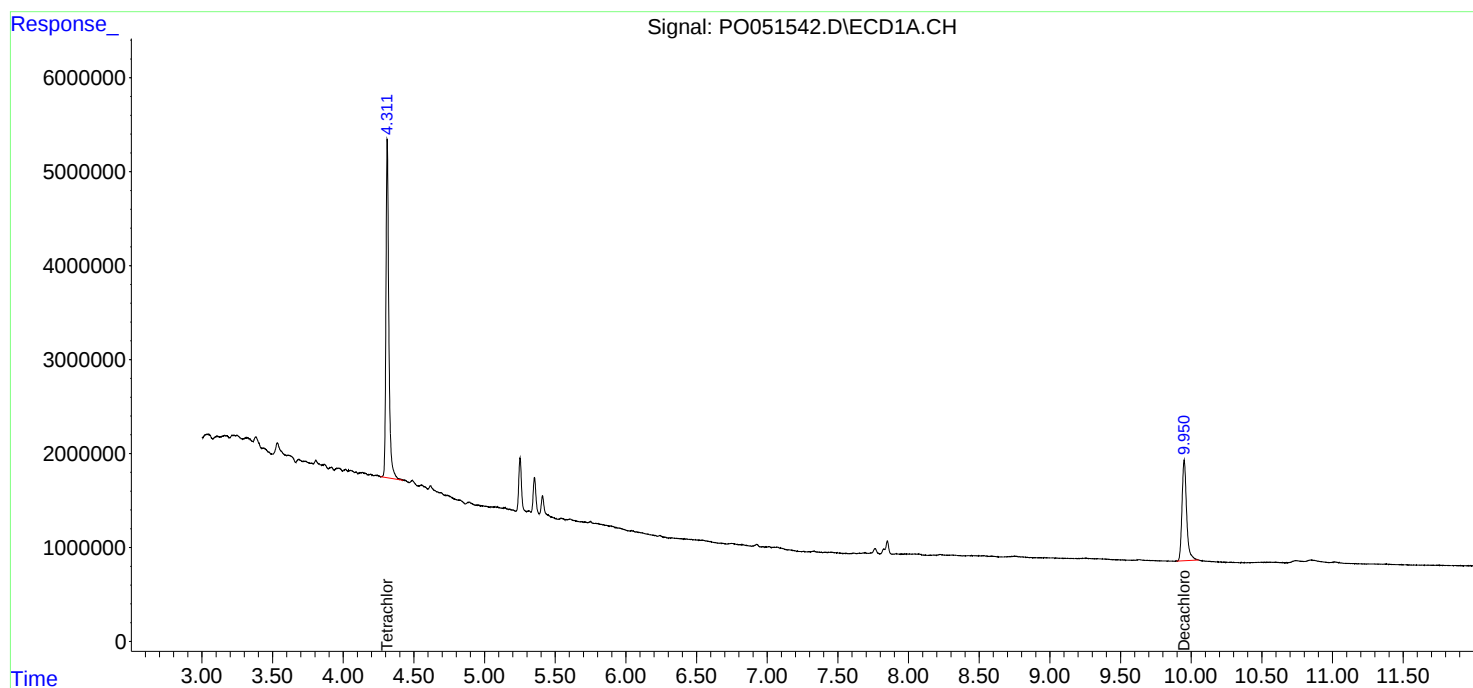


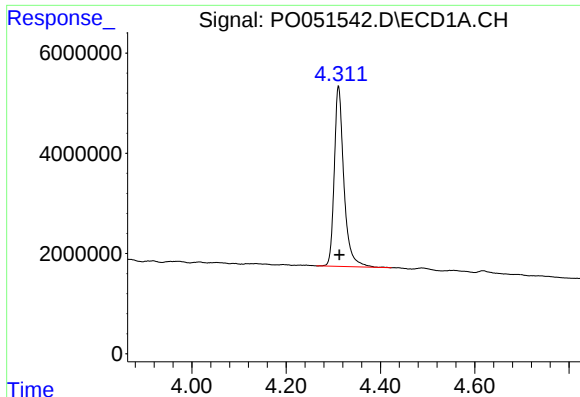

#1 Tetrachloro-m-xylene


R.T.: 4.311 min
Delta R.T.: -0.002 min
Response: 51069559
Conc: 15.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-TANK2-N48963

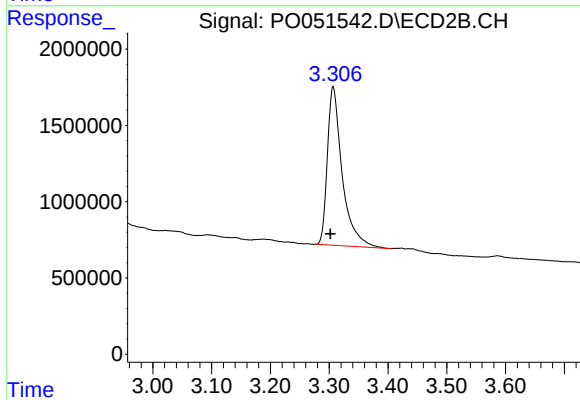


#1 Tetrachloro-m-xylene

R.T.: 3.307 min
Delta R.T.: 0.004 min
Response: 18163721
Conc: 16.49 ng/ml

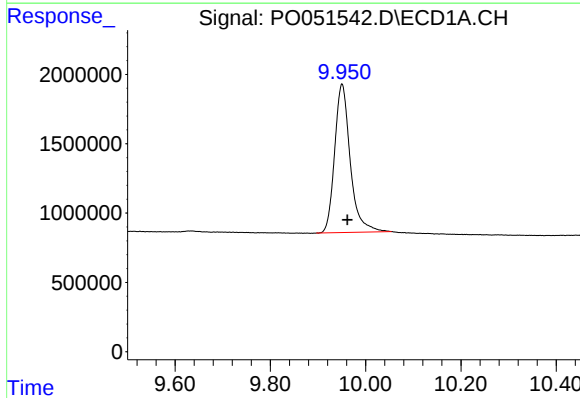

#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.011 min
Response: 24332204
Conc: 12.68 ng/ml

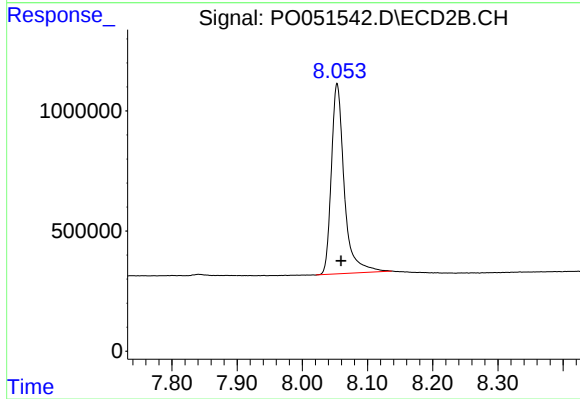

#2 Decachlorobiphenyl

R.T.: 8.053 min
Delta R.T.: -0.006 min
Response: 10884922
Conc: 13.13 ng/ml