

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111419\
 Data File : P0063714.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Nov 2019 21:50
 Operator : SM/AJ
 Sample : K5804-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GE-MW-58-1S

Manual Integrations
 APPROVED

Ankita
 11/15/2019 9:43:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 01:37:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.313	3.575	1401234	63077019	45.829m	2839.860m#
2) SA Decachlor...	9.936	8.539	900109	595037	22.151	20.345

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111419\
Data File : PO063714.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Nov 2019 21:50
Operator : SM/AJ
Sample : K5804-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GE-MW-58-1S


Manual Integrations
APPROVED

Ankita
11/15/2019 9:43:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 01:37:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

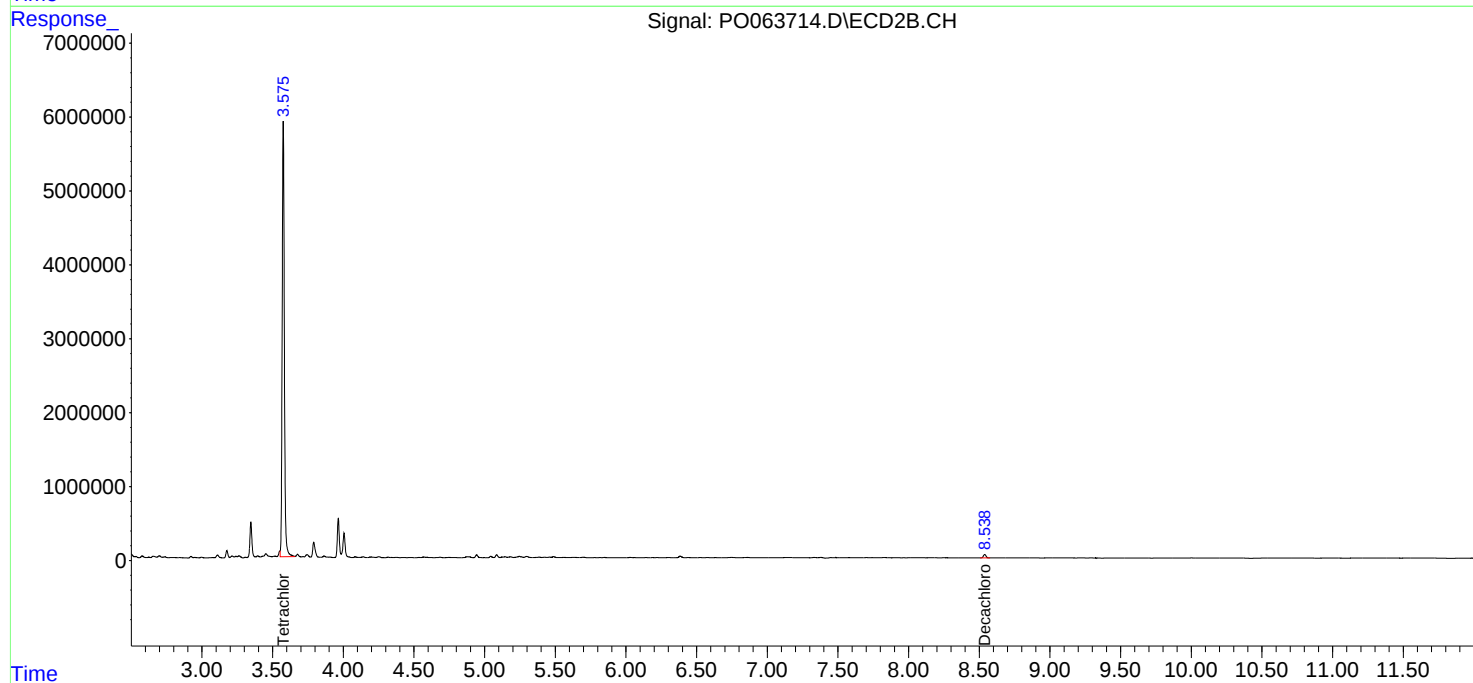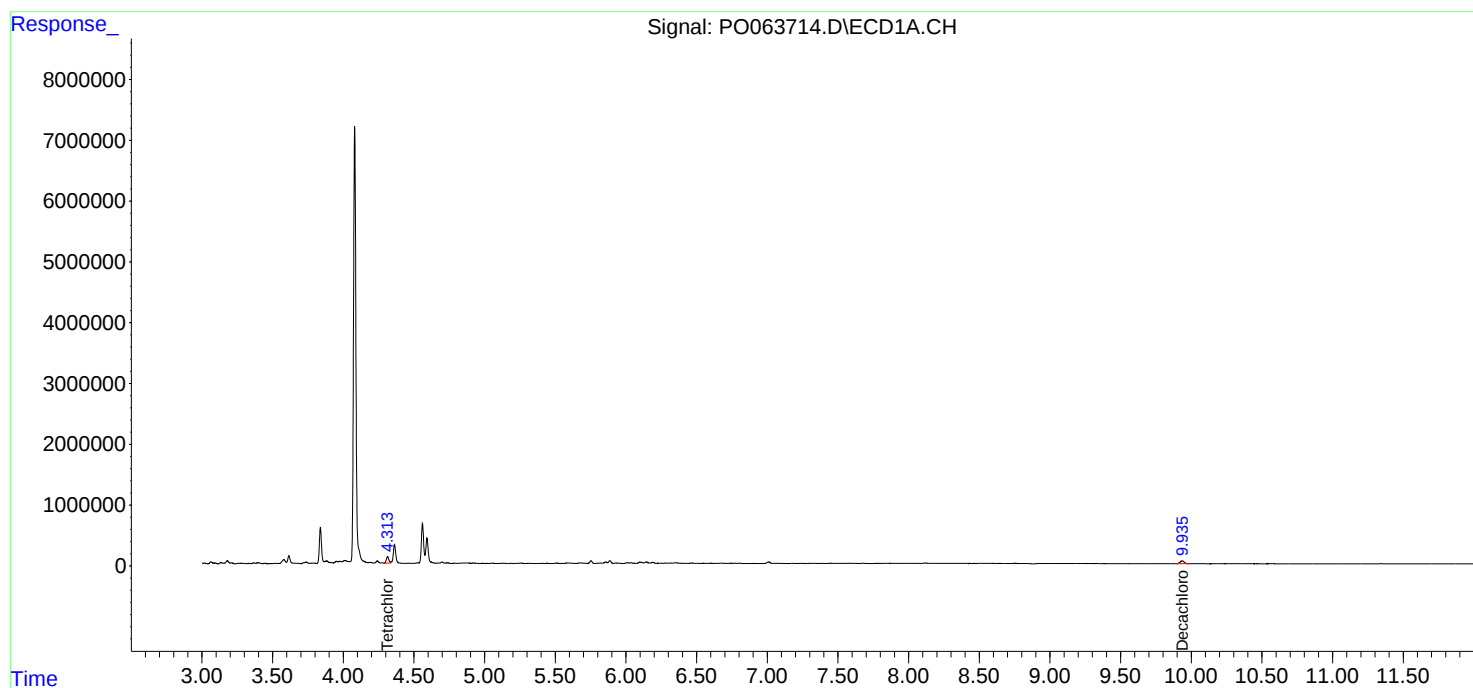

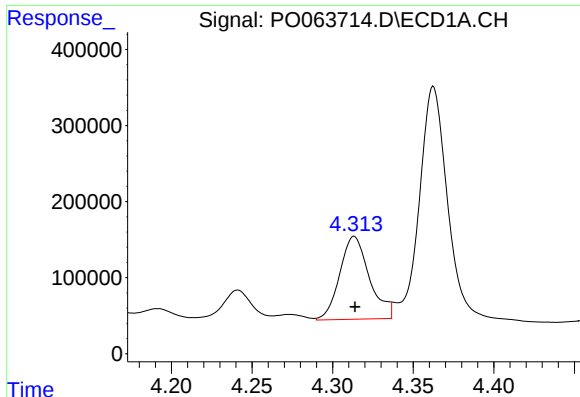


#1 Tetrachloro-m-xylene

R.T.: 4.313 min
Delta R.T.: -0.001 min
Response: 1401234
Conc: 45.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
GE-MW-58-1S


Manual Integrations
APPROVED

Ankita
11/15/2019 9:43:47 AM

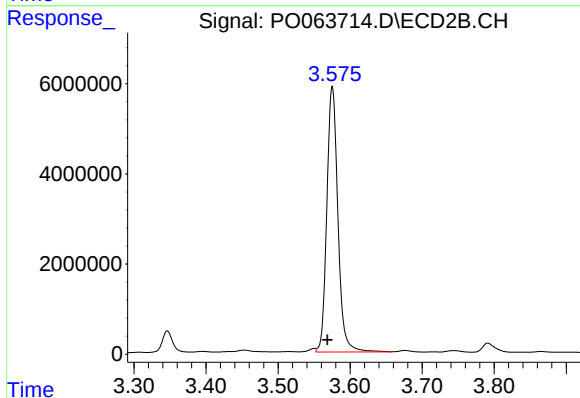


#1 Tetrachloro-m-xylene

R.T.: 3.575 min
Delta R.T.: 0.006 min
Response: 63077019
Conc: 2839.86 ng/ml m

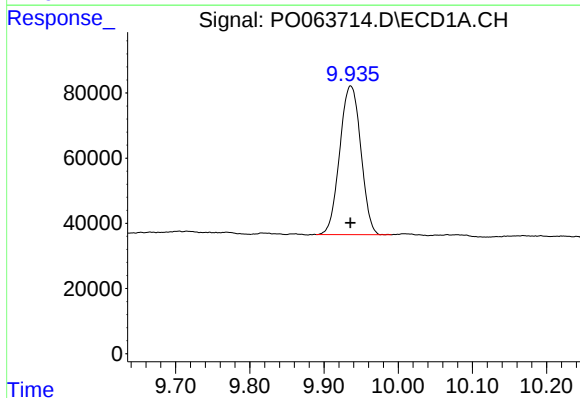

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.000 min
Response: 900109
Conc: 22.15 ng/ml

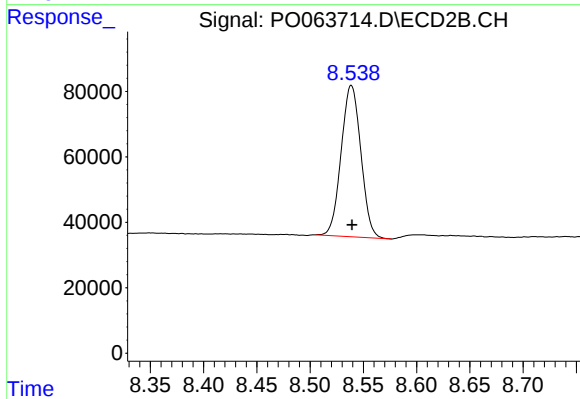

#2 Decachlorobiphenyl

R.T.: 8.539 min
Delta R.T.: 0.000 min
Response: 595037
Conc: 20.35 ng/ml