

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111422\
 Data File : PO090547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2022 14:57
 Operator : YP/AJ
 Sample : PB149022BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB149022BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/15/2022
 Supervised By :Ankita Jodhani 11/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 16:02:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 28 05:05:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.303	3.480	62870859	19728086	19.562	18.562m
2) SA Decachlor...	10.052	8.484	52000644	20593076	21.220	19.995

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111422\
Data File : PO090547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2022 14:57
Operator : YP/AJ
Sample : PB149022BL
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB149022BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2022
Supervised By :Ankita Jodhani 11/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 16:02:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102722.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 28 05:05:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

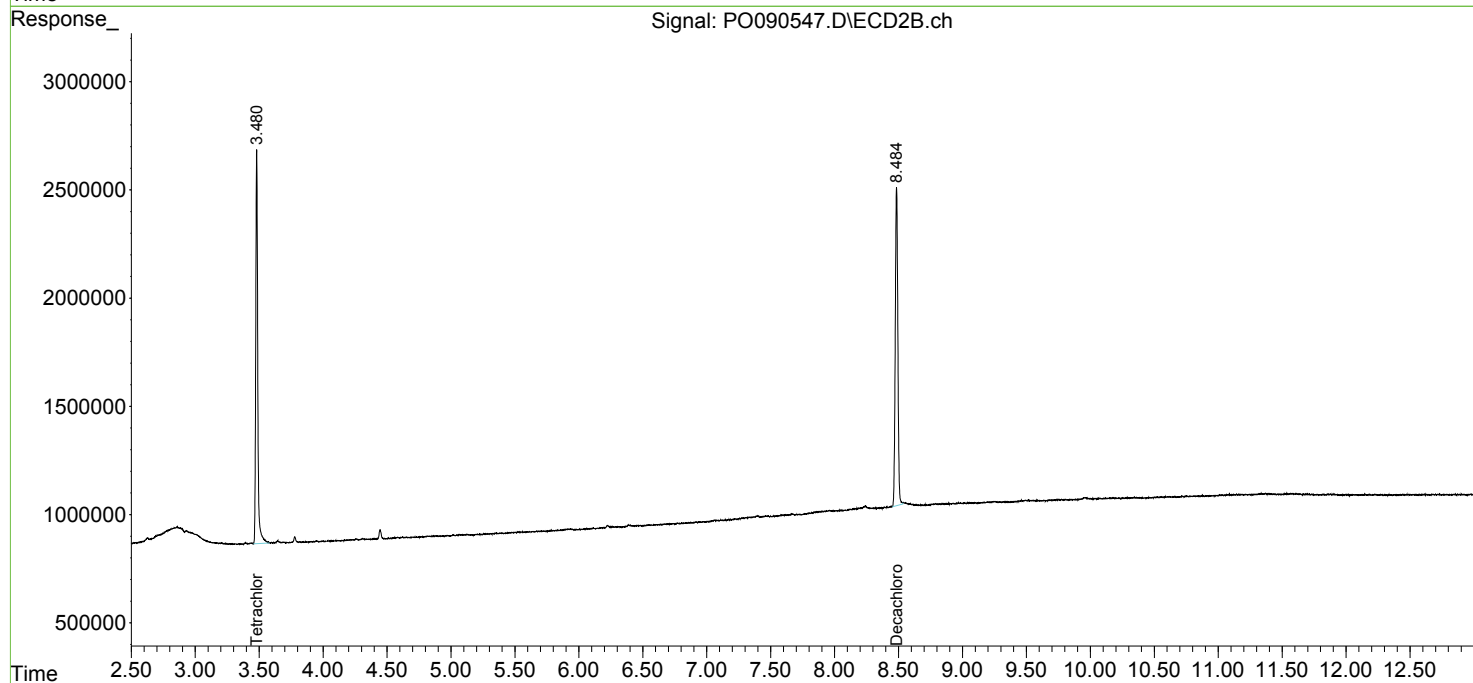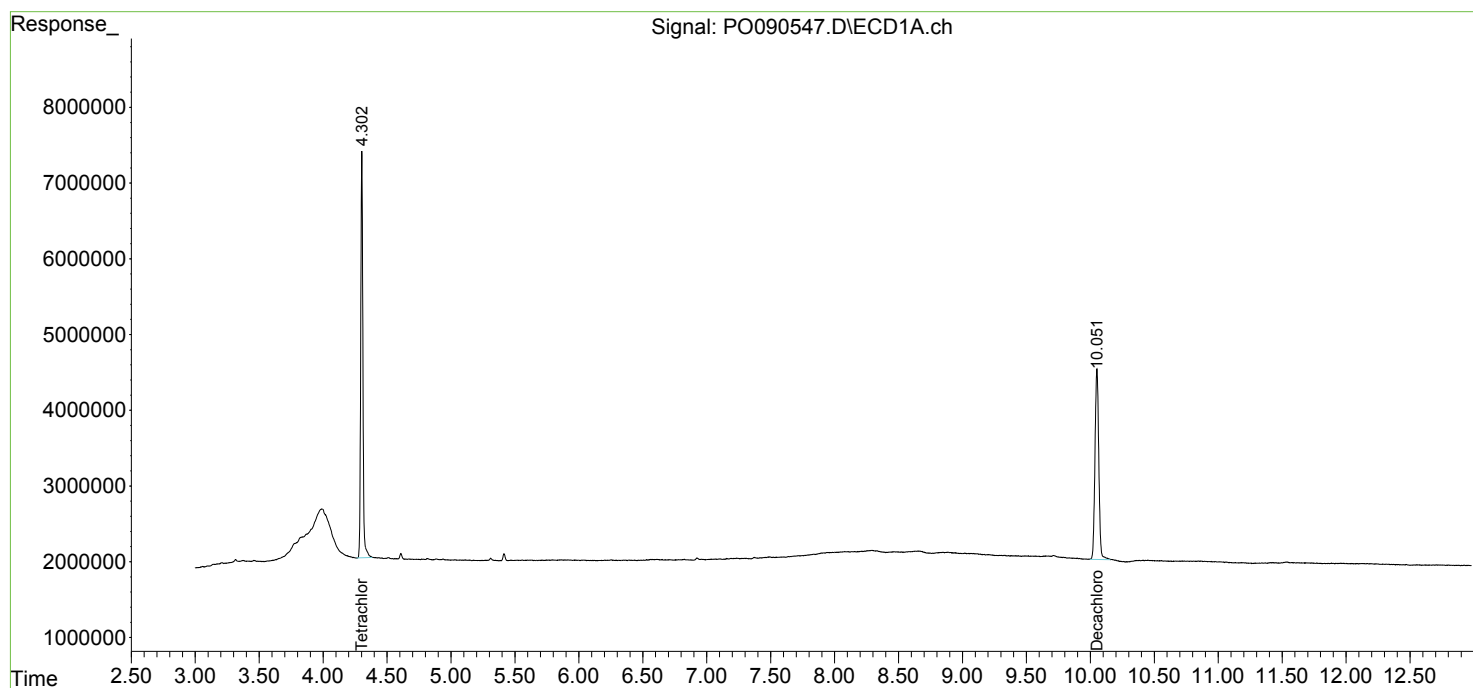

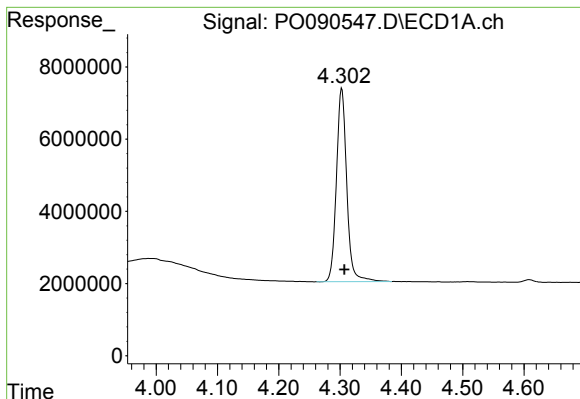


#1 Tetrachloro-m-xylene

R.T.: 4.303 min
Delta R.T.: -0.004 min
Response: 62870859
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB149022BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/15/2022
Supervised By :Ankita Jodhani 11/15/2022

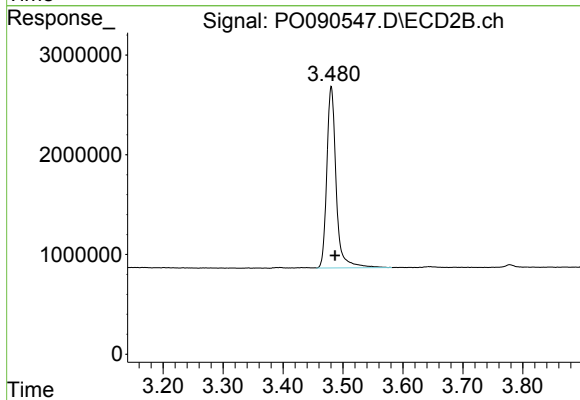


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: -0.007 min
Response: 19728086
Conc: 18.56 ng/ml m

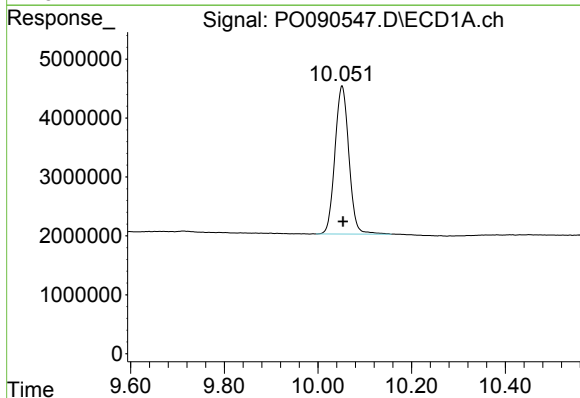

#2 Decachlorobiphenyl

R.T.: 10.052 min
Delta R.T.: -0.002 min
Response: 52000644
Conc: 21.22 ng/ml

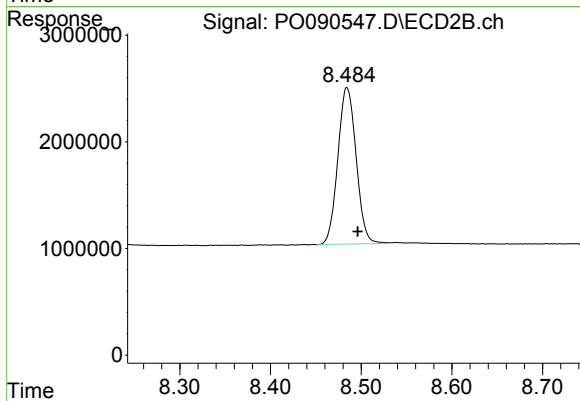

#2 Decachlorobiphenyl

R.T.: 8.484 min
Delta R.T.: -0.012 min
Response: 20593076
Conc: 19.99 ng/ml